

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101921\
 Data File : PD066420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2021 22:56
 Operator : AJ\MA
 Sample : M4204-08MS
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JDGG4MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 07:49:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.970	37881872	162.1E6	18.552	18.189
27)	SA Decachlor...	8.167	9.021	75074739	211.2E6	55.219	44.476
Target Compounds							
2)	A alpha-BHC	3.878	4.363	162.5E6	536.8E6	52.081	46.198
3)	MA gamma-BHC...	4.159	4.648	153.7E6	505.3E6	49.803	45.784
4)	MA Heptachlor	4.453	5.147	153.3E6	470.4E6	52.372	46.485
5)	MB Aldrin	4.699	5.451	152.3E6	443.6E6	49.515	43.996
6)	B beta-BHC	4.407	4.824	60733675	226.0E6	45.612	43.404
7)	B delta-BHC	4.610	5.039	151.1E6	502.9E6	52.365	51.968
8)	B Heptachlo...	5.140	5.839	141.5E6	399.0E6	52.285	49.688
9)	A Endosulfan I	5.476	6.196	130.6E6	391.1E6	51.649	46.381
10)	B trans-Chl...	5.364	6.073	144.0E6	414.4E6	52.522	45.836
11)	B cis-Chlor...	5.422	6.144	140.1E6	408.1E6	52.235	46.034
12)	B 4,4'-DDE	5.586	6.304	273.5E6	773.7E6	109.172	97.368
13)	MA Dieldrin	5.718	6.454	301.6E6	825.6E6	112.278	97.668
14)	MA Endrin	5.975	6.672	255.2E6	686.1E6	107.348	129.624
15)	B Endosulfa...	6.247	6.886	241.1E6	683.2E6	107.360	95.863
16)	A 4,4'-DDD	6.100	6.798	227.6E6	647.7E6	109.583	97.064
17)	MA 4,4'-DDT	6.338	7.095	242.2E6	667.0E6	121.694	101.698
18)	B Endrin al...	6.416	7.011	196.6E6	575.3E6	125.526	108.531
19)	B Endosulfa...	6.627	7.234	227.8E6	654.6E6	114.815	99.267
20)	A Methoxychlor	6.885	7.556	616.8E6	1535.9E6	594.815	472.932
21)	B Endrin ke...	7.119	7.706	277.4E6	732.0E6	120.138	102.055

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101921\
Data File : PD066420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2021 22:56
Operator : AJ\MA
Sample : M4204-08MS
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 07:49:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

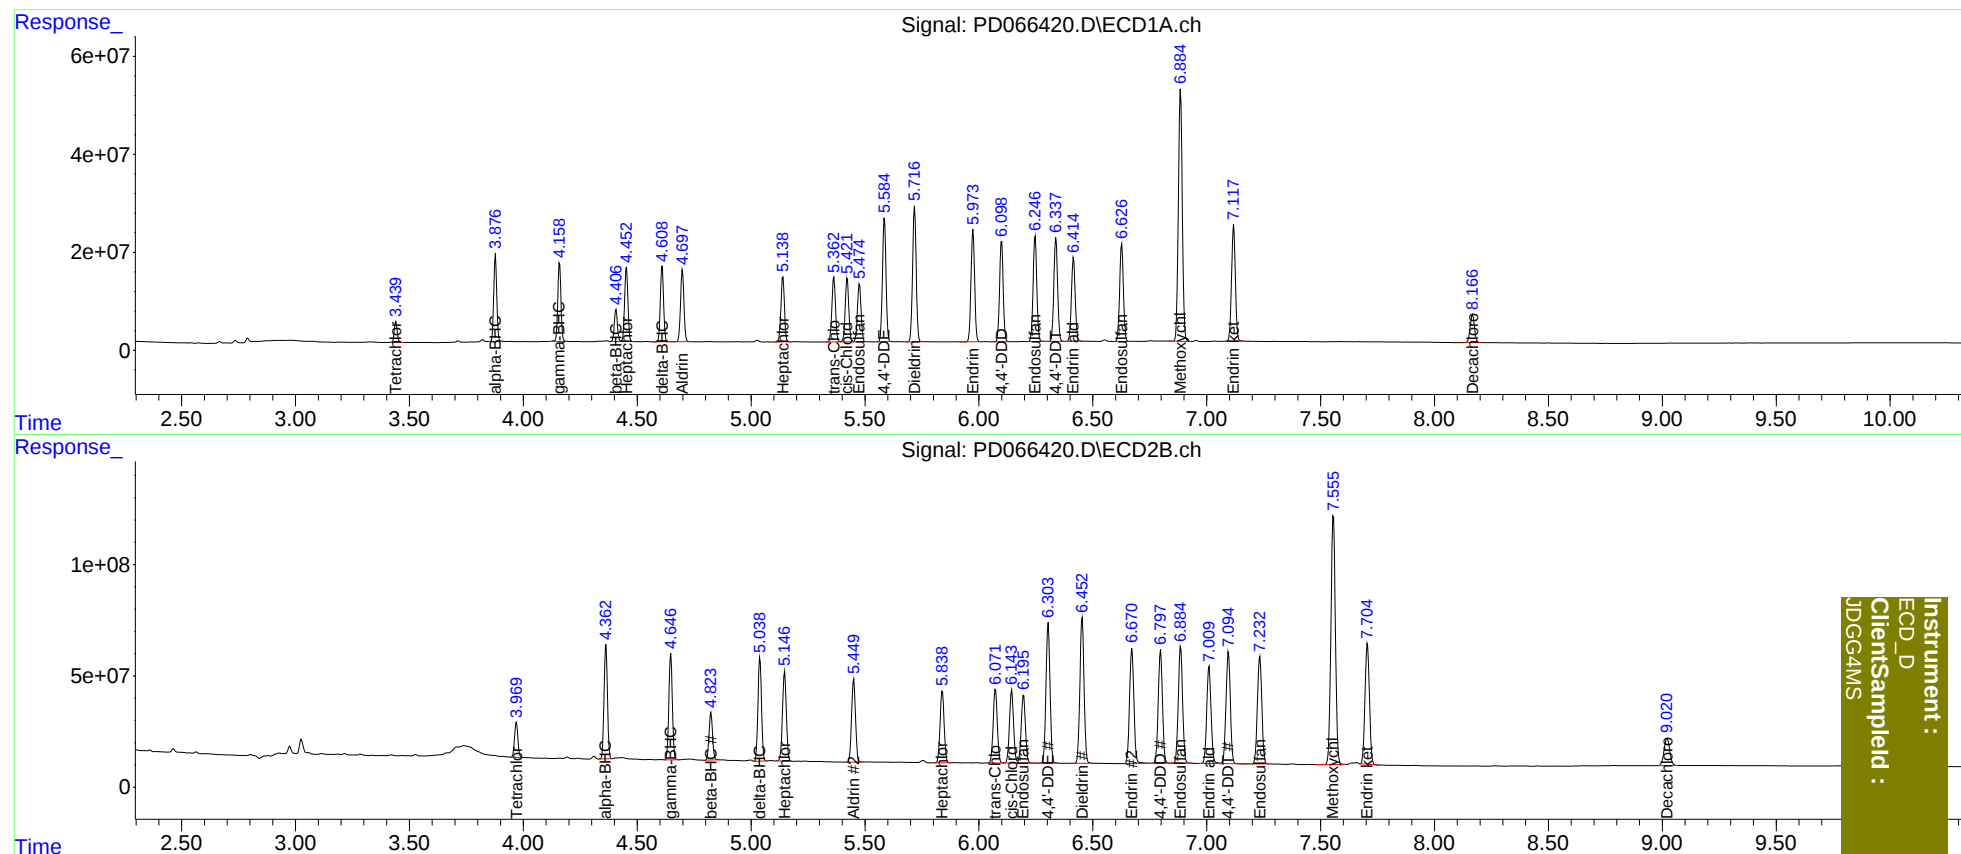

Instrument :
ECD_D
ClientSampled :
JDGG4MS