

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101921\
 Data File : PD066421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2021 23:10
 Operator : AJ\MA
 Sample : M4204-09MSD
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JDGG4MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 07:55:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	36691307	159.2E6	17.969	17.867
27)	SA Decachlor...	8.167	9.020	49346791	197.6E6	36.296	41.601
Target Compounds							
2)	A alpha-BHC	3.877	4.363	151.1E6	507.8E6	48.440	43.702
3)	MA gamma-BHC...	4.159	4.648	143.8E6	478.2E6	46.570	43.329
4)	MA Heptachlor	4.453	5.148	142.5E6	442.2E6	48.671	43.700
5)	MB Aldrin	4.699	5.451	140.2E6	417.3E6	45.597	41.384
6)	B beta-BHC	4.407	4.824	57150359	211.1E6	42.921	40.535
7)	B delta-BHC	4.610	5.039	140.2E6	464.0E6	48.580	47.949
8)	B Heptachlo...	5.140	5.839	131.6E6	364.3E6	48.635	45.367
9)	A Endosulfan I	5.476	6.196	121.2E6	367.4E6	47.939	43.570
10)	B trans-Chl...	5.364	6.073	133.7E6	389.6E6	48.788	43.095
11)	B cis-Chlor...	5.421	6.144	130.2E6	383.4E6	48.529	43.252
12)	B 4,4'-DDE	5.585	6.304	256.4E6	727.6E6	102.348	91.564
13)	MA Dieldrin	5.718	6.454	281.0E6	773.4E6	104.604	91.498
14)	MA Endrin	5.975	6.672	237.4E6	639.7E6	99.848	120.867
15)	B Endosulfa...	6.247	6.886	228.9E6	640.4E6	101.892	89.867
16)	A 4,4'-DDD	6.100	6.798	214.7E6	608.9E6	103.411	91.262
17)	MA 4,4'-DDT	6.339	7.095	229.3E6	629.9E6	115.207	96.051
18)	B Endrin al...	6.416	7.011	182.5E6	531.4E6	116.507	100.244
19)	B Endosulfa...	6.627	7.233	215.0E6	613.4E6	108.333	93.018
20)	A Methoxychlor	6.886	7.556	514.9E6	1439.7E6	496.541	443.311
21)	B Endrin ke...	7.119	7.706	225.7E6	684.9E6	97.743	95.491

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101921\
Data File : PD066421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2021 23:10
Operator : AJ\MA
Sample : M4204-09MSD
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 07:55:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

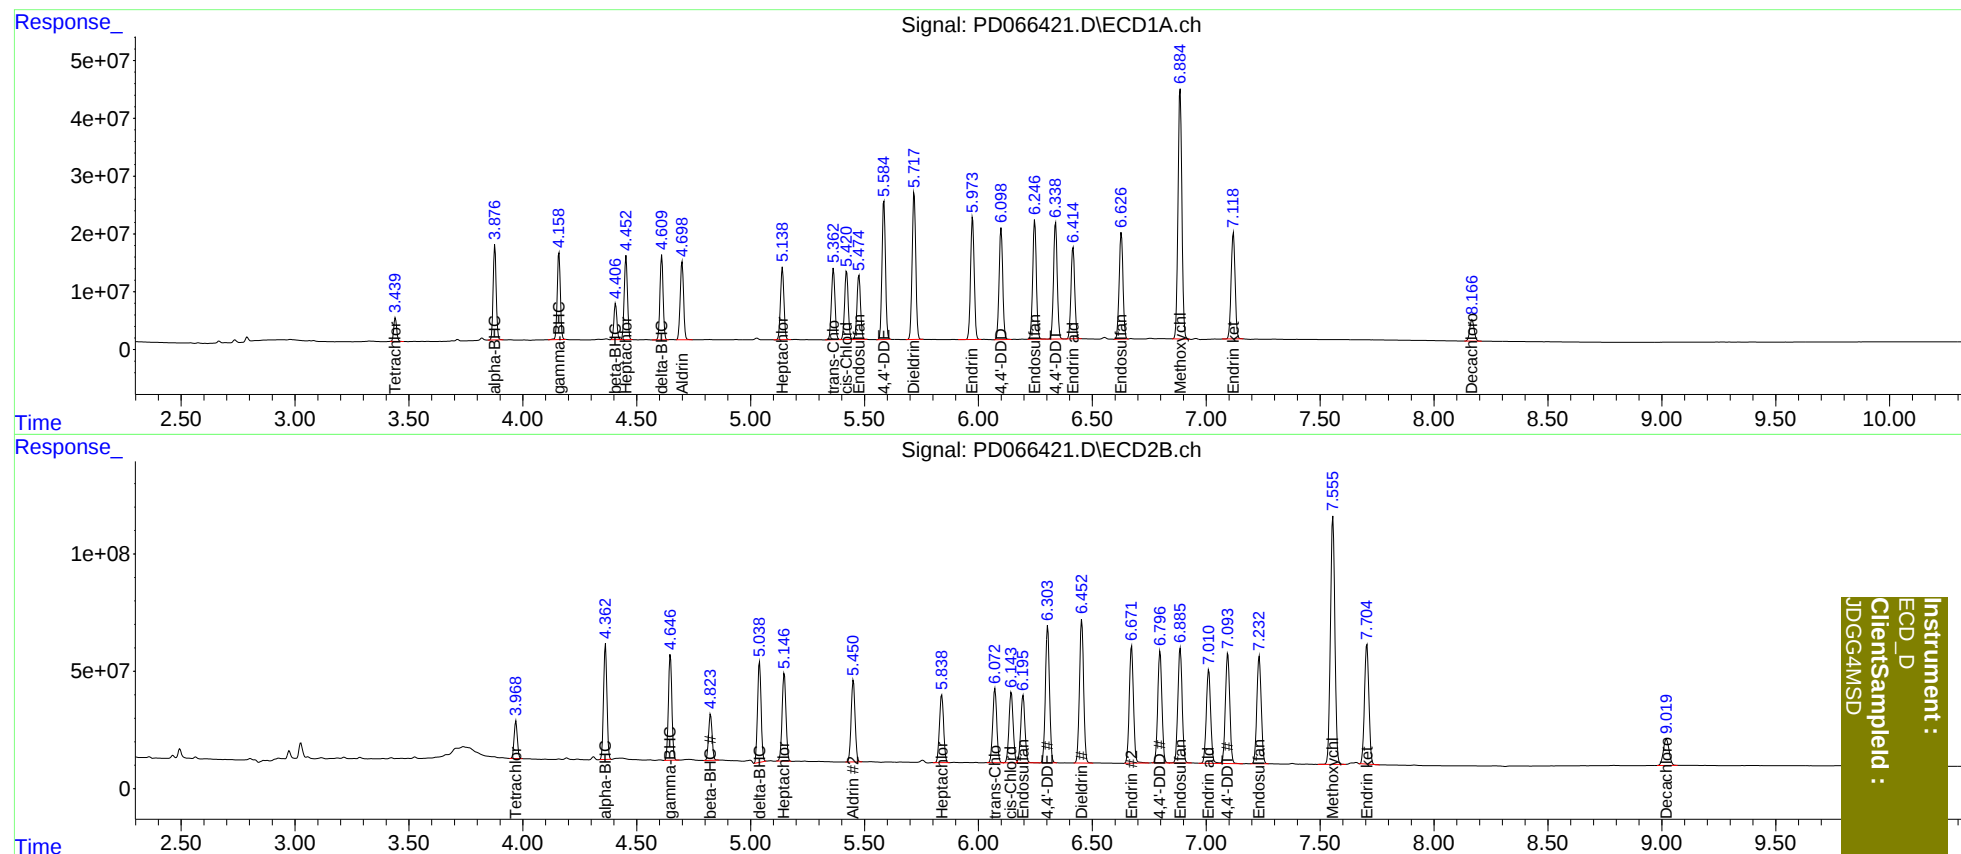

Instrument :
ECD_D
ClientSampleId :
JDGG4MSD