

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101921\
 Data File : PD066426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2021 00:19
 Operator : AJ\MA
 Sample : M4218-02MS
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JDGE9MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 08:22:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	30186189	137.2E6	14.783	15.393
27)	SA Decachlor...	8.166	9.020	41268524	167.9E6	30.354	35.358
Target Compounds							
2)	A alpha-BHC	3.877	4.363	142.1E6	478.1E6	45.544	41.146
3)	MA gamma-BHC...	4.159	4.647	135.5E6	453.2E6	43.883	41.062
4)	MA Heptachlor	4.453	5.147	138.1E6	428.0E6	47.164	42.292
5)	MB Aldrin	4.699	5.451	122.0E6	407.2E6	39.675	40.385
6)	B beta-BHC	4.407	4.824	54883689	201.4E6	41.218	38.675
7)	B delta-BHC	4.610	5.039	132.6E6	429.2E6	45.963	44.350
8)	B Heptachlo...	5.139	5.839	122.7E6	325.8E6	45.328	40.571
9)	A Endosulfan I	5.475	6.196	112.4E6	352.8E6	44.444	41.832
10)	B trans-Chl...	5.363	6.073	124.7E6	370.4E6	45.480	40.970
11)	B cis-Chlor...	5.421	6.144	121.4E6	369.6E6	45.276	41.693
12)	B 4,4'-DDE	5.585	6.304	245.5E6	698.6E6	98.030	87.917
13)	MA Dieldrin	5.717	6.454	265.5E6	729.3E6	98.835	86.275
14)	MA Endrin	5.975	6.673	225.4E6	603.4E6	94.804	114.003
15)	B Endosulfa...	6.247	6.886	212.0E6	596.6E6	94.403	83.718
16)	A 4,4'-DDD	6.100	6.798	200.5E6	578.8E6	96.569	86.749
17)	MA 4,4'-DDT	6.338	7.095	218.0E6	605.2E6	109.538	92.274
18)	B Endrin al...	6.416	7.011	166.4E6	494.9E6	106.248	93.358
19)	B Endosulfa...	6.628	7.233	200.8E6	573.6E6	101.194	86.988
20)	A Methoxychlor	6.885	7.556	491.7E6	1353.7E6	474.184	416.807
21)	B Endrin ke...	7.119	7.706	205.9E6	650.5E6	89.155	90.702

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101921\
Data File : PD066426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2021 00:19
Operator : AJ\MA
Sample : M4218-02MS
Misc :
ALS Vial : 42 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 08:22:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

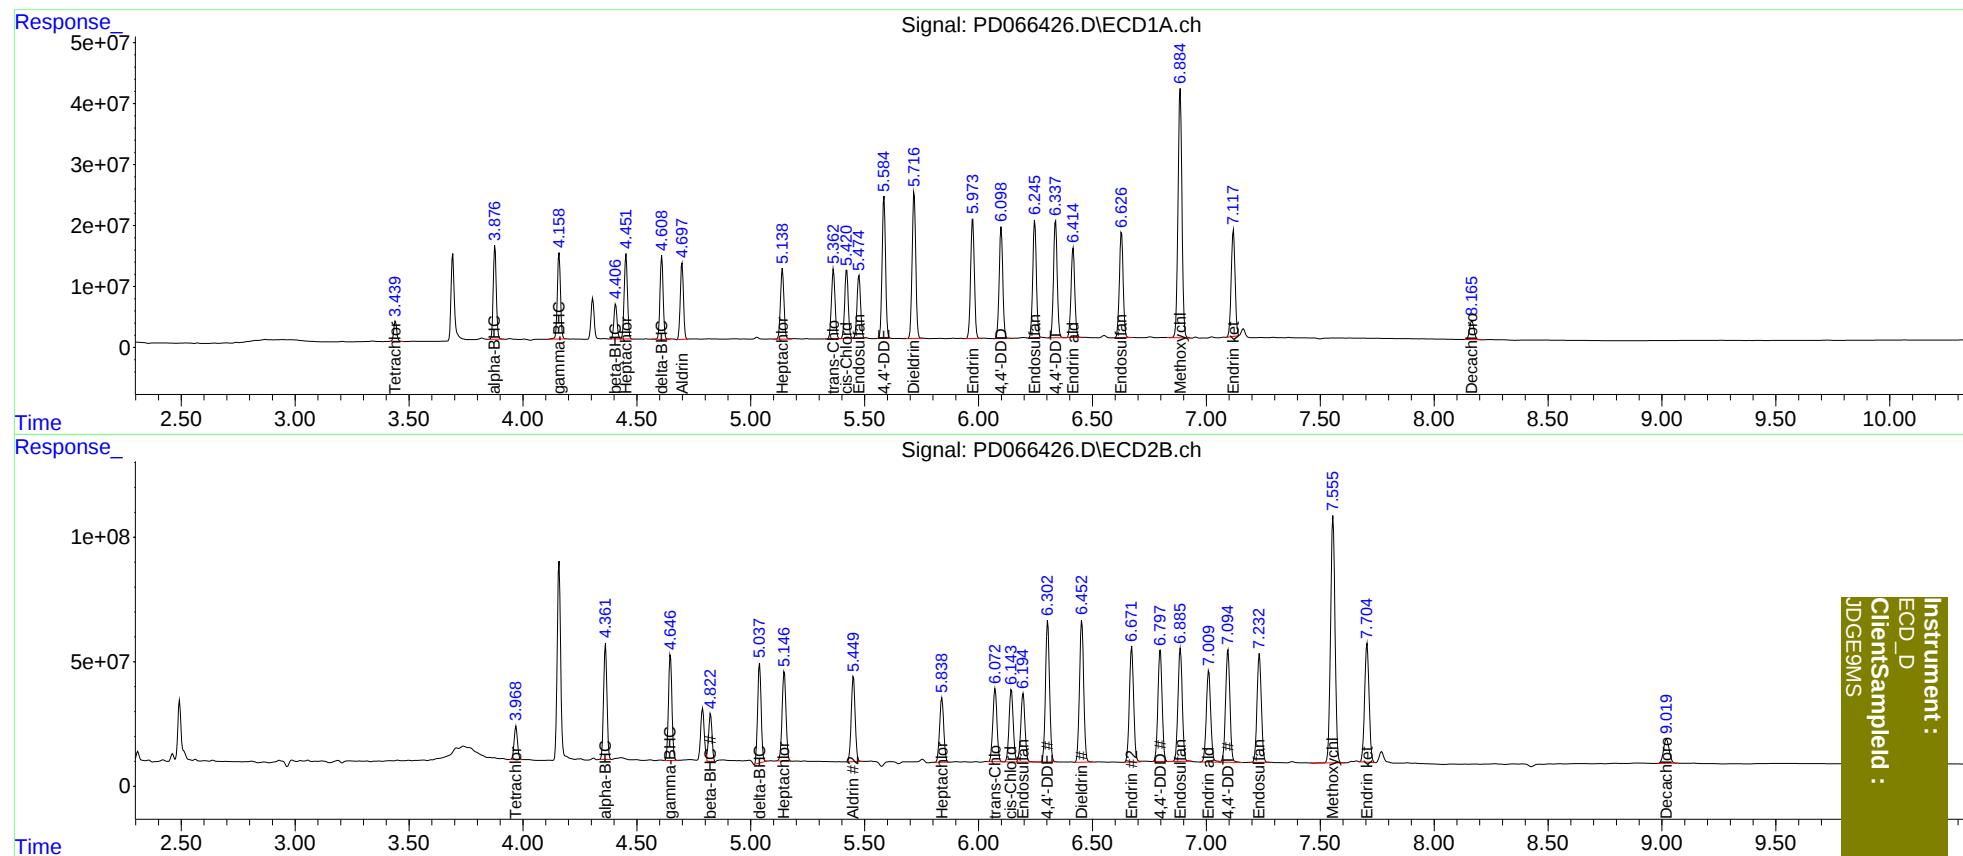

Instrument :
ECD_D
ClientSampled :
JDGE9MS