

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101921\
 Data File : PD066427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2021 00:32
 Operator : AJ\MA
 Sample : M4218-03MSD
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JDGE9MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 06:31:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	31091566	140.2E6	15.227	15.737
27)	SA Decachlor...	8.167	9.020	42560551	174.9E6	31.304	36.836
Target Compounds							
2)	A alpha-BHC	3.877	4.363	139.1E6	470.1E6	44.573	40.463
3)	MA gamma-BHC...	4.159	4.648	133.0E6	446.9E6	43.071	40.491
4)	MA Heptachlor	4.453	5.147	134.2E6	420.8E6	45.853	41.583
5)	MB Aldrin	4.699	5.451	119.2E6	403.9E6	38.759	40.054
6)	B beta-BHC	4.407	4.824	53490128	200.1E6	40.172	38.436
7)	B delta-BHC	4.609	5.039	131.4E6	426.7E6	45.532	44.093
8)	B Heptachlo...	5.139	5.839	120.5E6	316.3E6	44.532	39.387
9)	A Endosulfan I	5.476	6.196	108.9E6	351.4E6	43.091	41.670
10)	B trans-Chl...	5.363	6.073	122.1E6	365.1E6	44.549	40.381
11)	B cis-Chlor...	5.422	6.144	118.5E6	367.1E6	44.200	41.412
12)	B 4,4'-DDE	5.586	6.304	240.6E6	697.9E6	96.065	87.829
13)	MA Dieldrin	5.717	6.454	258.6E6	729.4E6	96.289	86.288
14)	MA Endrin	5.974	6.672	222.7E6	604.1E6	93.667	114.134
15)	B Endosulfa...	6.247	6.886	206.4E6	591.6E6	91.886	83.009
16)	A 4,4'-DDD	6.101	6.798	196.7E6	570.2E6	94.748	85.459
17)	MA 4,4'-DDT	6.339	7.096	210.5E6	597.4E6	105.774	91.084
18)	B Endrin al...	6.415	7.010	163.6E6	492.9E6	104.431	92.990
19)	B Endosulfa...	6.628	7.234	197.5E6	570.3E6	99.556	86.475
20)	A Methoxychlor	6.886	7.556	547.3E6	1352.1E6	527.840	416.333
21)	B Endrin ke...	7.119	7.705	200.2E6	628.5E6	86.675	87.623

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101921\
Data File : PD066427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2021 00:32
Operator : AJ\MA
Sample : M4218-03MSD
Misc :
ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 06:31:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

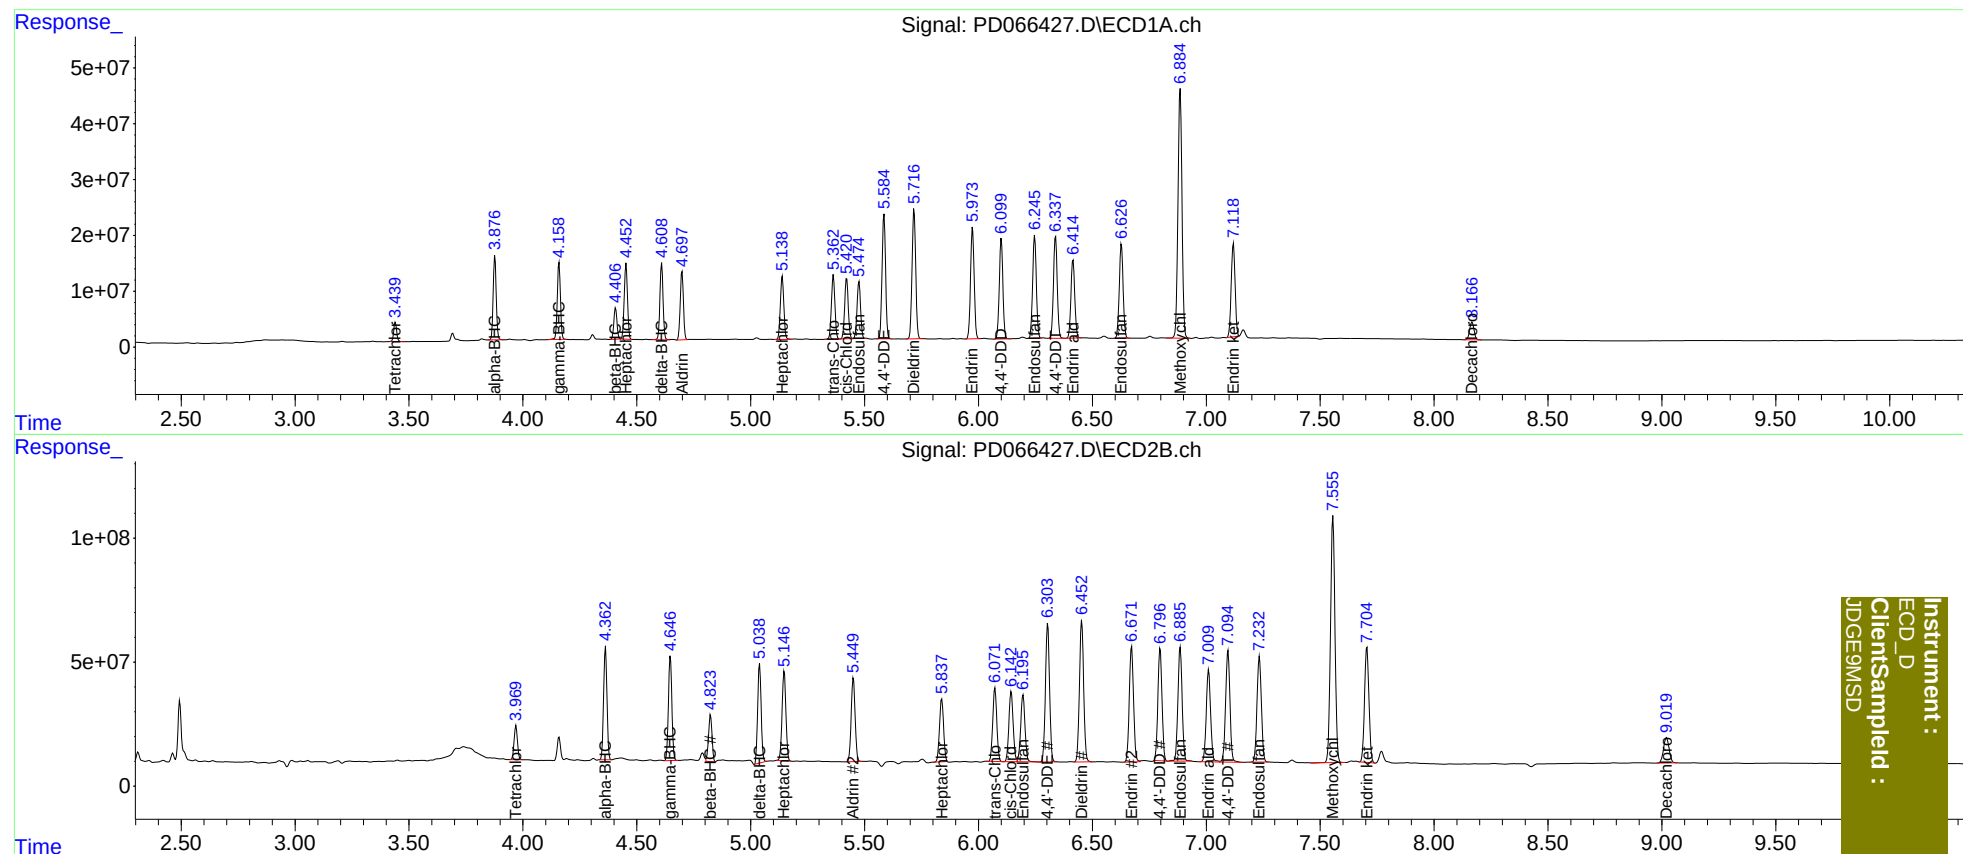

Instrument :
ECD_D
ClientSampled :
JDGE9MSD