

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101921\
 Data File : PD066428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2021 00:46
 Operator : AJ\MA
 Sample : M4218-04
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JDGF1

Manual Integrations
 APPROVED

mohammad
 10/20/2021 1:26:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 08:26:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.970	26725585	122.0E6	13.089	13.685
27)	SA Decachlor...	8.166	9.020	36521127	151.4E6	26.862	31.881
Target Compounds							
2)	A alpha-BHC	3.876	4.365	1871476	1013984	0.600	<MDL #
3)	MA gamma-BHC...	4.159	4.646	2941453	2287669	0.953	0.207 #
4)	MA Heptachlor	4.451	5.147	598922	2614901	0.205	0.258m#
5)	MB Aldrin	4.698	5.450	426846	1153098	0.139	0.114
6)	B beta-BHC	4.409	4.822	1179745	8443084	0.886	1.622 #
9)	A Endosulfan I	5.480	6.196	1118447	1692282	0.442	0.201 #
10)	B trans-Chl...	5.363	6.074	515541	1321318	0.188	0.146
11)	B cis-Chlor...	5.420	6.143	944049	5578922	0.352	0.629 #
12)	B 4,4'-DDE	5.586	6.304	1074035	4108680	0.429	0.517
13)	MA Dieldrin	5.717	6.455	1101880	4380194	0.410	0.518 #
14)	MA Endrin	5.970	6.673	1622841	2182943	0.683	0.412 #
15)	B Endosulfa...	6.247	6.887	1173417	5291509	0.522	0.743 #
16)	A 4,4'-DDD	6.099	6.798	905098	3965273	0.436	0.594 #
17)	MA 4,4'-DDT	6.337	7.090	812857	7014267	0.408	1.070m#
18)	B Endrin al...	6.415	7.011	1270274	7318648	0.811	1.381 #
19)	B Endosulfa...	6.626	7.234	1508098	4772652	0.760	0.724
20)	A Methoxychlor	6.885	7.555	2693972	11197788	2.598	3.448 #
21)	B Endrin ke...	7.119	7.696	2253788	4049123	0.976	0.565m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101921\
Data File : PD066428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2021 00:46
Operator : AJ\MA
Sample : M4218-04
Misc :
ALS Vial : 44 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 08:26:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

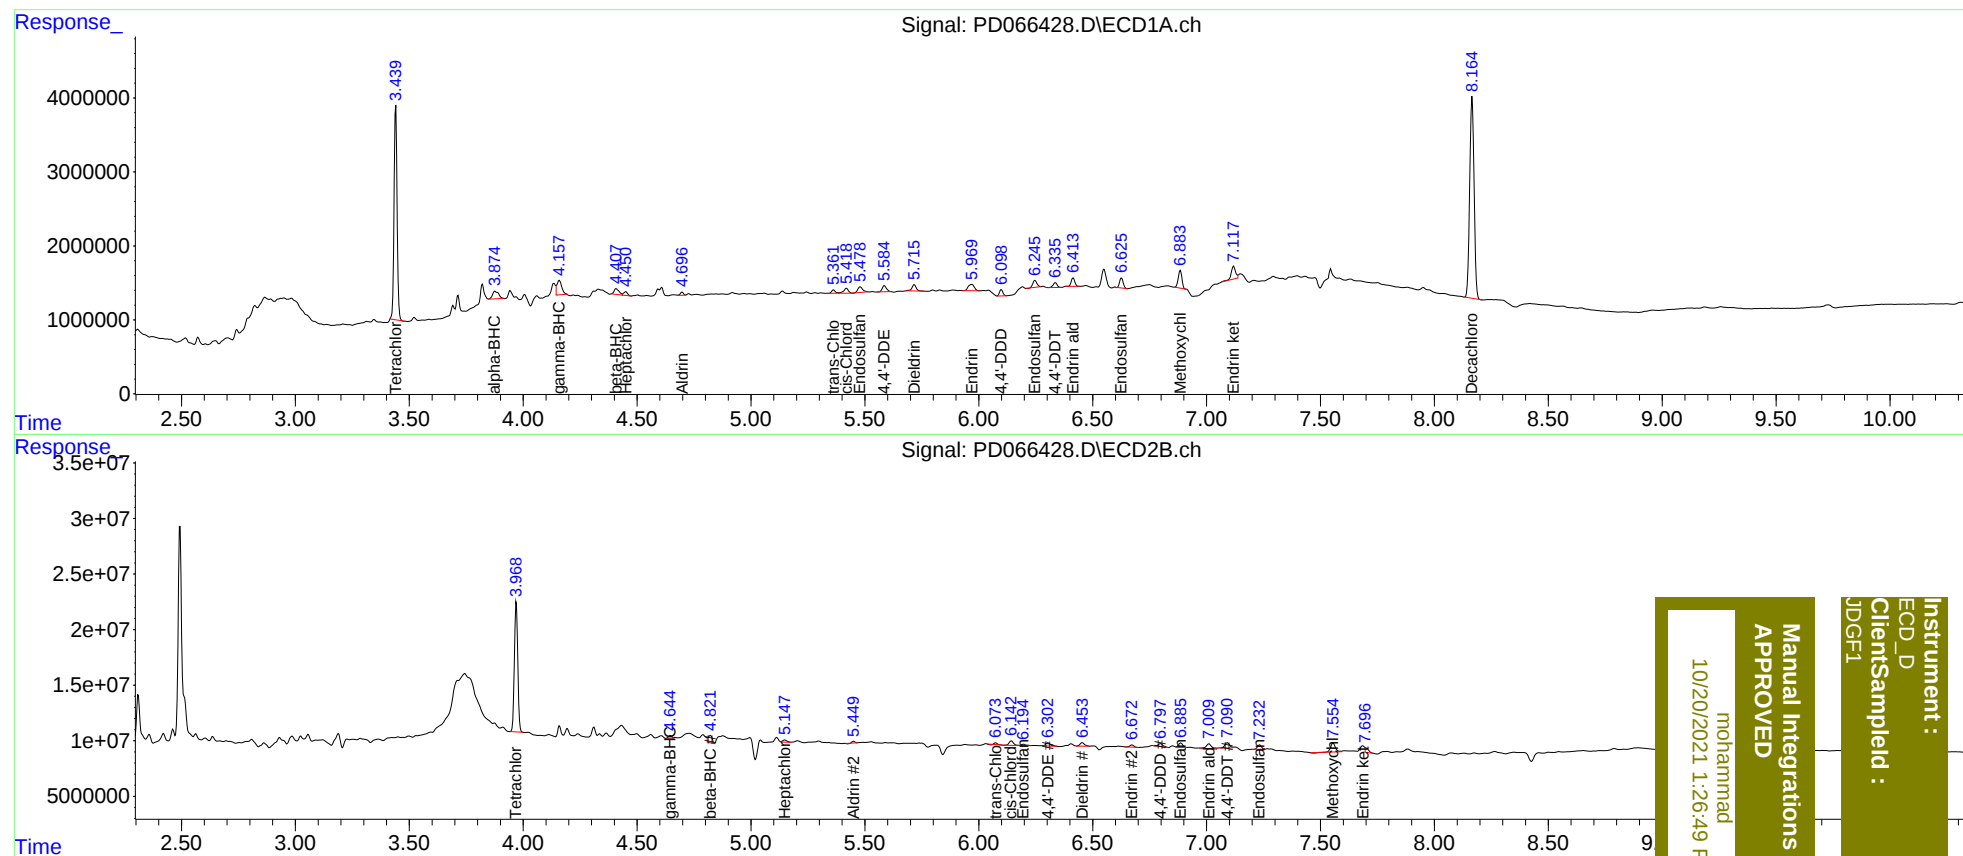

Manual Integrations
APPROVED

mohammad
10/20/2021 1:26:49 PM

Instrument :
ECD_D
Client Sampled :
JDGF1