

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101921\
 Data File : PD066431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2021 01:28
 Operator : AJ\MA
 Sample : INDA321
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3184

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 06:32:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.970	34673809	154.6E6	16.981	17.344
27)	SA Decachlor...	8.167	9.021	48383661	193.5E6	35.587	40.751
Target Compounds							
2)	A alpha-BHC	3.878	4.363	52233778	197.1E6	16.742	16.963
3)	MA gamma-BHC...	4.159	4.648	52549655	185.3E6	17.023	16.784
4)	MA Heptachlor	4.453	5.147	50872895	175.2E6	17.378	17.312
9)	A Endosulfan I	5.475	6.196	43575927	145.4E6	17.237	17.237
13)	MA Dieldrin	5.718	6.454	97152742	296.0E6	36.172	35.019
14)	MA Endrin	5.974	6.672	81582039	240.9E6	34.317	45.517 #
16)	A 4,4'-DDD	6.100	6.798	75440758	234.3E6	36.330	35.110
17)	MA 4,4'-DDT	6.339	7.095	76973607	232.9E6	38.682	35.505
20)	A Methoxychlor	6.885	7.557	187.3E6	569.6E6	180.594	175.394

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101921\
Data File : PD066431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2021 01:28
Operator : AJ\MA
Sample : INDA321
Misc :
ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 06:32:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

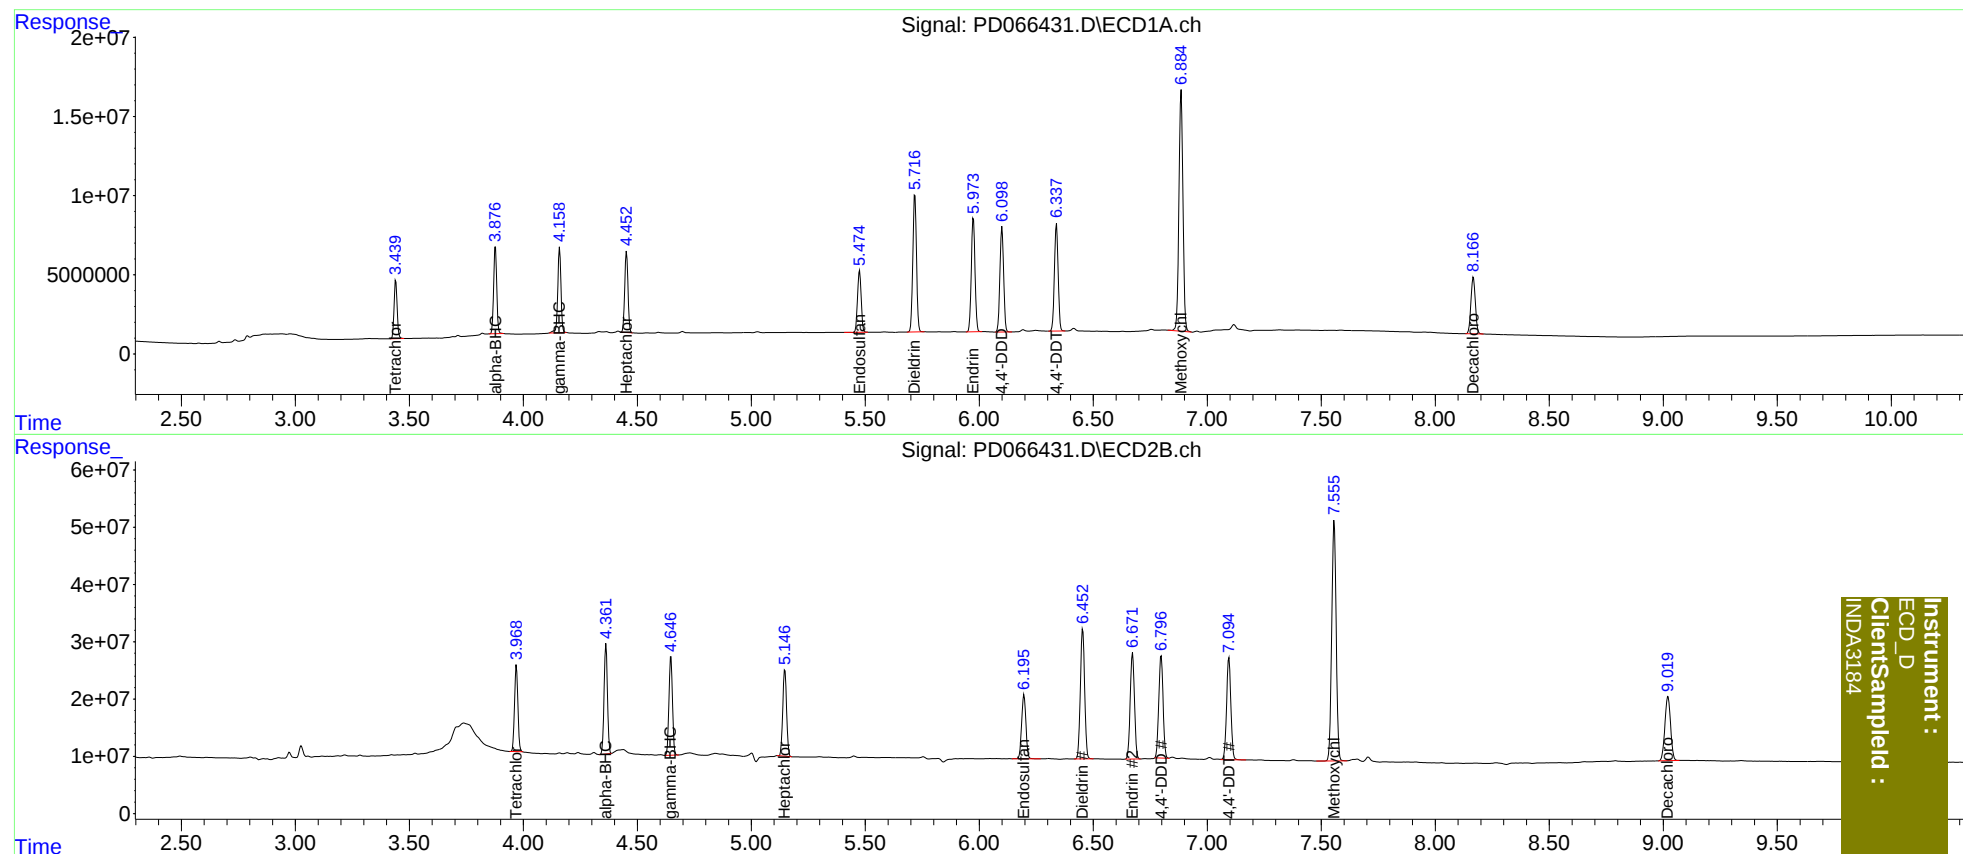

Instrument :
ECD_D
ClientSampled :
INDA3184