

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101924\
 Data File : PD086124.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2024 13:32
 Operator : AR\AJ
 Sample : P4361-09MS
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAZ0MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/21/2024
 Supervised By :Ankita Jodhani 10/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 01:39:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 09 17:21:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	2.877	8445374	48598622	7.383m	7.826
2)	SA Decachlor...	8.895	8.055	12529503	35993956	6.497	7.401
Target Compounds							
2)	A alpha-BHC	3.884	3.386	112.7E6	435.8E6	56.211m	47.220
3)	MA gamma-BHC...	4.213	3.720	110.5E6	412.4E6	55.407	47.858
4)	MA Heptachlor	4.805	4.072	109.4E6	403.9E6	56.765	54.930
5)	MB Aldrin	5.144	4.357	110.1E6	397.1E6	45.748	41.067
6)	B beta-BHC	4.399	4.015	43837548	179.6E6	41.608	39.820
7)	B delta-BHC	4.644	4.251	105.2E6	396.4E6	47.826	42.783
8)	B Heptachlo...	5.563	4.860	97935037	353.3E6	43.972	40.556
9)	A Endosulfan I	5.944	5.234	95417627	312.6E6	52.302	45.092
10)	B trans-Chl...	5.817	5.112	98498801	367.3E6	43.826	40.832
11)	B cis-Chlor...	5.898	5.176	101.4E6	360.3E6	44.469	40.136
12)	B 4,4'-DDE	6.070	5.360	186.5E6	655.2E6	97.822	87.172
13)	MA Dieldrin	6.216	5.498	212.3E6	698.4E6	107.879	94.352m
14)	MA Endrin	6.441	5.775	181.0E6	609.3E6	117.139	103.309
15)	B Endosulfa...	6.654	6.067	174.2E6	577.1E6	87.750	82.522
16)	A 4,4'-DDD	6.578	5.915	150.1E6	522.8E6	120.335	109.564
17)	MA 4,4'-DDT	6.892	6.169	153.4E6	541.3E6	113.691	108.685
18)	B Endrin al...	6.783	6.246	130.6E6	416.4E6	85.174	80.375
19)	B Endosulfa...	7.017	6.470	169.6E6	525.8E6	92.634	86.803
20)	A Methoxychlor	7.365	6.740	432.8E6	1172.4E6	541.346	559.272
21)	B Endrin ke...	7.494	6.979	185.2E6	596.9E6	91.117	81.961

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101924\
Data File : PD086124.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2024 13:32
Operator : AR\AJ
Sample : P4361-09MS
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 01:39:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

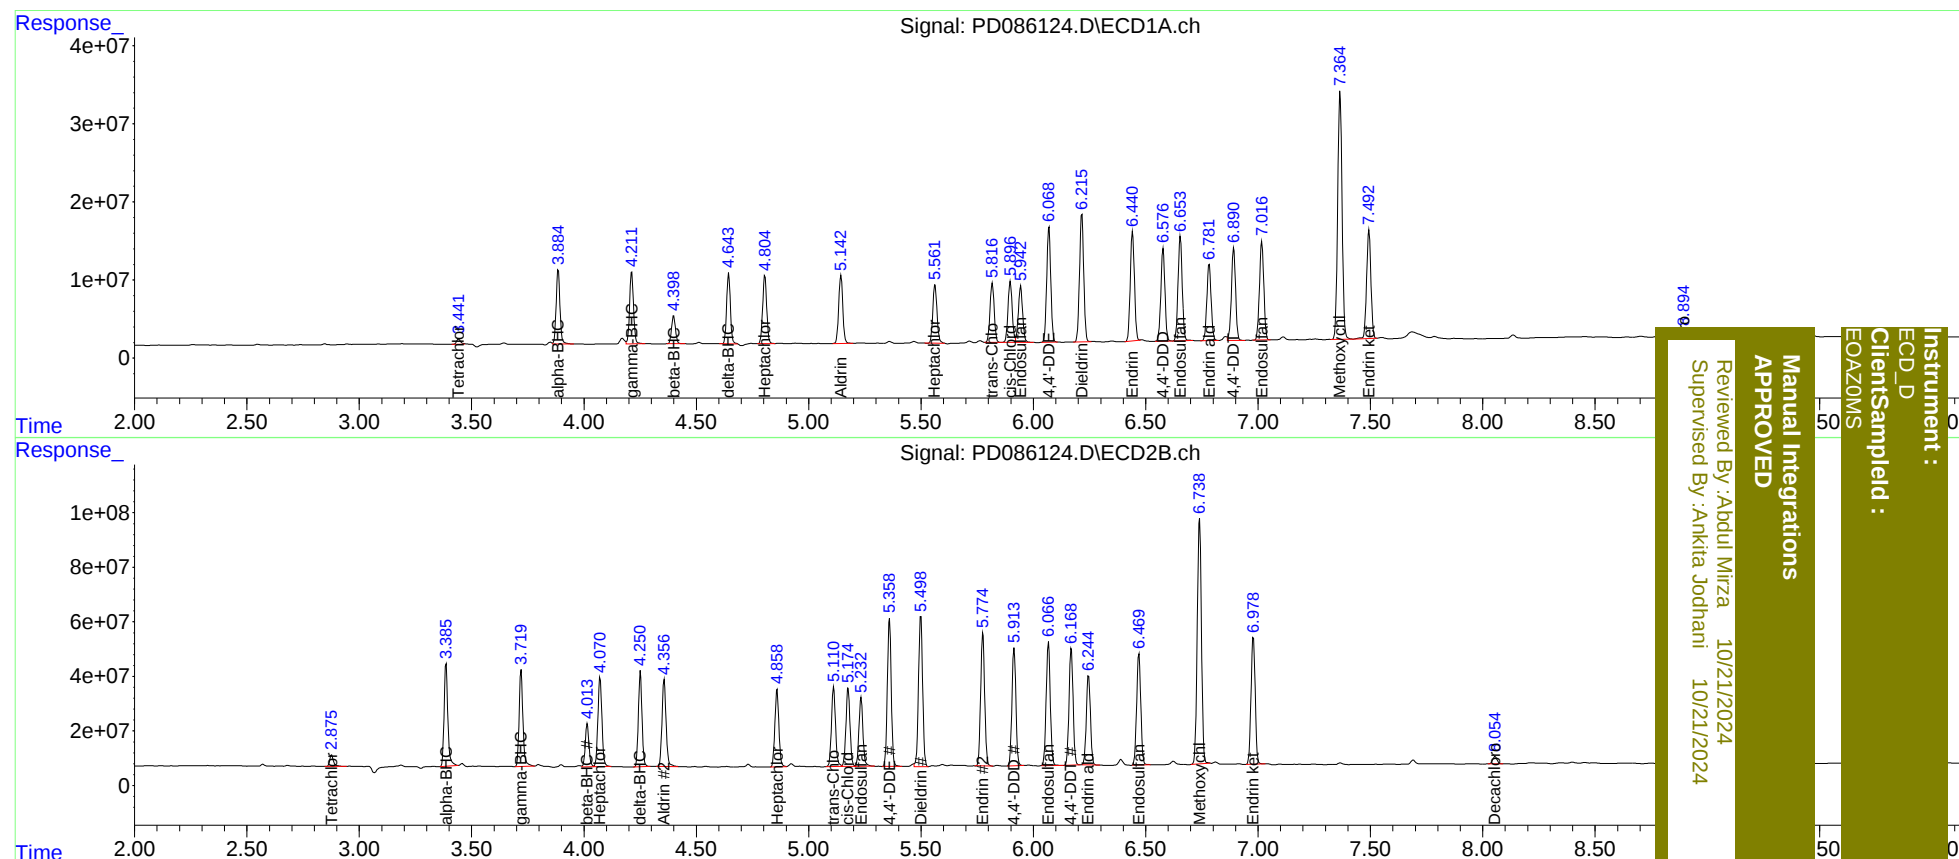

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/21/2024
Supervised By: Ankita Jodhani 10/21/2024

Instrument :
ECD_D
Client Sampled :
EOAZOMS