

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102020\
 Data File : PD059853.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2020 14:20
 Operator : DD\AJ
 Sample : L4214-07
 Misc : CHLOR LOD 25 PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 08:15:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:13:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.024	31370330	50966568	21.127	20.765
28)	SA Decachlor...	8.306	9.108	36827438	41214525	23.819	22.759
Target Compounds							
23)	Chlordane-1	4.389	5.023	2125248	2464436	34.573	25.767 #
24)	Chlordane-2	4.896	5.490	1775976	3824838	28.853	38.813 #
25)	Chlordane-3	5.471	6.139	5002787	9547822	26.533	25.306
26)	Chlordane-4	5.529	6.214	4124263	12554803	27.006	28.104
27)	Chlordane-5	6.373	7.020	2146036	2750938	29.655	33.406



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102020\
Data File : PD059853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2020 14:20
Operator : DD\AJ
Sample : L4214-07
Misc : CHLOR LOD 25 PPB
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 08:15:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:13:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

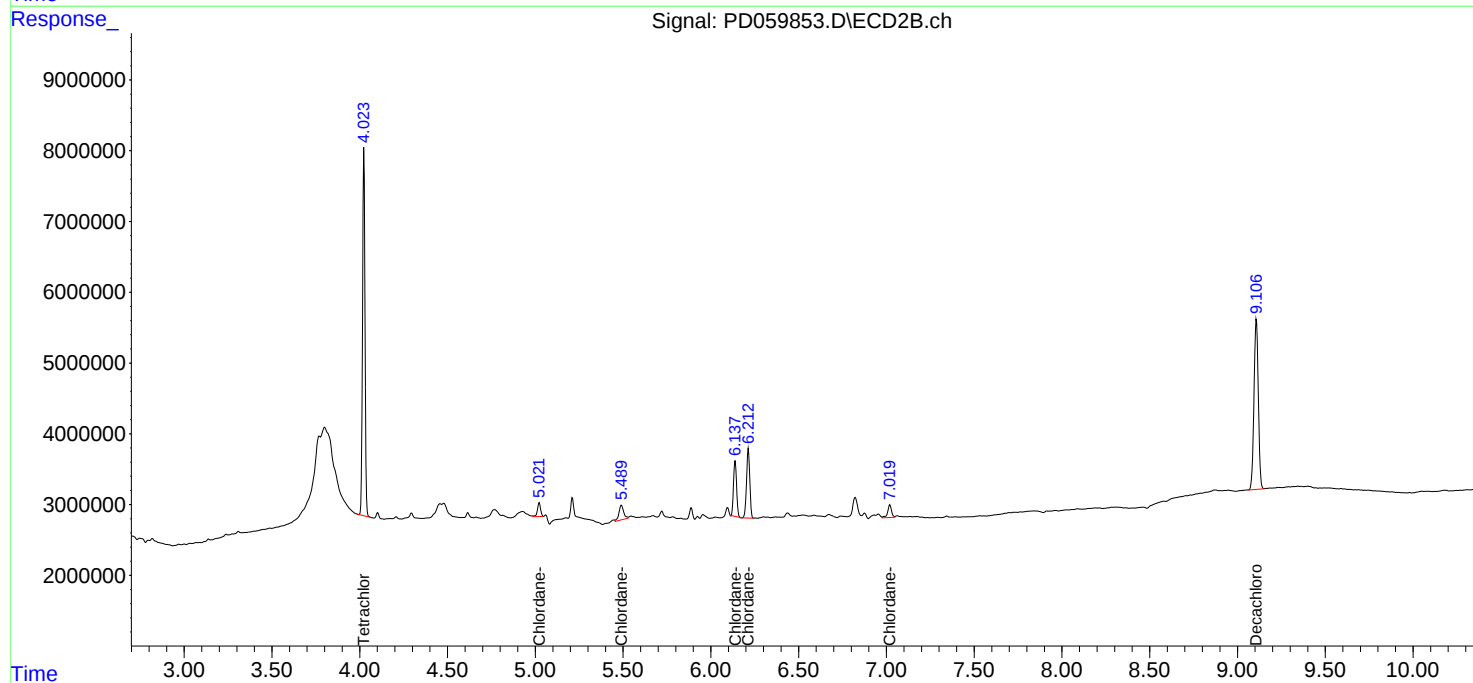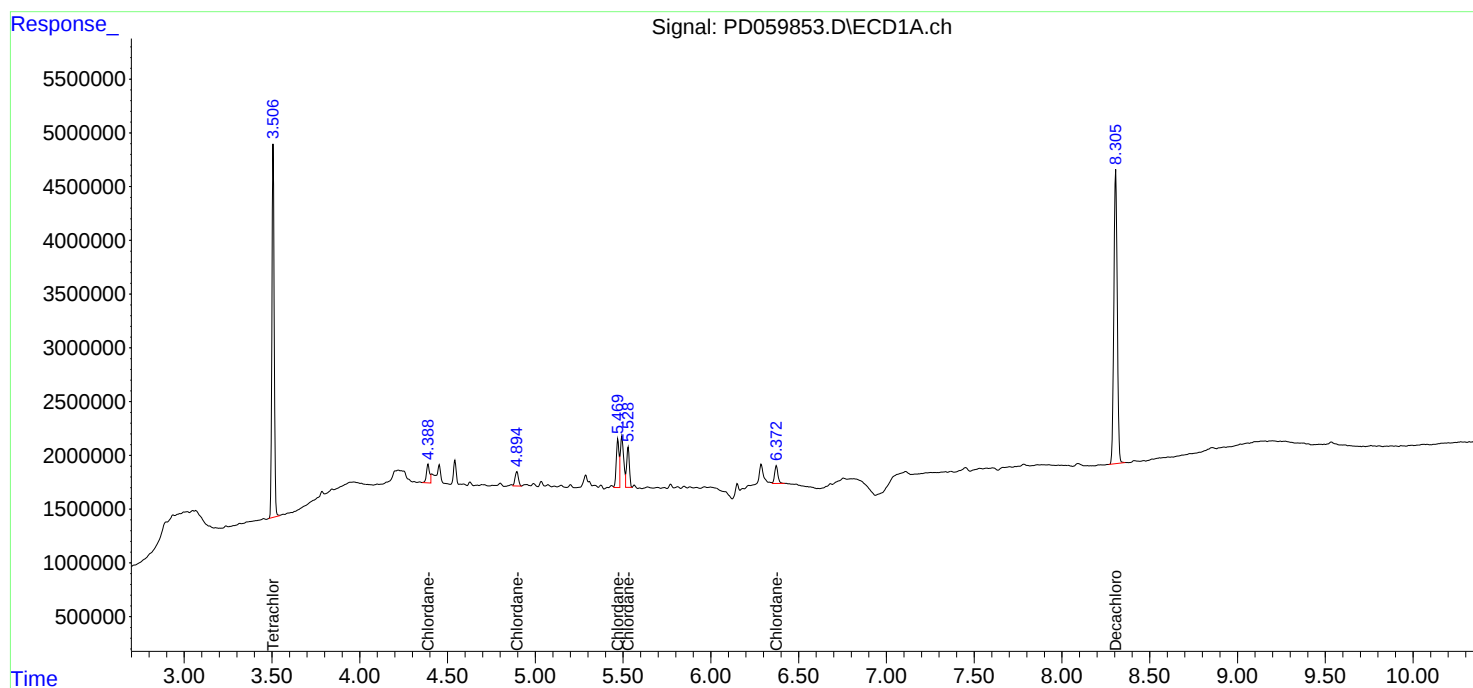


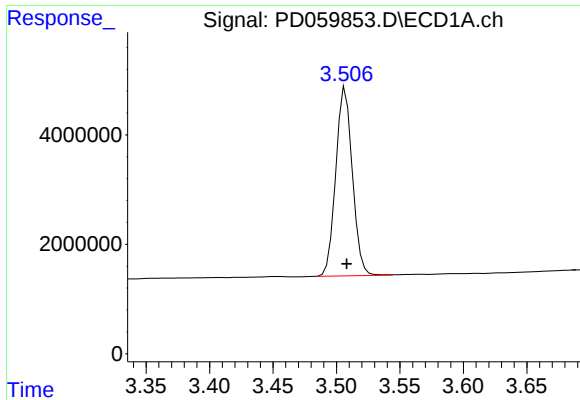

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 31370330
Conc: 21.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

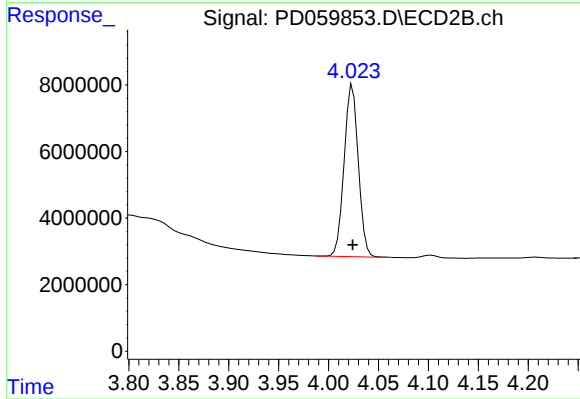


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 50966568
Conc: 20.76 ng/ml

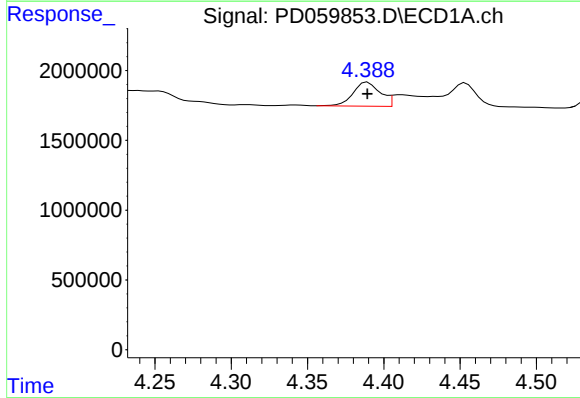


#23 Chlordane-1

R.T.: 4.389 min
Delta R.T.: 0.000 min
Response: 2125248
Conc: 34.57 ng/ml

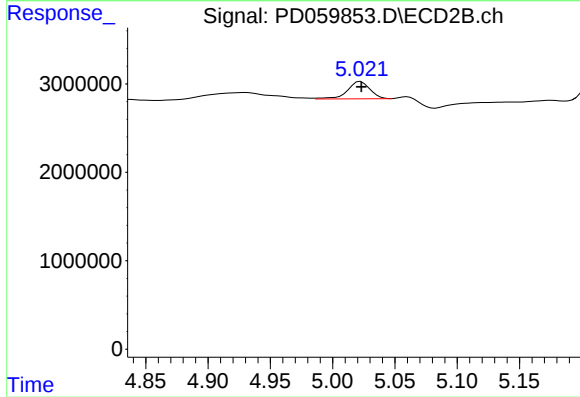

#23 Chlordane-1


R.T.: 5.023 min
Delta R.T.: 0.000 min
Response: 2464436
Conc: 25.77 ng/ml

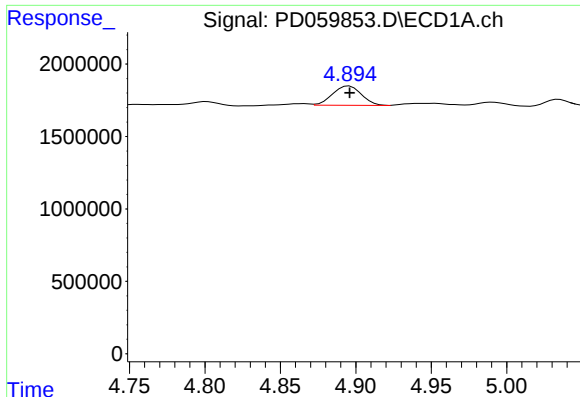

#24 Chlordane-2


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 1775976
Conc: 28.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

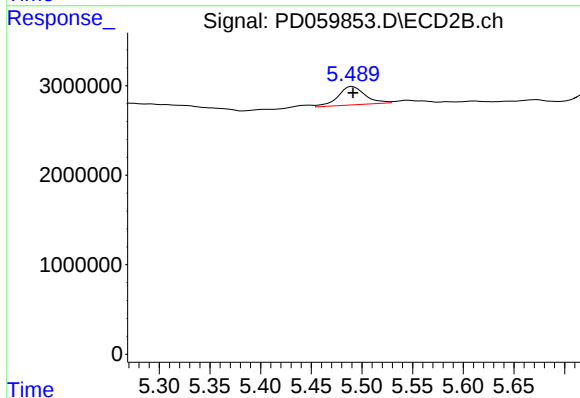


#24 Chlordane-2

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 3824838
Conc: 38.81 ng/ml

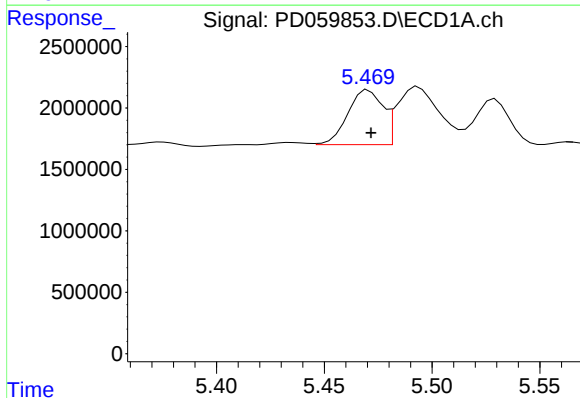


#25 Chlordane-3

R.T.: 5.471 min
Delta R.T.: -0.001 min
Response: 5002787
Conc: 26.53 ng/ml

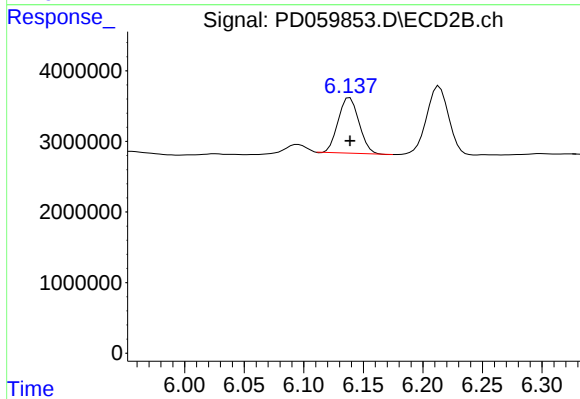

#25 Chlordane-3


R.T.: 6.139 min
Delta R.T.: 0.000 min
Response: 9547822
Conc: 25.31 ng/ml

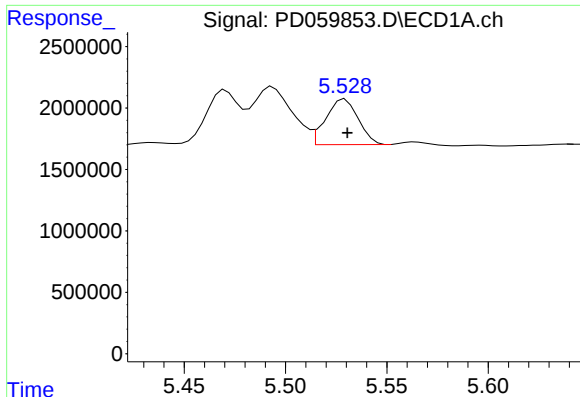

#26 Chlordane-4


R.T.: 5.529 min
Delta R.T.: -0.001 min
Response: 4124263
Conc: 27.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

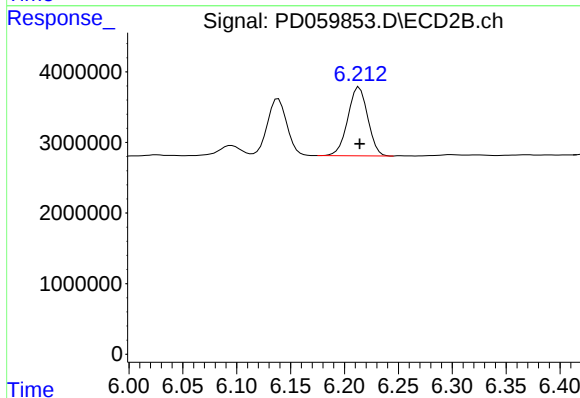


#26 Chlordane-4

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 12554803
Conc: 28.10 ng/ml

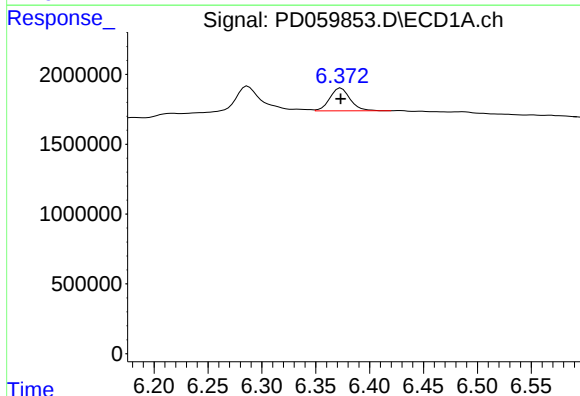


#27 Chlordane-5

R.T.: 6.373 min
Delta R.T.: 0.000 min
Response: 2146036
Conc: 29.66 ng/ml

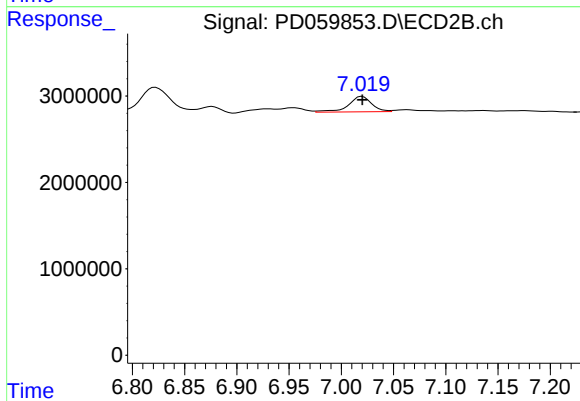

#27 Chlordane-5


R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 2750938
Conc: 33.41 ng/ml

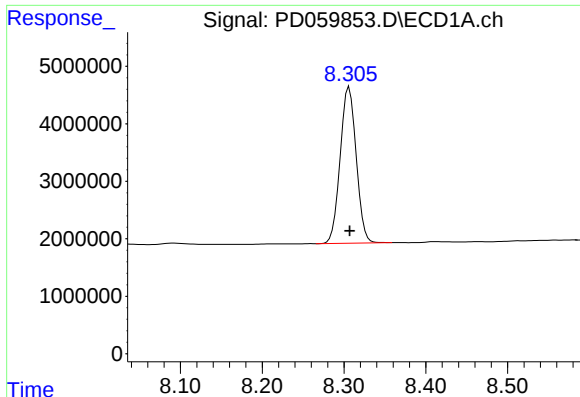

#28 Decachlorobiphenyl

R.T.: 8.306 min
Delta R.T.: 0.000 min
Response: 36827438
Conc: 23.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

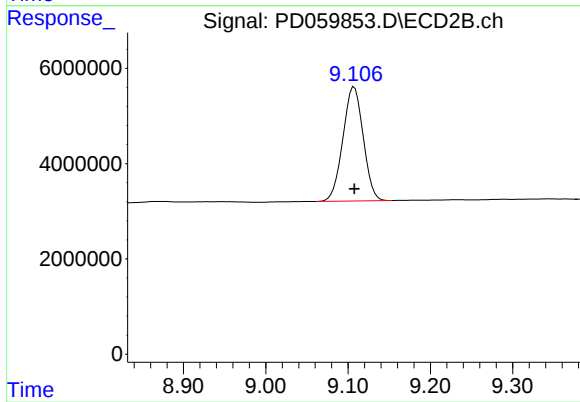

#28 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: 0.000 min
Response: 41214525
Conc: 22.76 ng/ml