

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102020\
 Data File : PD059854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2020 14:34
 Operator : DD\AJ
 Sample : L4214-08
 Misc : CHLOR LOQ 50 PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOQ-WATER-02-QT4-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 08:17:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:13:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.024	30347026	48306741	20.438	19.681
28)	SA Decachlor...	8.306	9.108	35086062	41218019	22.693	22.761
Target Compounds							
23)	Chlordane-1	4.388	5.023	3529153	4248406	57.412	44.420
24)	Chlordane-2	4.894	5.491	3369391	6087129	54.740	61.769
25)	Chlordane-3	5.470	6.139	9644731	17689273	51.152	46.884
26)	Chlordane-4	5.529	6.213	8008324	22914124	52.439	51.294
27)	Chlordane-5	6.373	7.020	3634283	4633721	50.221	56.269



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102020\
Data File : PD059854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2020 14:34
Operator : DD\AJ
Sample : L4214-08
Misc : CHLOR LOQ 50 PPB
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT4-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 08:17:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:13:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

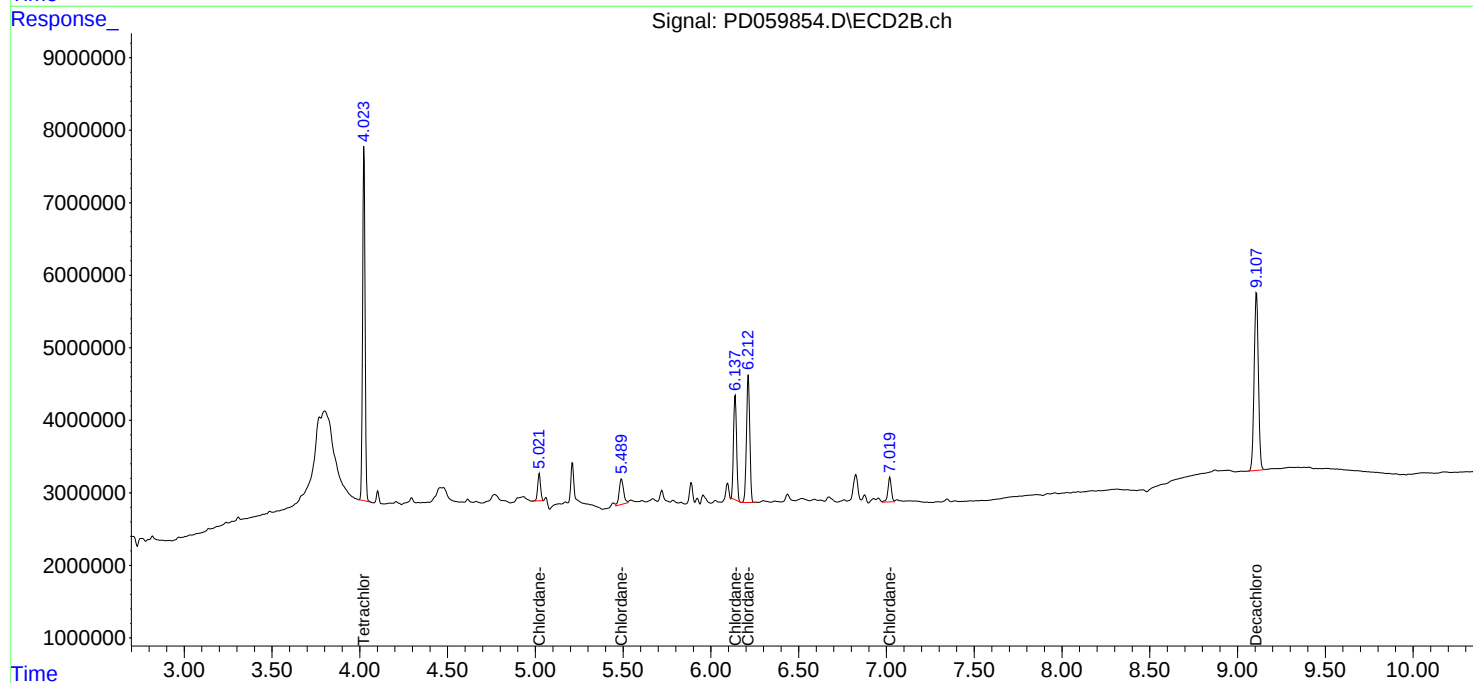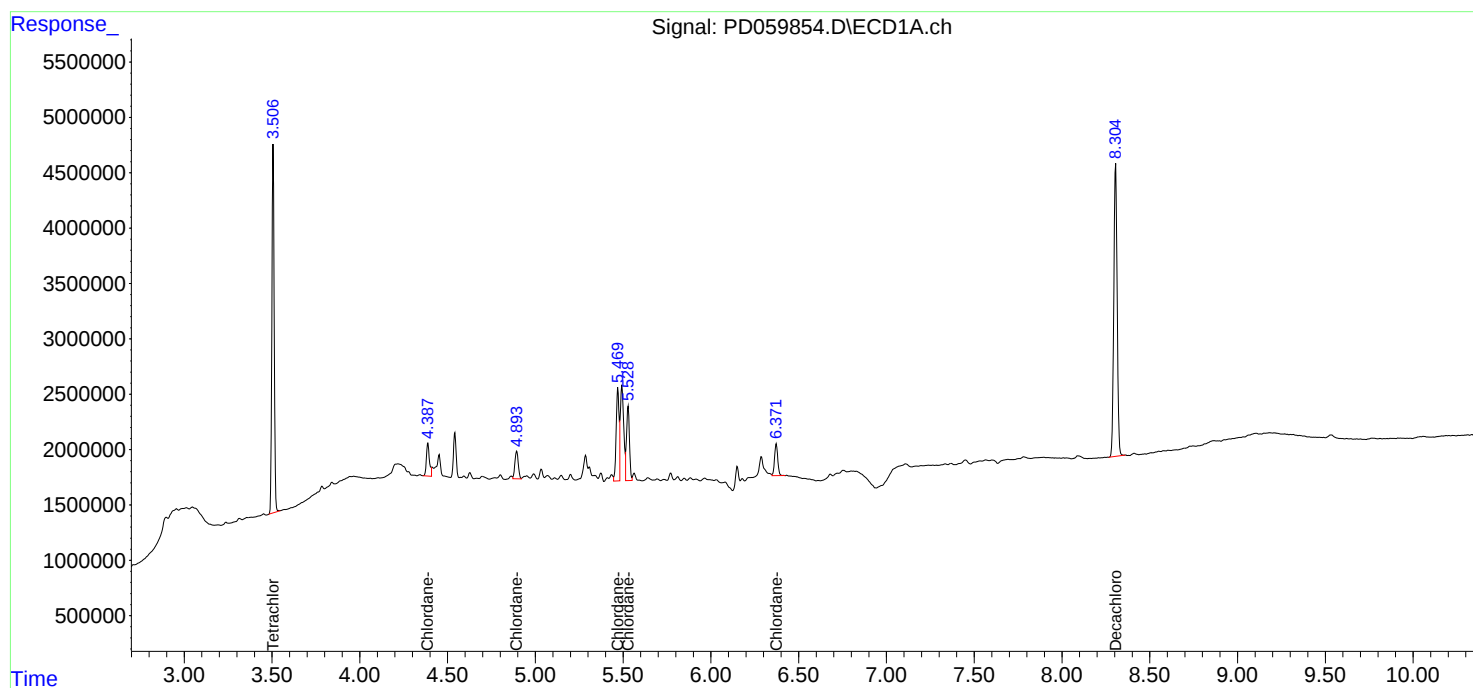


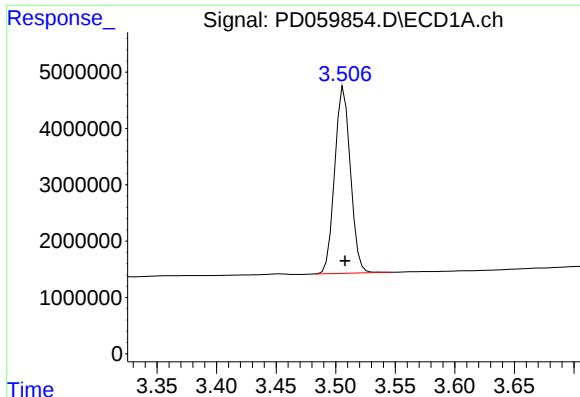

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: -0.001 min
Response: 30347026
Conc: 20.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT4-2020

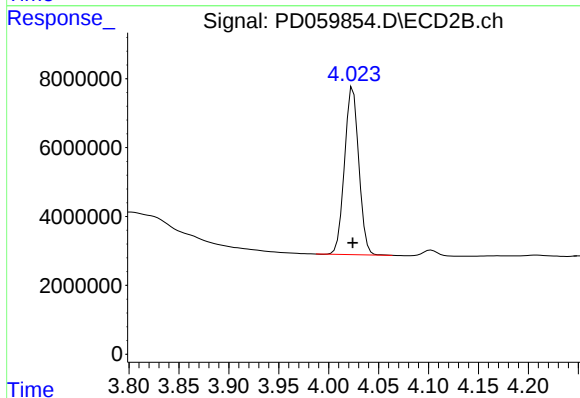


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 48306741
Conc: 19.68 ng/ml

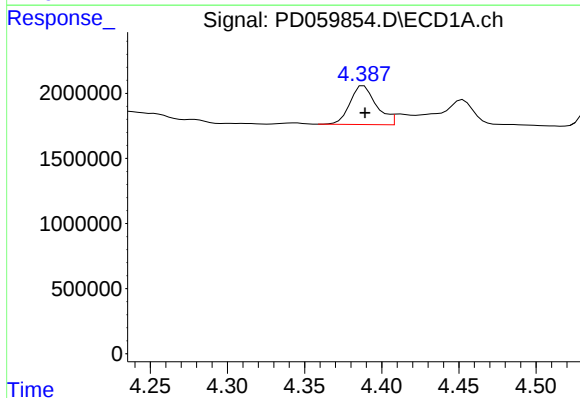


#23 Chlordane-1

R.T.: 4.388 min
Delta R.T.: 0.000 min
Response: 3529153
Conc: 57.41 ng/ml

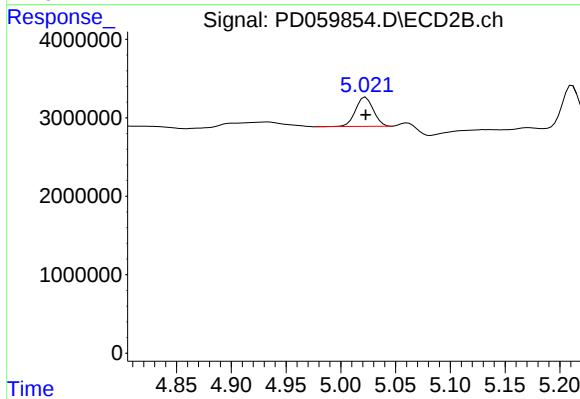

#23 Chlordane-1


R.T.: 5.023 min
Delta R.T.: 0.000 min
Response: 4248406
Conc: 44.42 ng/ml

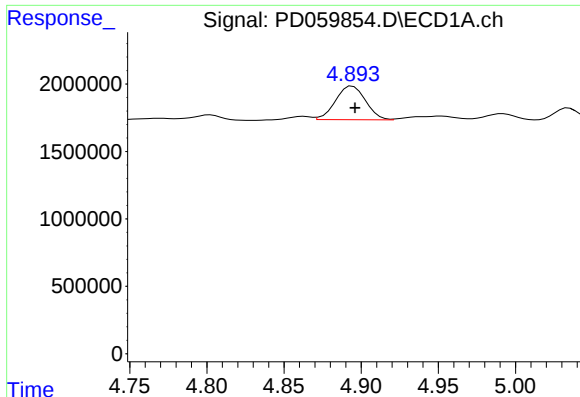

#24 Chlordane-2


R.T.: 4.894 min
Delta R.T.: -0.002 min
Response: 3369391
Conc: 54.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT4-2020

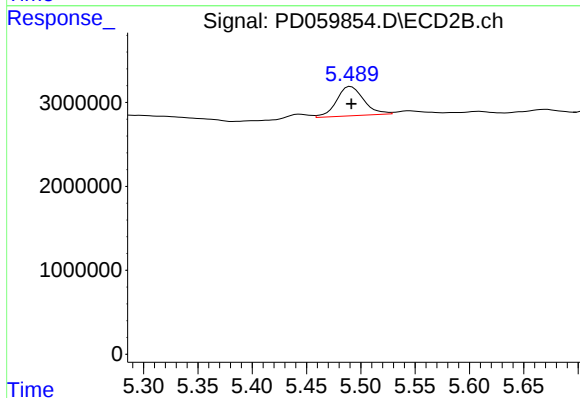


#24 Chlordane-2

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 6087129
Conc: 61.77 ng/ml

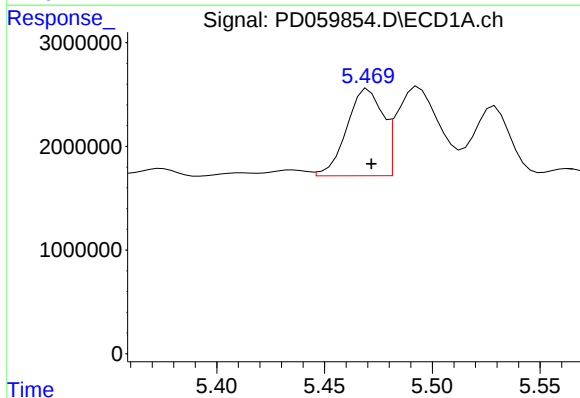


#25 Chlordane-3

R.T.: 5.470 min
Delta R.T.: -0.001 min
Response: 9644731
Conc: 51.15 ng/ml

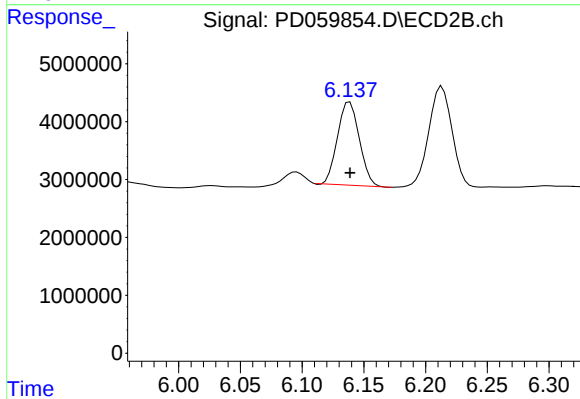

#25 Chlordane-3


R.T.: 6.139 min
Delta R.T.: 0.000 min
Response: 17689273
Conc: 46.88 ng/ml

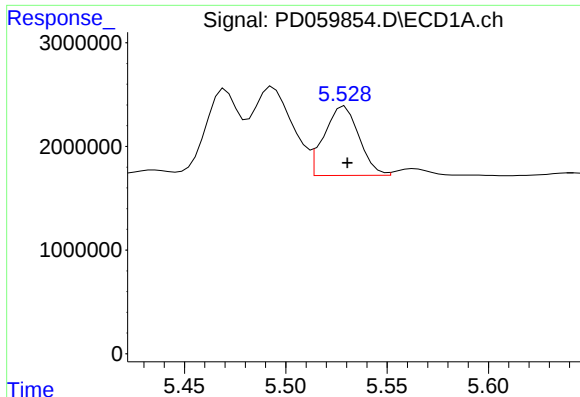

#26 Chlordane-4


R.T.: 5.529 min
Delta R.T.: -0.001 min
Response: 8008324
Conc: 52.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT4-2020

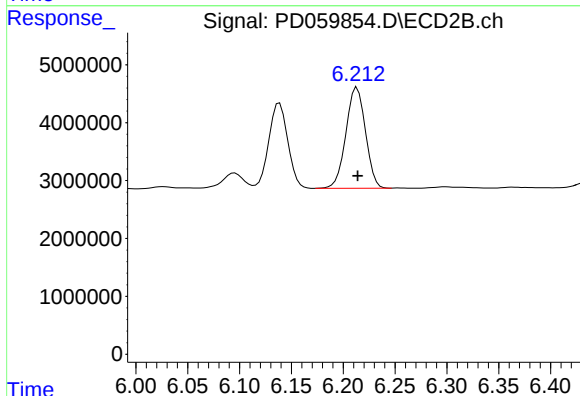


#26 Chlordane-4

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 22914124
Conc: 51.29 ng/ml

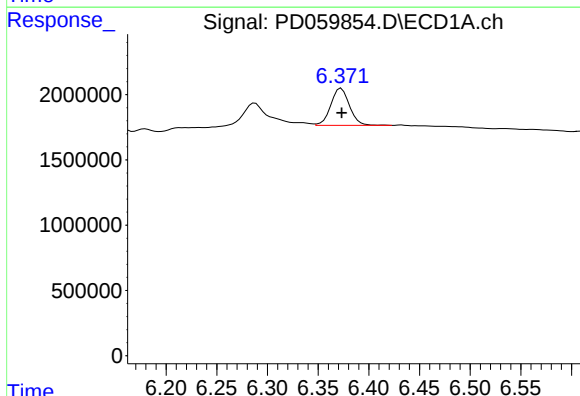


#27 Chlordane-5

R.T.: 6.373 min
Delta R.T.: 0.000 min
Response: 3634283
Conc: 50.22 ng/ml

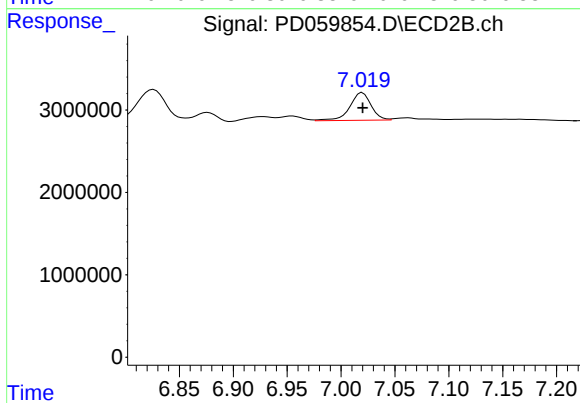

#27 Chlordane-5


R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 4633721
Conc: 56.27 ng/ml

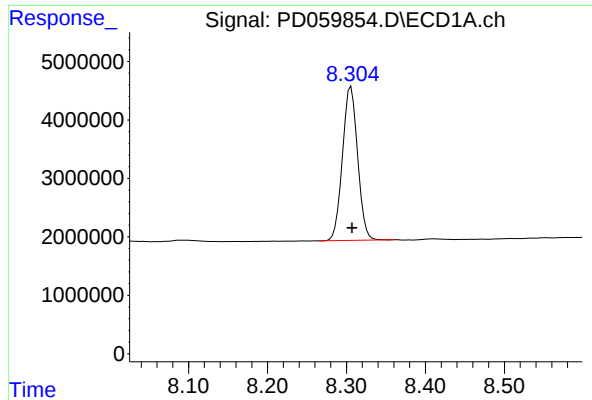

#28 Decachlorobiphenyl

R.T.: 8.306 min
Delta R.T.: -0.001 min
Response: 35086062
Conc: 22.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT4-2020

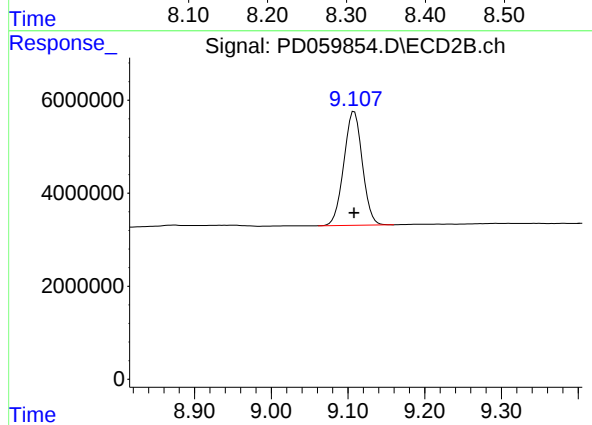

#28 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: 0.000 min
Response: 41218019
Conc: 22.76 ng/ml