

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102021\
 Data File : PD066443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2021 15:03
 Operator : AJ\MA
 Sample : M4126-16DL 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AD1DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/21/2021
 Supervised By : mohammad ahmed 10/21/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:21:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.446	3.978	256.7E6	21148.5E6	125.704	2373.169m#
2) SA Decachlor...	8.182	8.997	156.4E6	113.9E6	115.065m	23.986m#
Target Compounds						
8) B Heptachlo...	5.137	5.830	115.6E6	502.2E6	42.716	62.538m#
12) B 4,4'-DDE	5.597	6.306	53184058	300.7E6	21.233m	37.846 #
14) MA Endrin	5.971	6.664	86428378	747.5E6	36.355m	141.227m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102021\
Data File : PD066443.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2021 15:03
Operator : AJ\MA
Sample : M4126-16DL 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:21:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

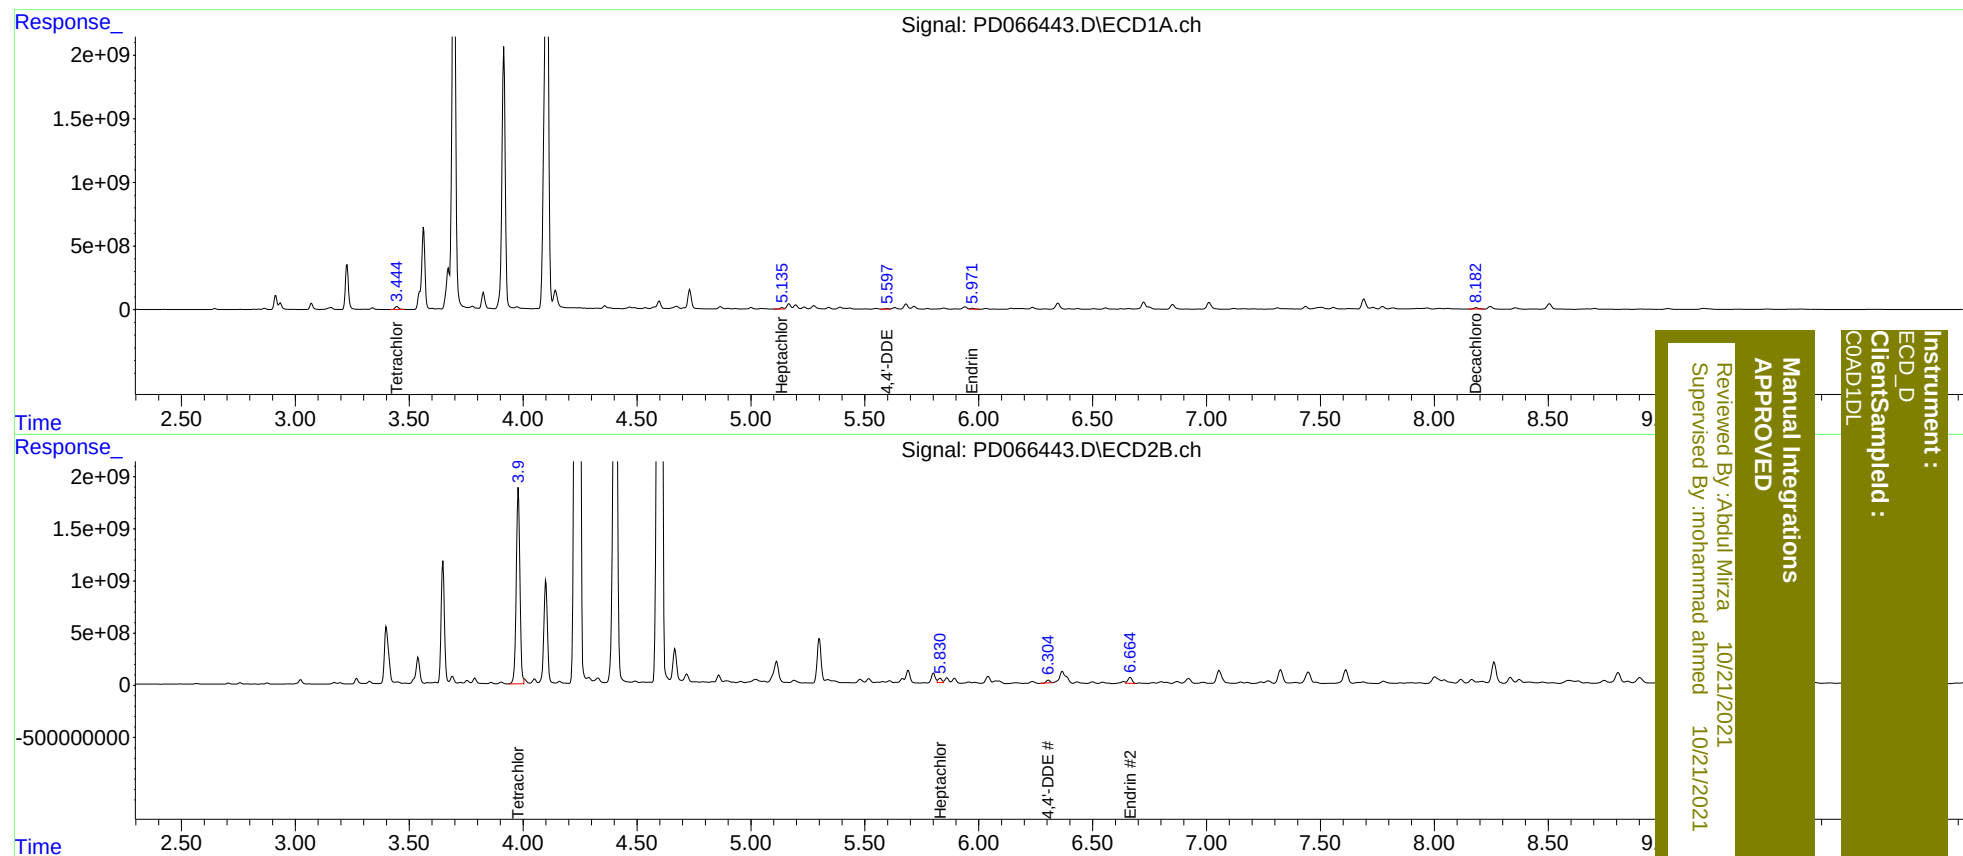

Instrument :
ECD_D
ClientSampled :
COAD1DL

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 10/21/2021
Supervised By: mohammad ahmed 10/21/2021