

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102021\
 Data File : PD066454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2021 18:04
 Operator : AJ\MA
 Sample : M4217-07MS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JDGE3MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/21/2021
 Supervised By :mohammad ahmed 10/21/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 08:33:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	17279954	73557960	8.463	8.254
27)	SA Decachlor...	8.163	9.017	16291453	43652585	11.983m	9.192m
Target Compounds							
2)	A alpha-BHC	3.877	4.363	137.9E6	462.9E6	44.194	39.844
3)	MA gamma-BHC...	4.159	4.648	130.7E6	434.5E6	42.351	39.365
4)	MA Heptachlor	4.453	5.147	133.3E6	413.6E6	45.538	40.876
5)	MB Aldrin	4.698	5.451	129.4E6	383.9E6	42.093	38.072
6)	B beta-BHC	4.407	4.824	50818885	190.7E6	38.166	36.620
7)	B delta-BHC	4.609	5.038	125.4E6	356.6E6	43.462	36.851m
8)	B Heptachlo...	5.139	5.839	117.9E6	272.9E6	43.559	33.981
9)	A Endosulfan I	5.475	6.196	107.4E6	338.6E6	42.501	40.150
10)	B trans-Chl...	5.362	6.073	119.7E6	354.2E6	43.688	39.176
11)	B cis-Chlor...	5.421	6.144	116.7E6	352.4E6	43.528	39.758
12)	B 4,4'-DDE	5.585	6.304	232.3E6	685.7E6	92.733	86.293
13)	MA Dieldrin	5.717	6.454	250.3E6	716.3E6	93.182	84.740
14)	MA Endrin	5.973	6.672	214.8E6	598.7E6	90.339	113.118 #
15)	B Endosulfa...	6.246	6.886	202.4E6	569.1E6	90.116	79.864
16)	A 4,4'-DDD	6.099	6.798	189.3E6	561.9E6	91.163	84.216
17)	MA 4,4'-DDT	6.337	7.095	205.5E6	596.2E6	103.260	90.914
18)	B Endrin al...	6.415	7.010	162.7E6	492.5E6	103.849	92.900
19)	B Endosulfa...	6.626	7.233	198.6E6	554.0E6	100.084	84.003
20)	A Methoxychlor	6.885	7.556	530.3E6	1322.3E6	511.417	407.157
21)	B Endrin ke...	7.117	7.705	196.1E6	639.3E6	84.913	89.129

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102021\
Data File : PD066454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2021 18:04
Operator : AJ\MA
Sample : M4217-07MS
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 08:33:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

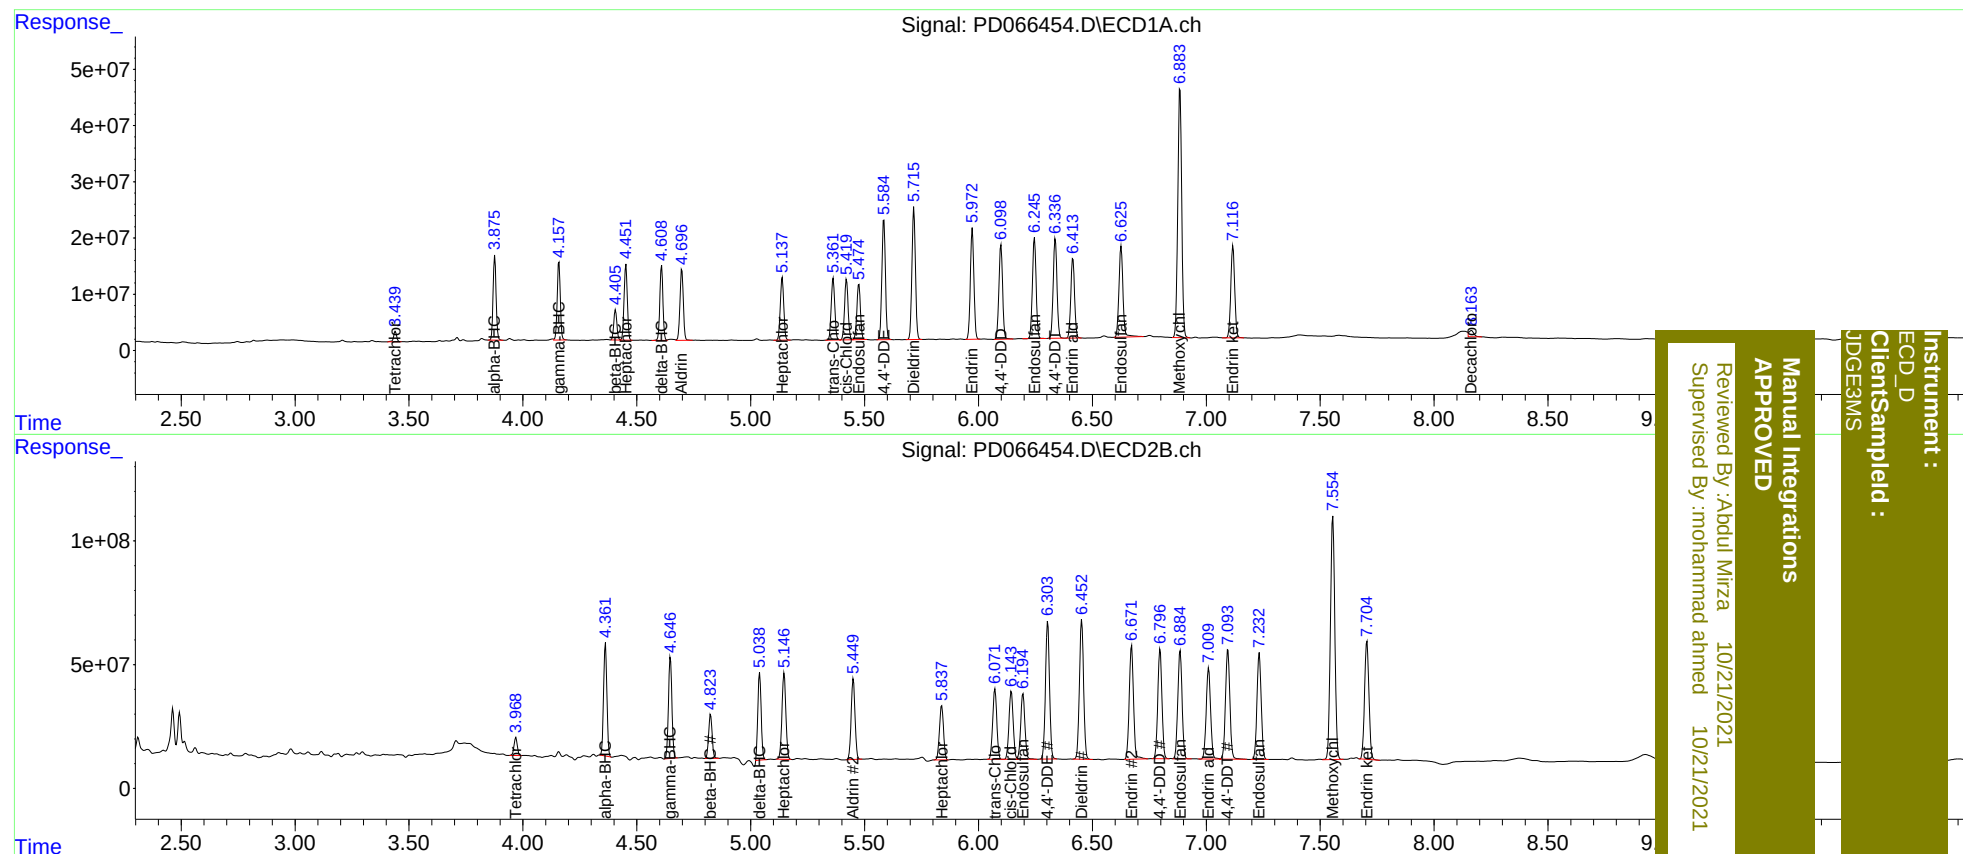

Instrument :
ECD_D
ClientSampled :
JDGE3MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 10/21/2021
Supervised By: mohammad ahmed 10/21/2021