

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102022\
 Data File : PD072532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2022 17:47
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:21:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 04:17:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.706	3.467	56544728	779.2E6	22.694	23.428
28)	SA Decachlor...	7.841	8.925	49937573	205.4E6	22.187	22.834
Target Compounds							
9)	A Endosulfan I	5.029	5.988	31586940	186.3E6	10.963	12.214
10)	B gamma-Chl...	4.908	5.857	34508147	199.2E6	10.886	12.092
12)	B 4,4'-DDE	5.160	6.106	64079977	347.0E6	21.451	22.676
13)	MA Dieldrin	5.295	6.265	67502512	365.8E6	22.091	23.146
19)	B Endosulfa...	6.276	7.092	50324055	234.1E6	20.016	20.656
20)	A Methoxychlor	6.552	7.420	141.2E6	587.6E6	104.925	99.238
21)	B Endrin ke...	6.787	7.582	63847721	272.3E6	21.373	21.824



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102022\
Data File : PD072532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2022 17:47
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:21:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 04:17:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

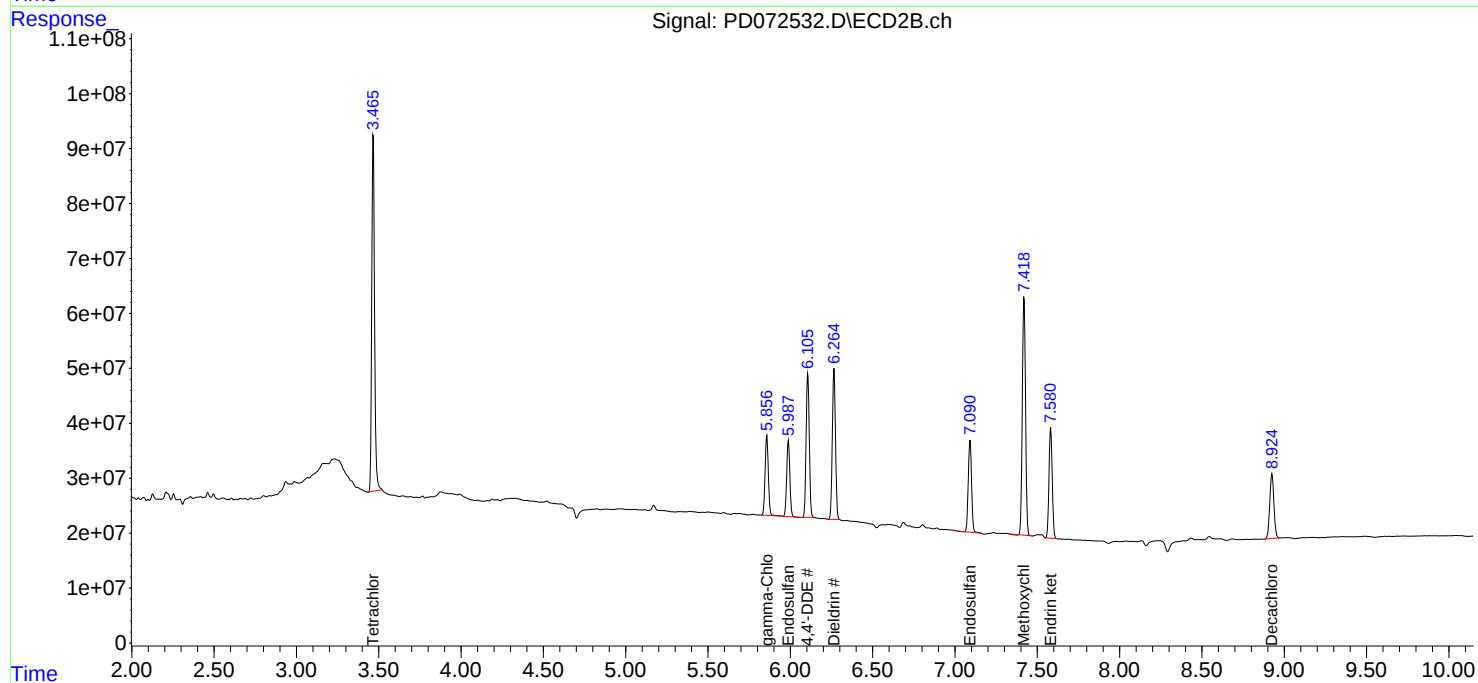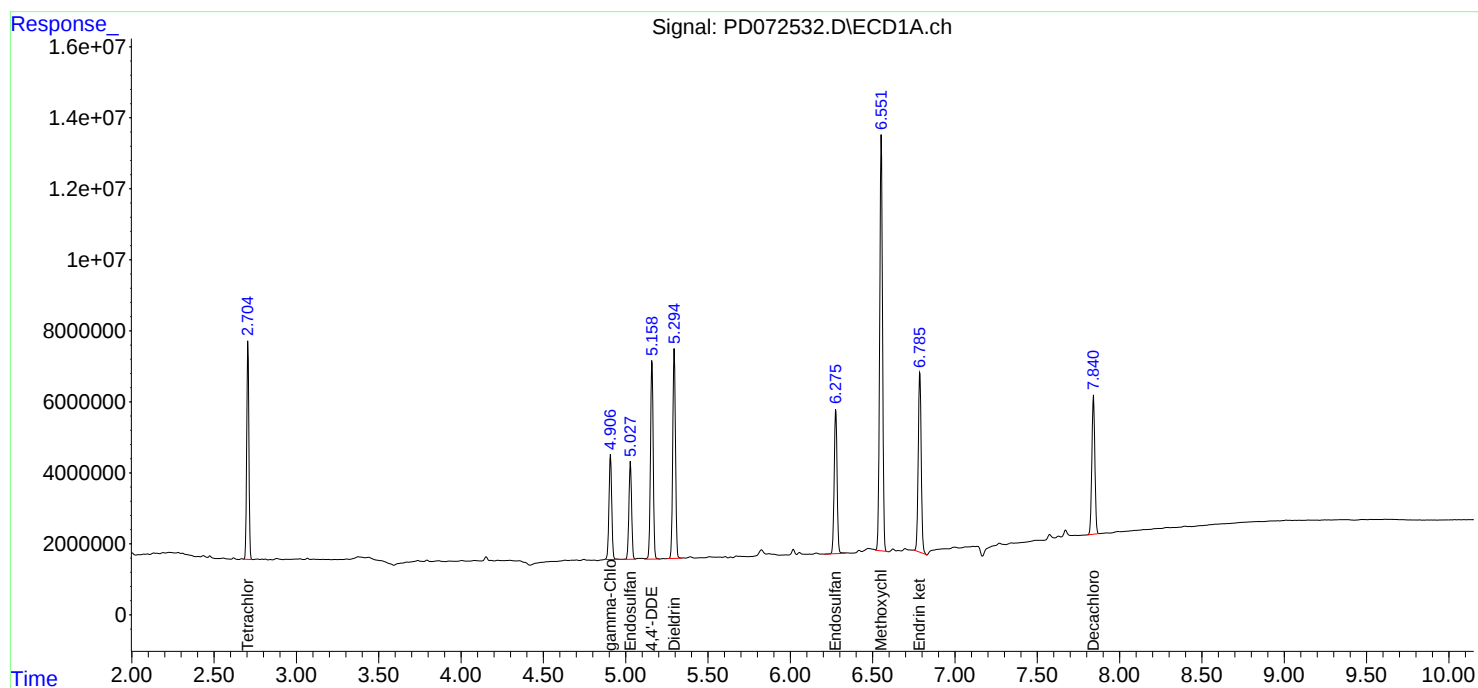


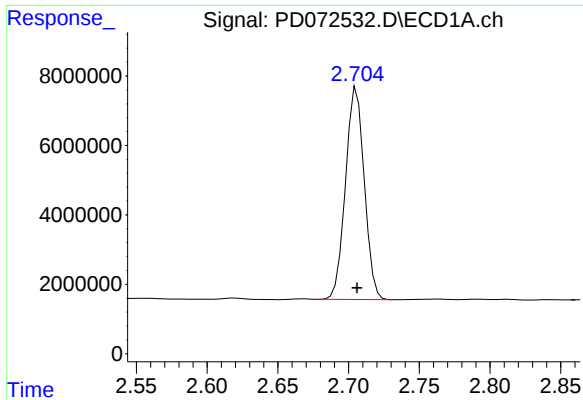

#1 Tetrachloro-m-xylene


R.T.: 2.706 min
Delta R.T.: 0.000 min
Response: 56544728
Conc: 22.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

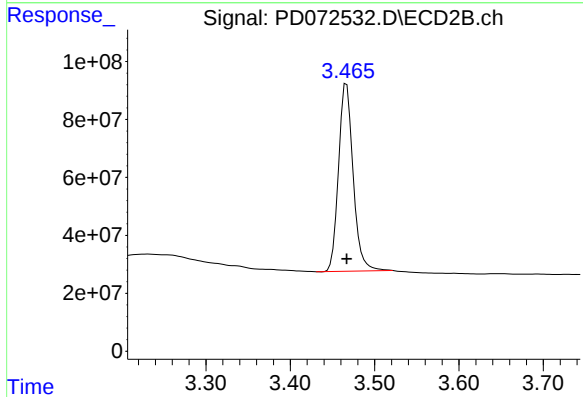


#1 Tetrachloro-m-xylene

R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 779153652
Conc: 23.43 ng/ml

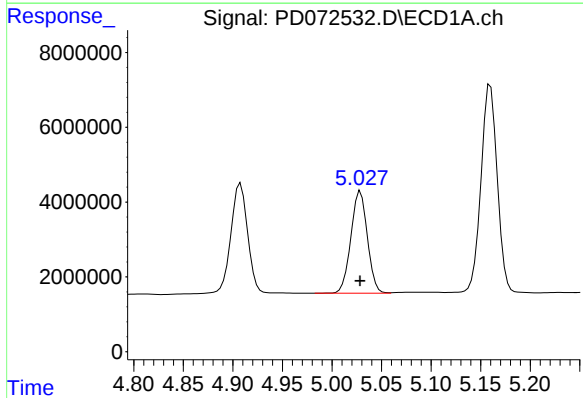


#9 Endosulfan I

R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 31586940
Conc: 10.96 ng/ml

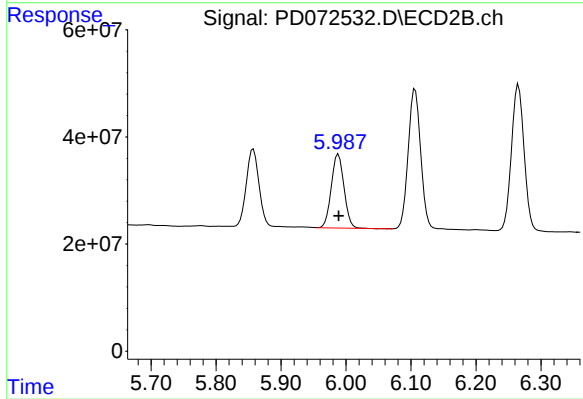

#9 Endosulfan I


R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 186337969
Conc: 12.21 ng/ml

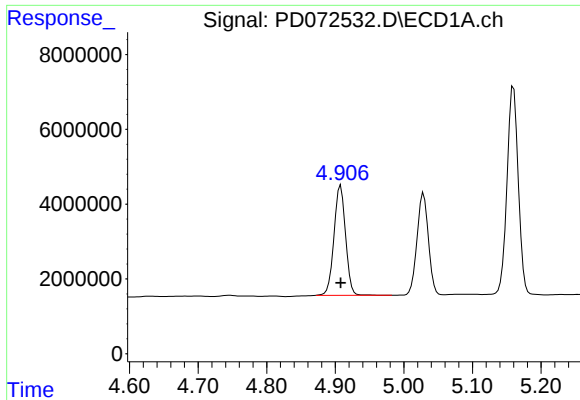

#10 gamma-Chlordane


R.T.: 4.908 min
Delta R.T.: 0.000 min
Response: 34508147
Conc: 10.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

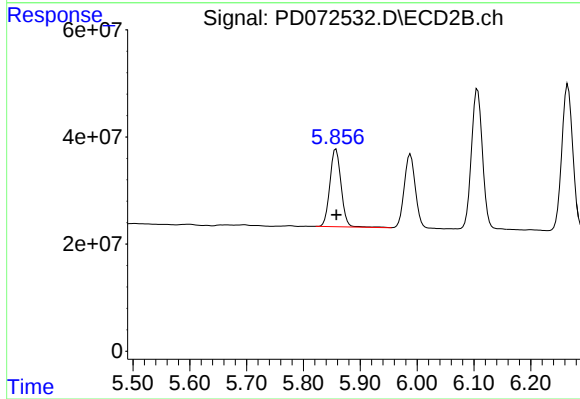


#10 gamma-Chlordane

R.T.: 5.857 min
Delta R.T.: 0.000 min
Response: 199222546
Conc: 12.09 ng/ml

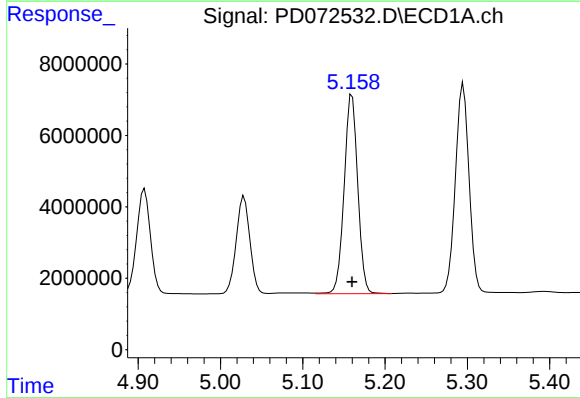


#12 4,4'-DDE

R.T.: 5.160 min
Delta R.T.: 0.000 min
Response: 64079977
Conc: 21.45 ng/ml

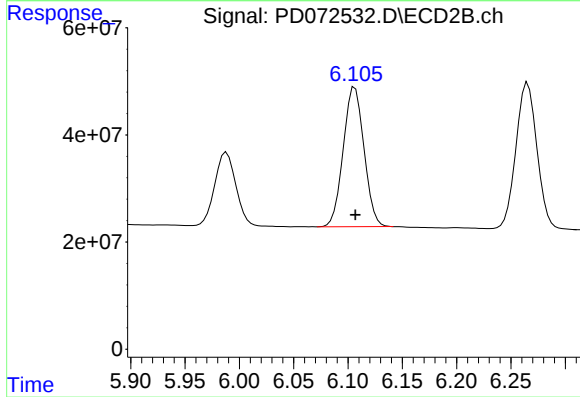

#12 4,4'-DDE


R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 347027410
Conc: 22.68 ng/ml

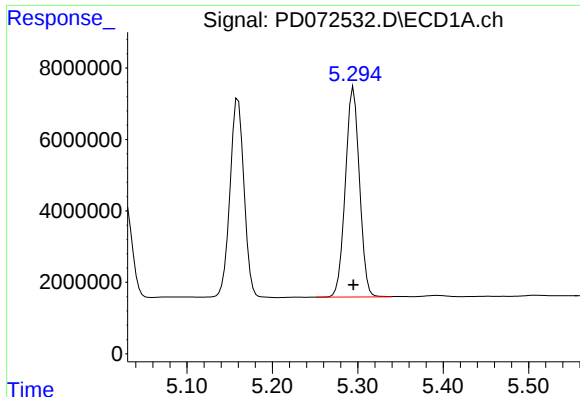

#13 Dieldrin


R.T.: 5.295 min
Delta R.T.: 0.000 min
Response: 67502512
Conc: 22.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

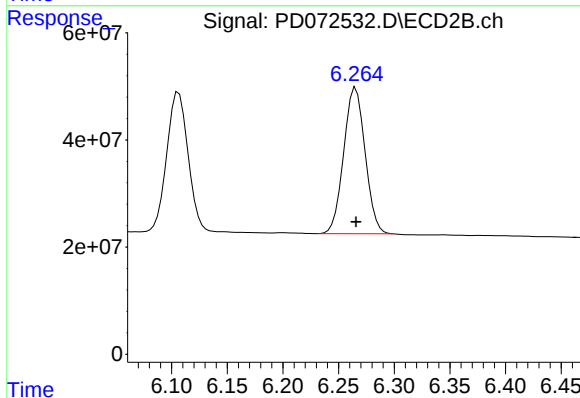


#13 Dieldrin

R.T.: 6.265 min
Delta R.T.: 0.000 min
Response: 365756575
Conc: 23.15 ng/ml

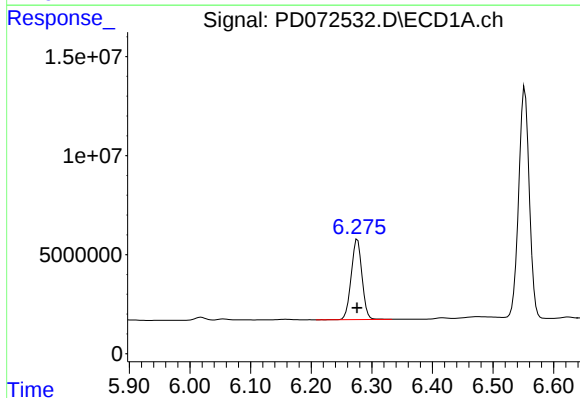


#19 Endosulfan Sulfate

R.T.: 6.276 min
Delta R.T.: 0.000 min
Response: 50324055
Conc: 20.02 ng/ml

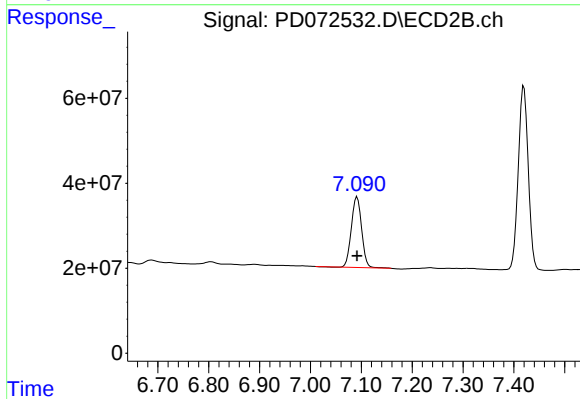

#19 Endosulfan Sulfate


R.T.: 7.092 min
Delta R.T.: 0.000 min
Response: 234136902
Conc: 20.66 ng/ml

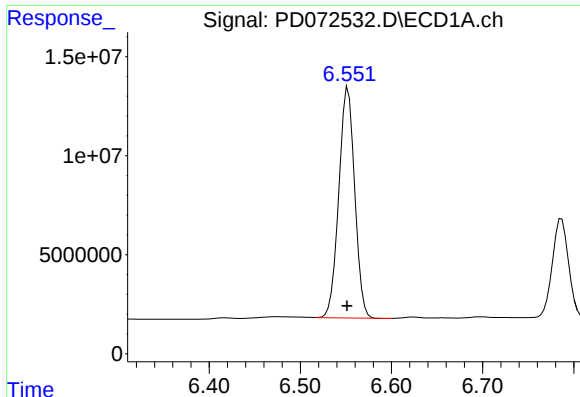

#20 Methoxychlor


R.T.: 6.552 min
Delta R.T.: 0.001 min
Response: 141153830
Conc: 104.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

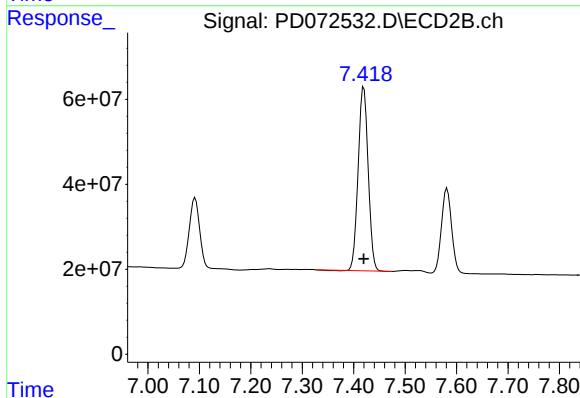


#20 Methoxychlor

R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 587606080
Conc: 99.24 ng/ml

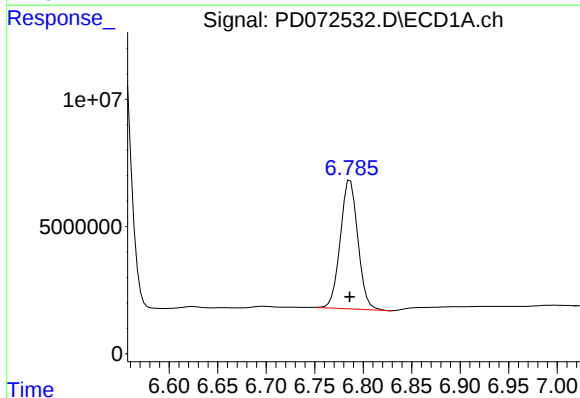


#21 Endrin ketone

R.T.: 6.787 min
Delta R.T.: 0.000 min
Response: 63847721
Conc: 21.37 ng/ml

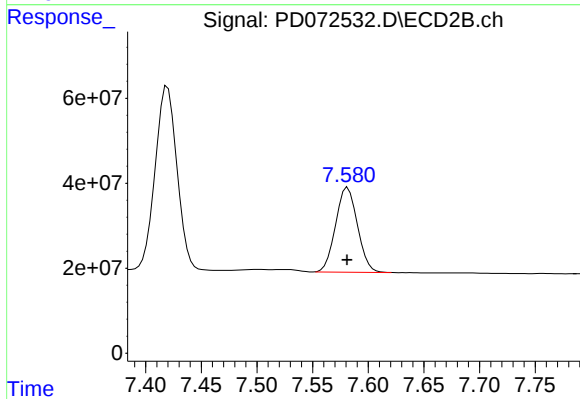

#21 Endrin ketone


R.T.: 7.582 min
Delta R.T.: 0.000 min
Response: 272321407
Conc: 21.82 ng/ml

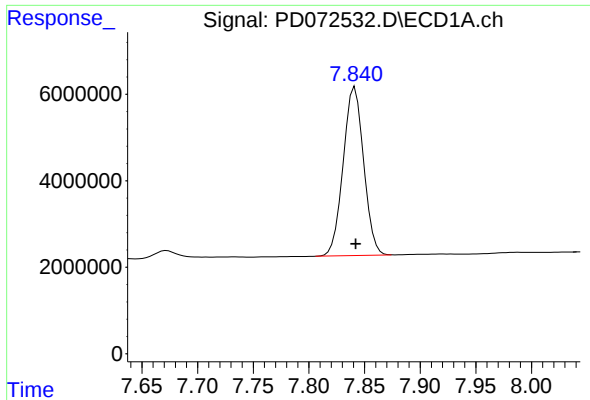

#28 Decachlorobiphenyl

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 49937573
Conc: 22.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

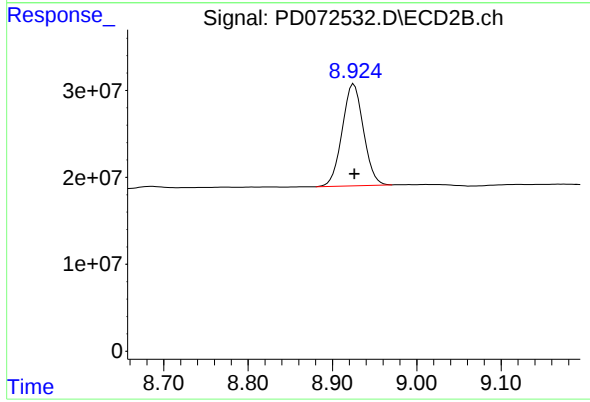

#28 Decachlorobiphenyl

R.T.: 8.925 min
Delta R.T.: 0.000 min
Response: 205435418
Conc: 22.83 ng/ml