

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102022\
 Data File : PD072538.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2022 19:07
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 00:57:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 00:57:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.705	3.466	289.5E6	3039.9E6	98.198	95.488
28)	SA Decachlor...	7.840	8.923	213.2E6	827.3E6	96.744	95.971
Target Compounds							
23)	Chlordane-1	3.699	4.617	90806883	895.7E6	977.938	941.007
24)	Chlordane-2	4.277	5.148	103.9E6	669.2E6	952.179	932.954
25)	Chlordane-3	4.908	5.857	341.8E6	2105.6E6	987.339	962.266
26)	Chlordane-4	4.970	5.933	342.1E6	2424.8E6	999.528	960.557
27)	Chlordane-5	5.867	6.790	109.3E6	456.1E6	982.876	957.695


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102022\
Data File : PD072538.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2022 19:07
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 00:57:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 00:57:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

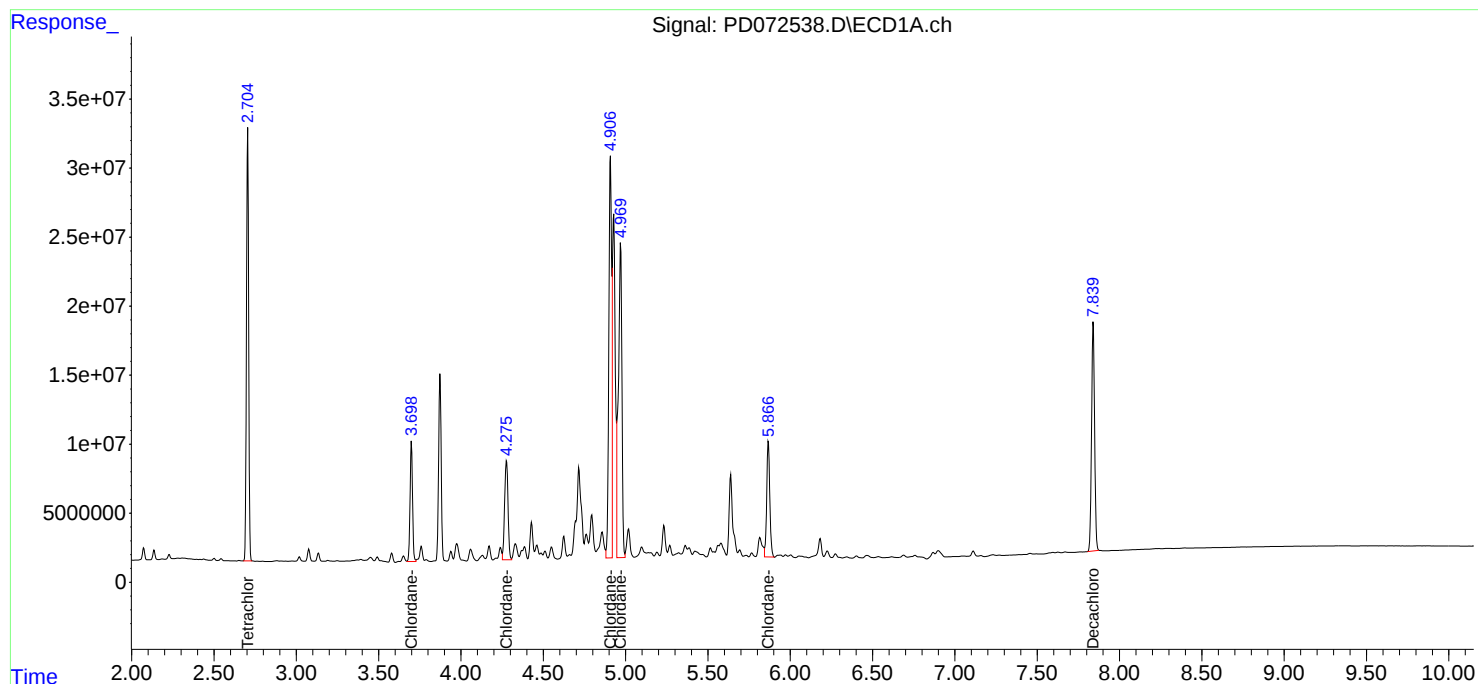


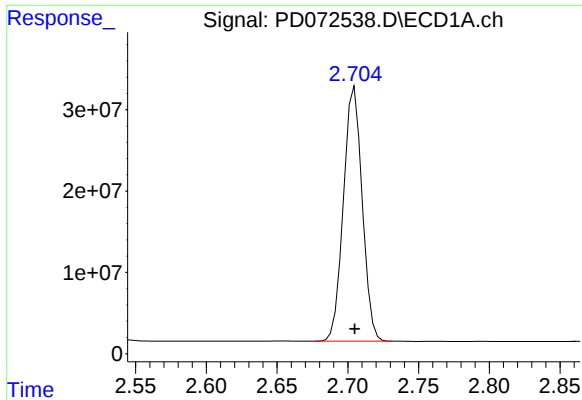

#1 Tetrachloro-m-xylene


R.T.: 2.705 min
Delta R.T.: 0.000 min
Response: 289526671
Conc: 98.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

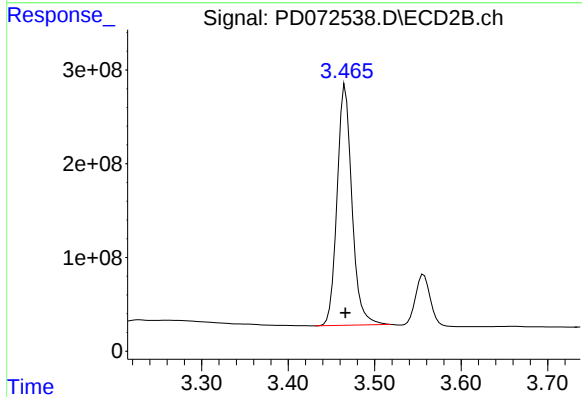


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 3039900493
Conc: 95.49 ng/ml

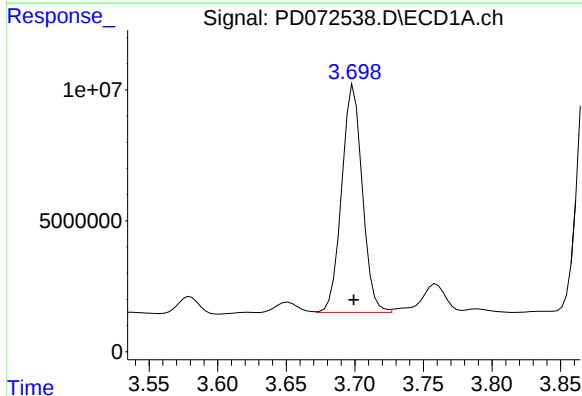


#23 Chlordane-1

R.T.: 3.699 min
Delta R.T.: 0.000 min
Response: 90806883
Conc: 977.94 ng/ml

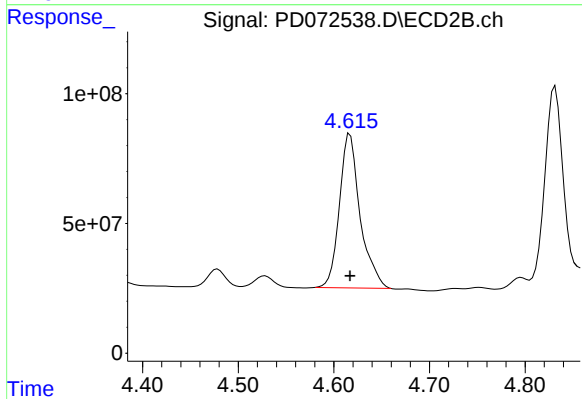

#23 Chlordane-1


R.T.: 4.617 min
Delta R.T.: 0.000 min
Response: 895666865
Conc: 941.01 ng/ml

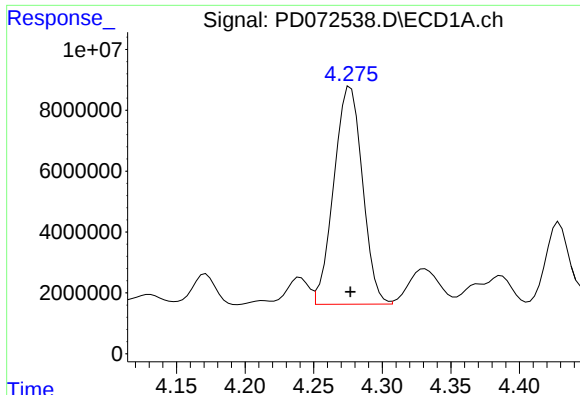

#24 Chlordane-2


R.T.: 4.277 min
Delta R.T.: 0.000 min
Response: 103869954
Conc: 952.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

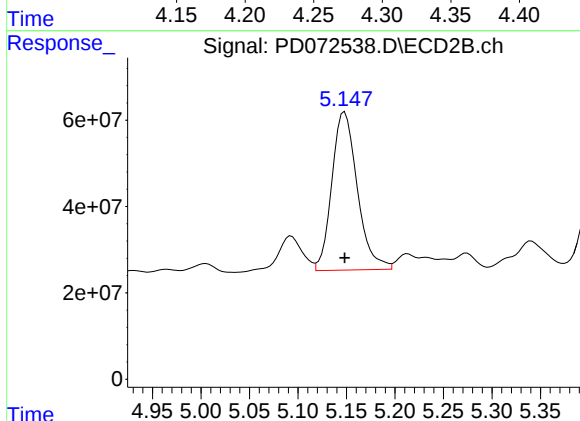


#24 Chlordane-2

R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 669209248
Conc: 932.95 ng/ml

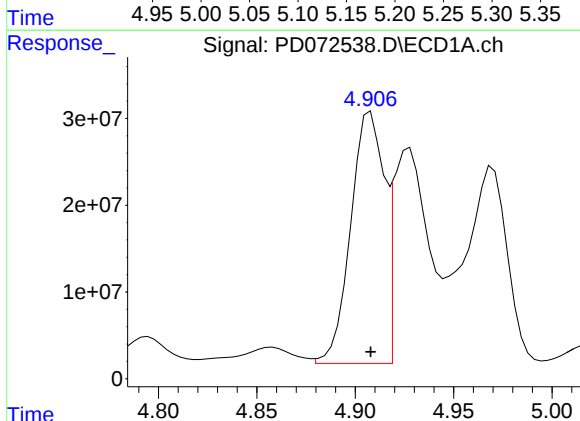


#25 Chlordane-3

R.T.: 4.908 min
Delta R.T.: 0.000 min
Response: 341765872
Conc: 987.34 ng/ml

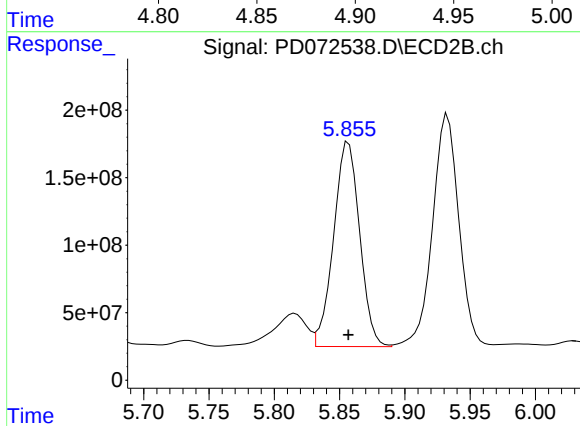

#25 Chlordane-3


R.T.: 5.857 min
Delta R.T.: 0.000 min
Response: 2105574037
Conc: 962.27 ng/ml

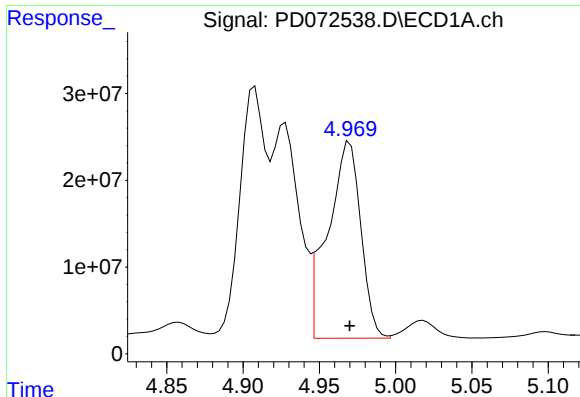

#26 Chlordane-4


R.T.: 4.970 min
Delta R.T.: 0.000 min
Response: 342055052
Conc: 999.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

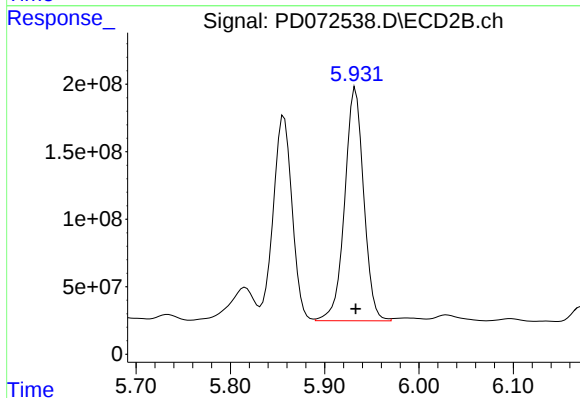


#26 Chlordane-4

R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 2424814544
Conc: 960.56 ng/ml

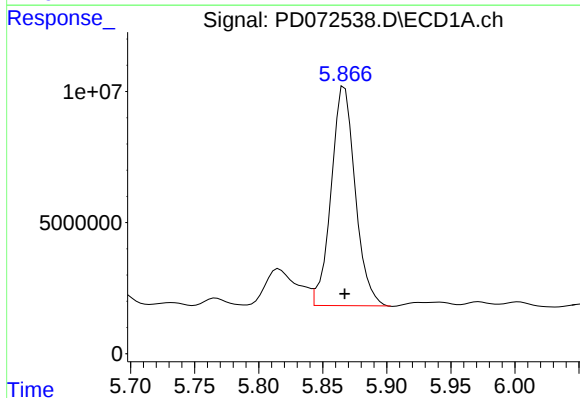


#27 Chlordane-5

R.T.: 5.867 min
Delta R.T.: 0.000 min
Response: 109258414
Conc: 982.88 ng/ml

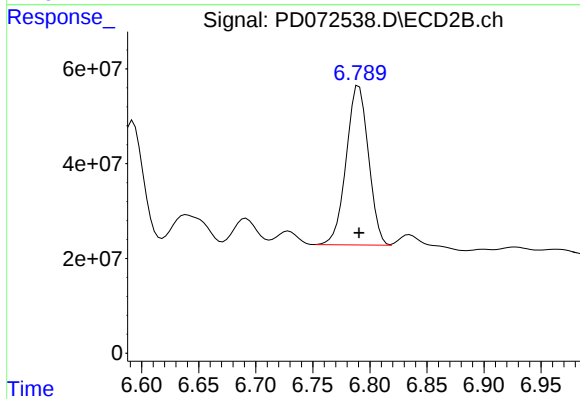

#27 Chlordane-5


R.T.: 6.790 min
Delta R.T.: 0.000 min
Response: 456062800
Conc: 957.70 ng/ml

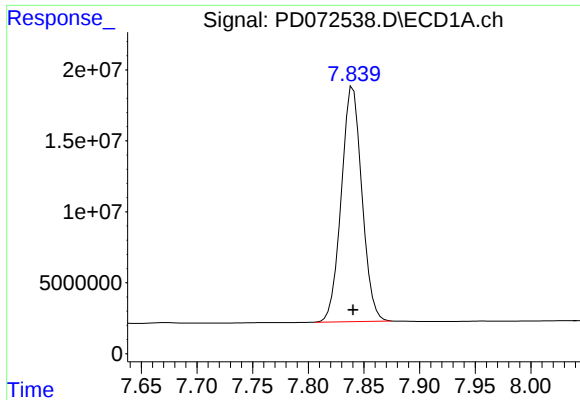

#28 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 213226877
Conc: 96.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

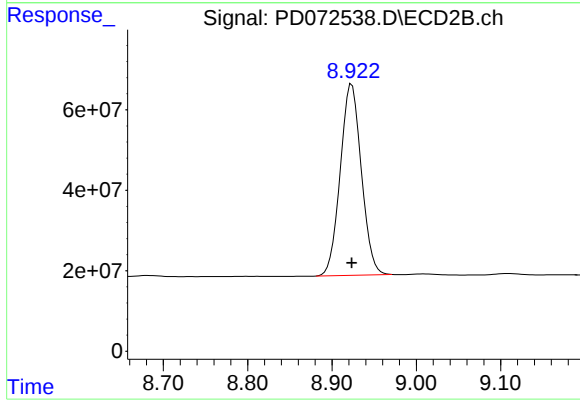

#28 Decachlorobiphenyl

R.T.: 8.923 min
Delta R.T.: 0.000 min
Response: 827297578
Conc: 95.97 ng/ml