

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102022\
 Data File : PD072539.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2022 19:21
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 01:00:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 01:00:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.705	3.466	215.9E6	2325.2E6	73.804	73.681
28)	SA Decachlor...	7.840	8.924	160.7E6	628.5E6	73.606	73.590
Target Compounds							
23)	Chlordane-1	3.699	4.617	67715571	688.1E6	736.043	731.743
24)	Chlordane-2	4.277	5.149	79921963	521.2E6	738.341	734.259
25)	Chlordane-3	4.908	5.857	256.5E6	1595.0E6	743.898	735.830
26)	Chlordane-4	4.970	5.933	250.1E6	1838.7E6	737.047	735.442
27)	Chlordane-5	5.867	6.790	81086117	347.6E6	736.168	736.513



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102022\
Data File : PD072539.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2022 19:21
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 01:00:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 01:00:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

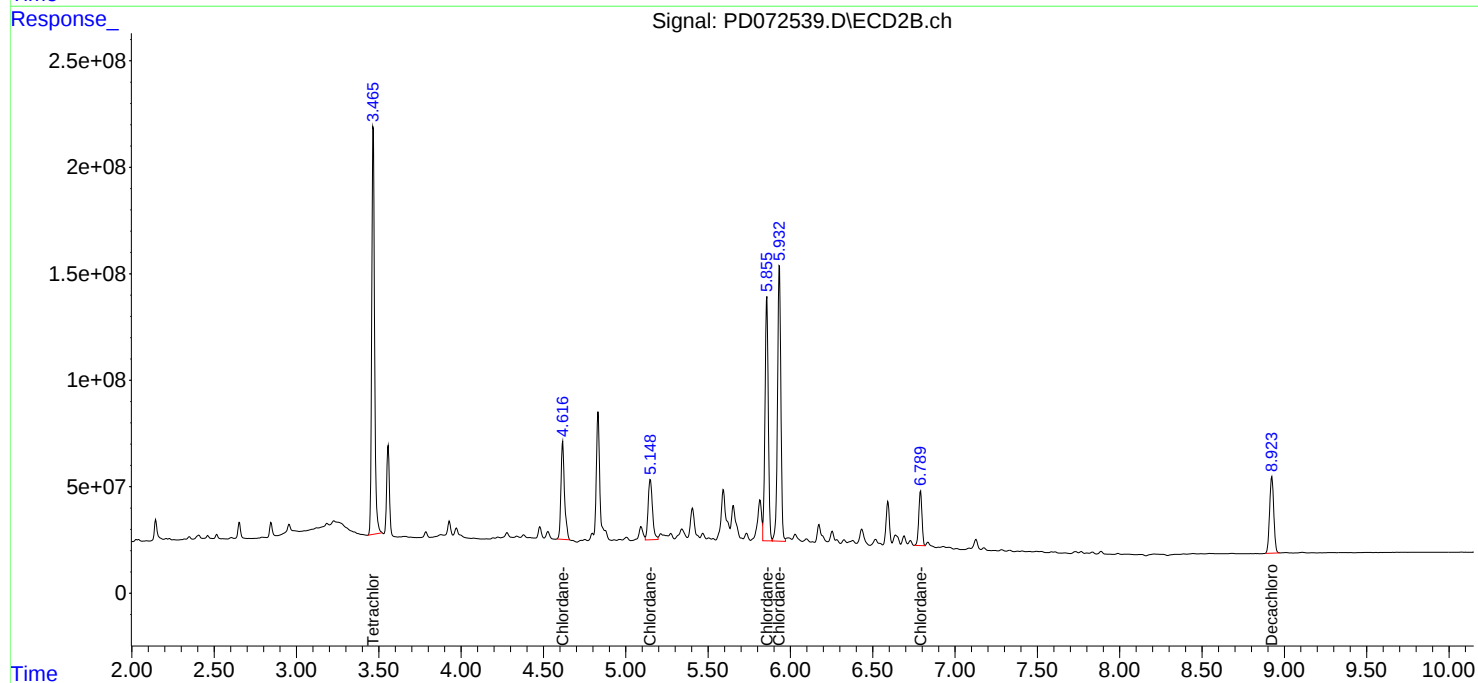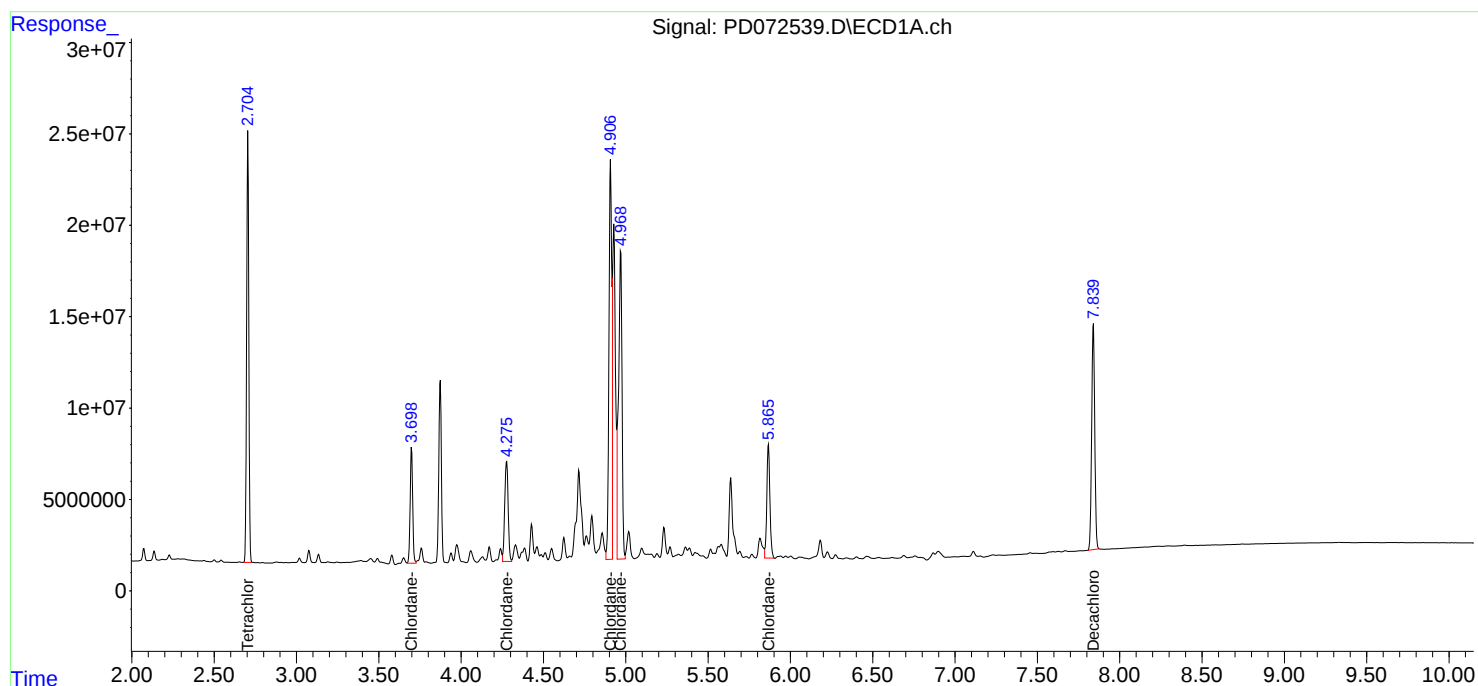


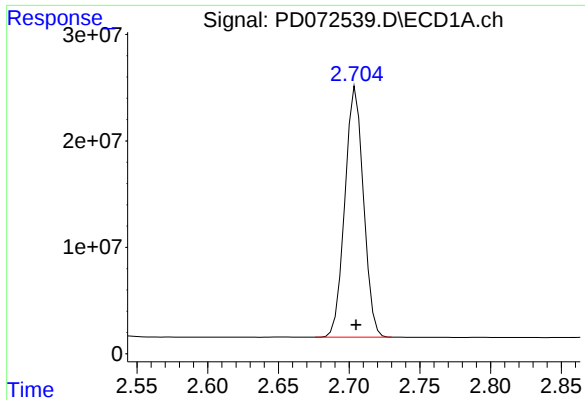

#1 Tetrachloro-m-xylene


R.T.: 2.705 min
Delta R.T.: 0.000 min
Response: 215881276
Conc: 73.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

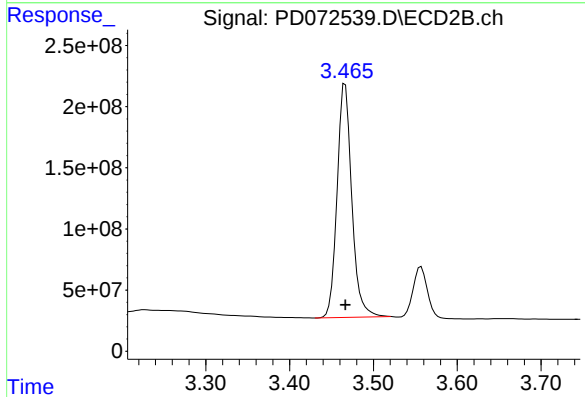


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 2325241888
Conc: 73.68 ng/ml

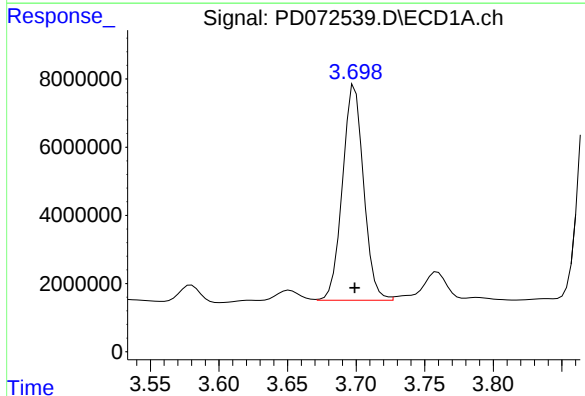


#23 Chlordane-1

R.T.: 3.699 min
Delta R.T.: 0.000 min
Response: 67715571
Conc: 736.04 ng/ml

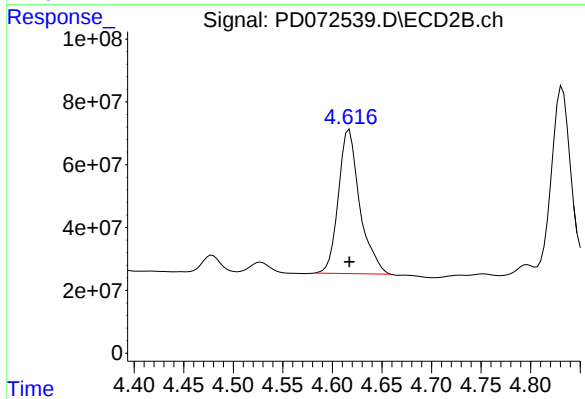

#23 Chlordane-1


R.T.: 4.617 min
Delta R.T.: 0.000 min
Response: 688110416
Conc: 731.74 ng/ml

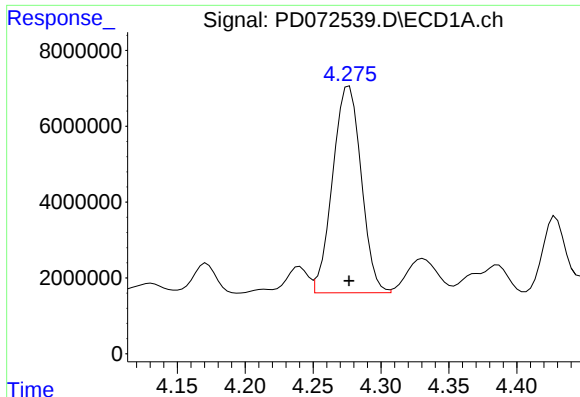

#24 Chlordane-2


R.T.: 4.277 min
Delta R.T.: 0.000 min
Response: 79921963
Conc: 738.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

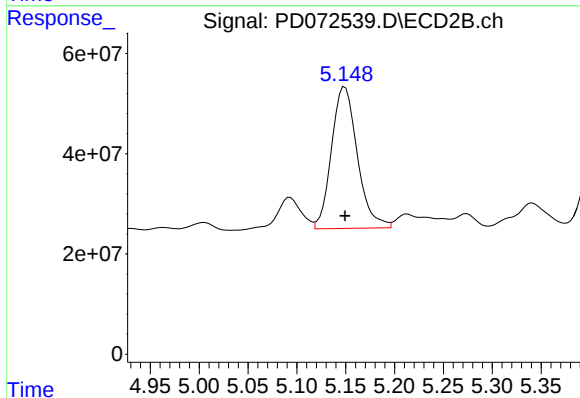


#24 Chlordane-2

R.T.: 5.149 min
Delta R.T.: 0.000 min
Response: 521215099
Conc: 734.26 ng/ml

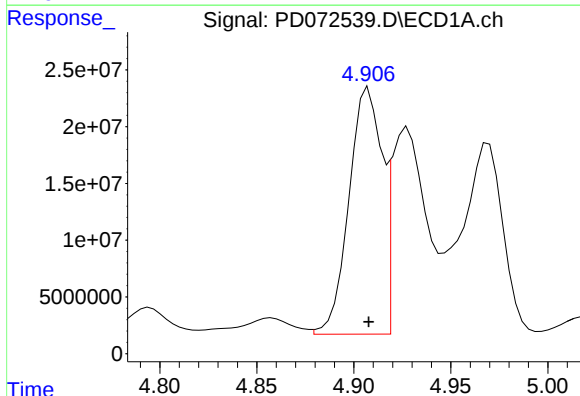


#25 Chlordane-3

R.T.: 4.908 min
Delta R.T.: 0.000 min
Response: 256455625
Conc: 743.90 ng/ml

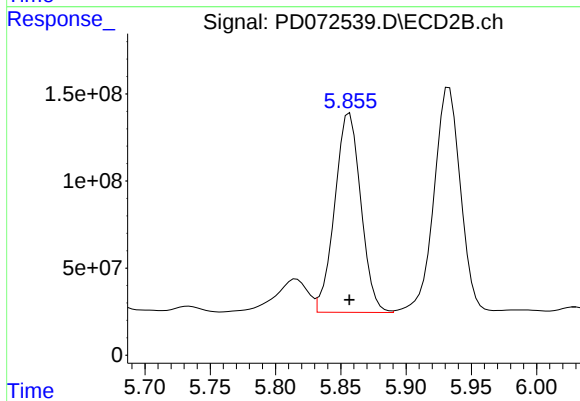

#25 Chlordane-3


R.T.: 5.857 min
Delta R.T.: 0.000 min
Response: 1595033235
Conc: 735.83 ng/ml

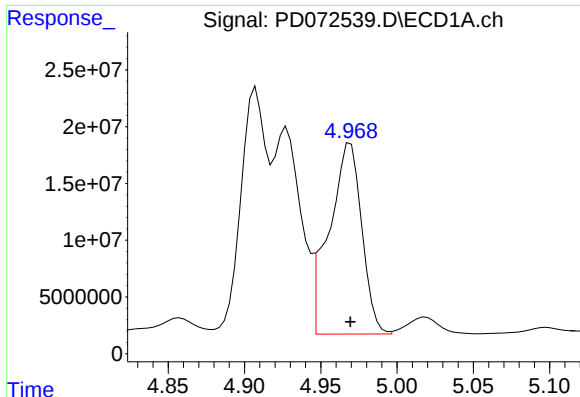

#26 Chlordane-4


R.T.: 4.970 min
Delta R.T.: 0.000 min
Response: 250070207
Conc: 737.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

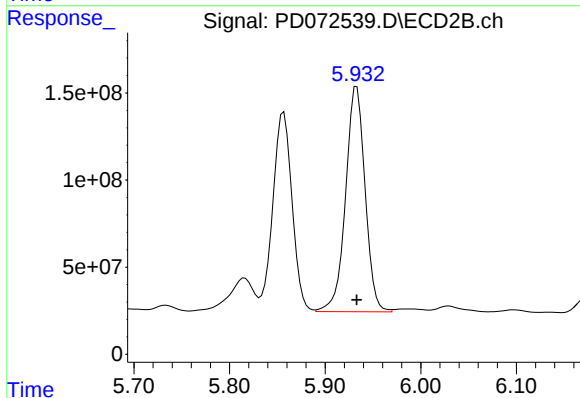


#26 Chlordane-4

R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 1838695276
Conc: 735.44 ng/ml

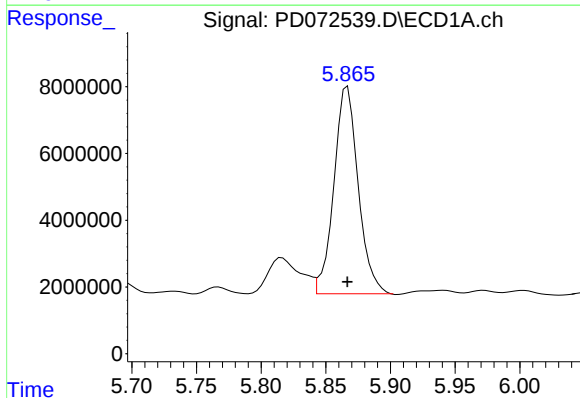


#27 Chlordane-5

R.T.: 5.867 min
Delta R.T.: 0.000 min
Response: 81086117
Conc: 736.17 ng/ml

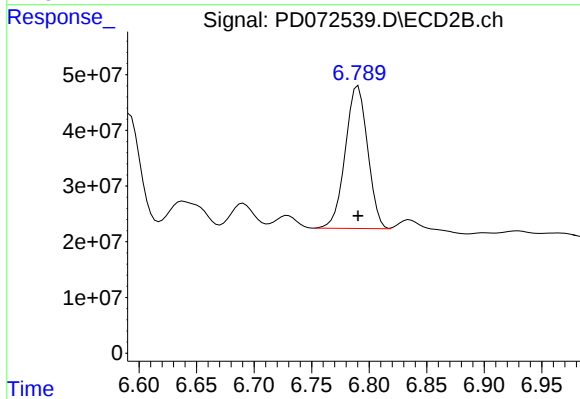

#27 Chlordane-5


R.T.: 6.790 min
Delta R.T.: 0.000 min
Response: 347608470
Conc: 736.51 ng/ml

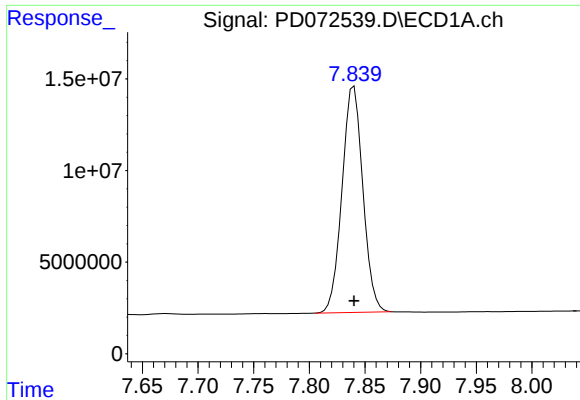

#28 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 160736636
Conc: 73.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

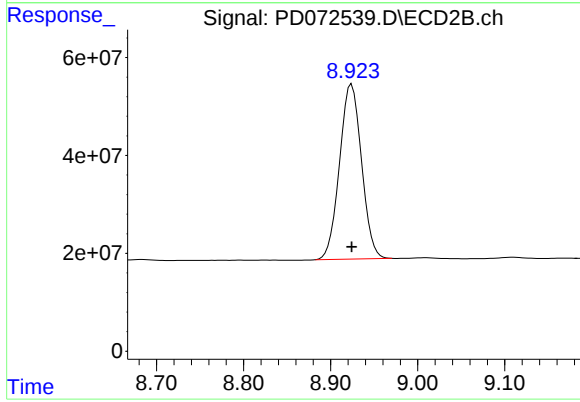

#28 Decachlorobiphenyl

R.T.: 8.924 min
Delta R.T.: 0.000 min
Response: 628464139
Conc: 73.59 ng/ml