

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102022\
 Data File : PD072540.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2022 19:34
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 00:54:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 00:51:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.705	3.466	150.1E6	1663.6E6	50.000	50.000
28)	SA Decachlor...	7.841	8.923	113.8E6	448.4E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	3.699	4.617	47451972	504.0E6	500.000	500.000
24)	Chlordane-2	4.276	5.149	57151612	382.7E6	500.000	500.000
25)	Chlordane-3	4.908	5.857	175.3E6	1135.4E6	500.000	500.000
26)	Chlordane-4	4.970	5.934	171.2E6	1312.0E6	500.000	500.000
27)	Chlordane-5	5.867	6.791	56532799	248.2E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102022\
Data File : PD072540.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2022 19:34
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 00:54:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 00:51:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

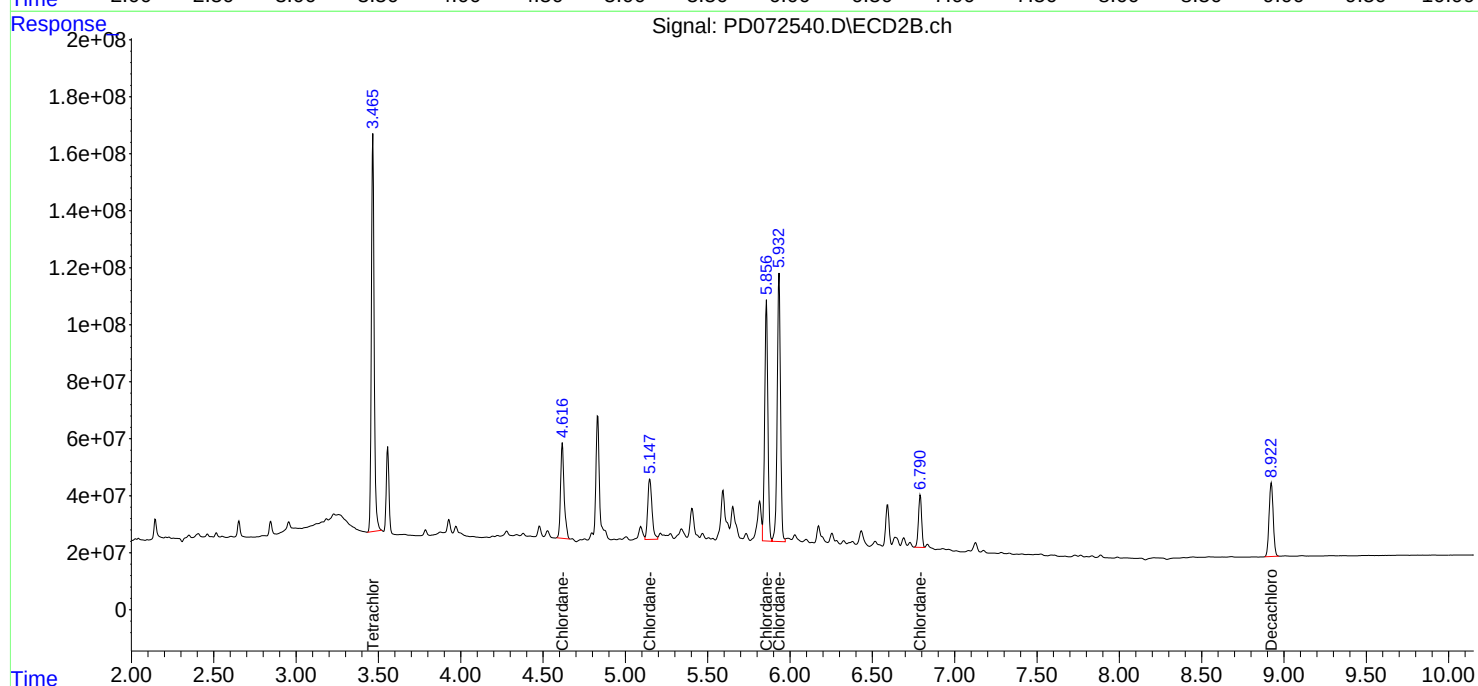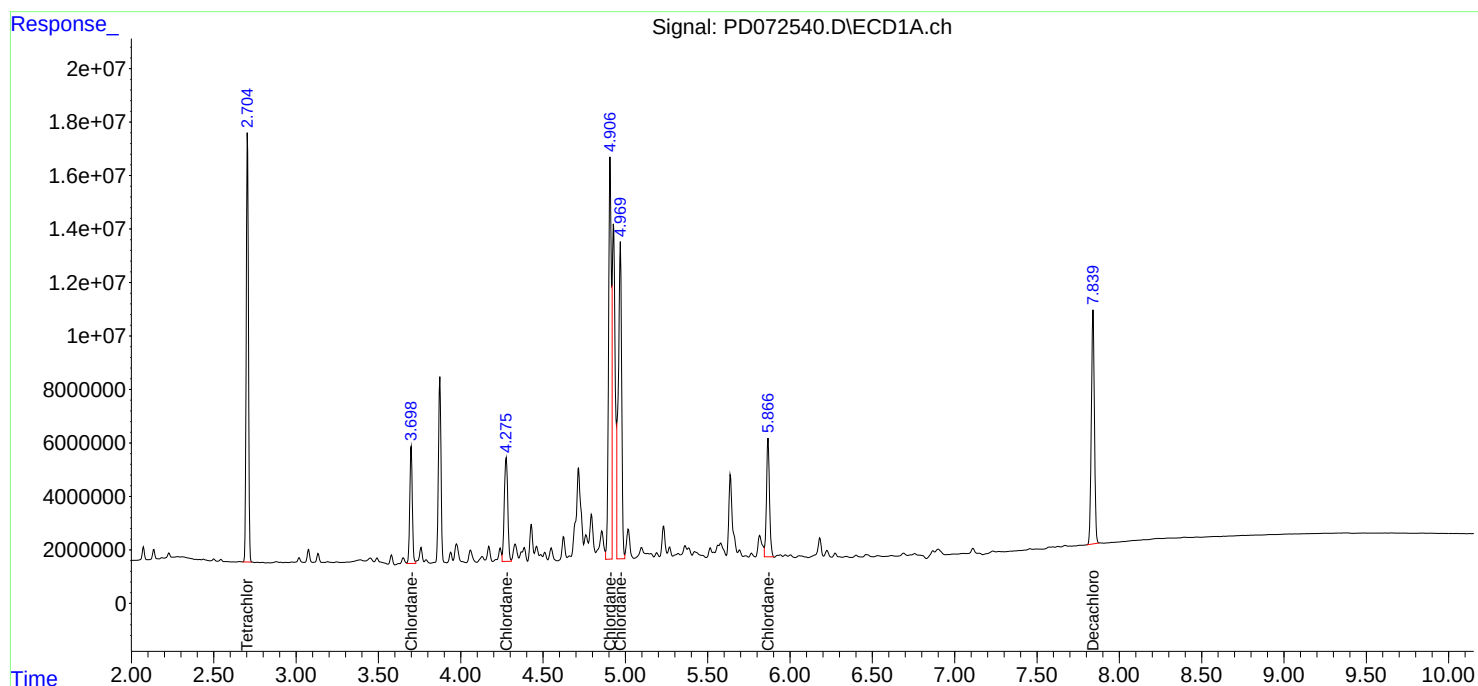


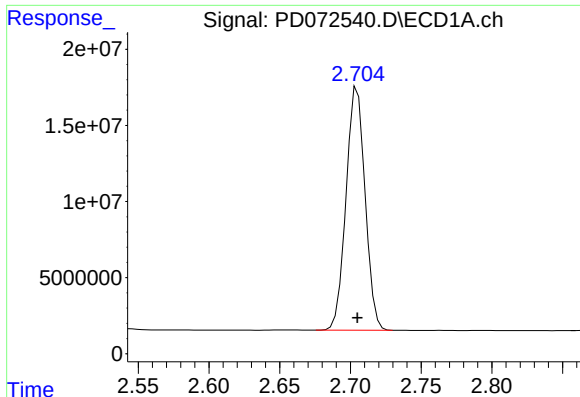

#1 Tetrachloro-m-xylene


R.T.: 2.705 min
Delta R.T.: 0.000 min
Response: 150076743
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

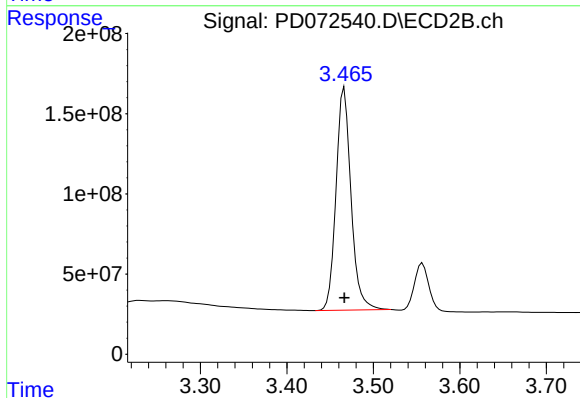


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 1663591721
Conc: 50.00 ng/ml

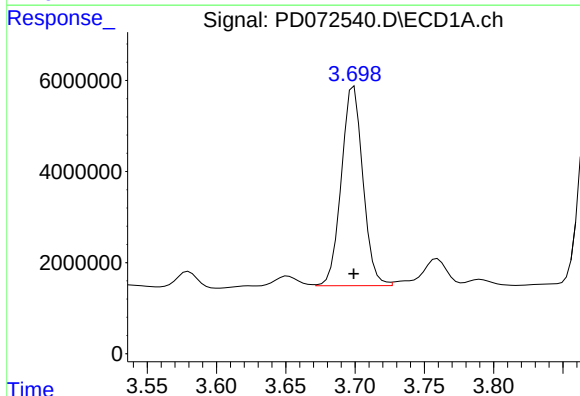


#23 Chlordane-1

R.T.: 3.699 min
Delta R.T.: 0.000 min
Response: 47451972
Conc: 500.00 ng/ml

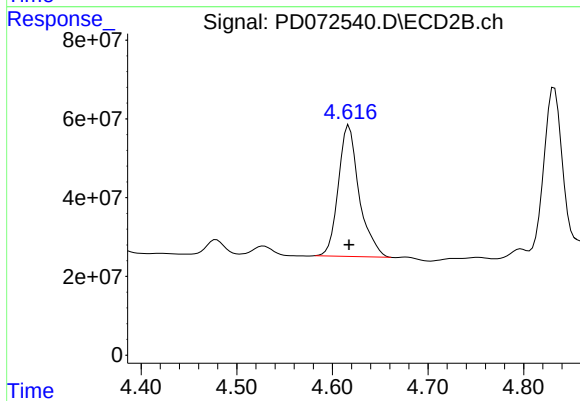

#23 Chlordane-1


R.T.: 4.617 min
Delta R.T.: 0.000 min
Response: 503983830
Conc: 500.00 ng/ml

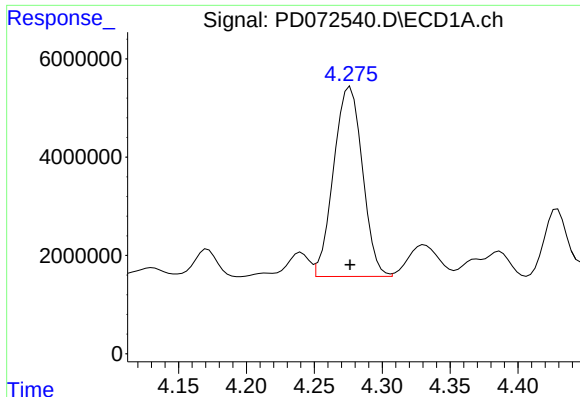

#24 Chlordane-2


R.T.: 4.276 min
Delta R.T.: 0.000 min
Response: 57151612
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

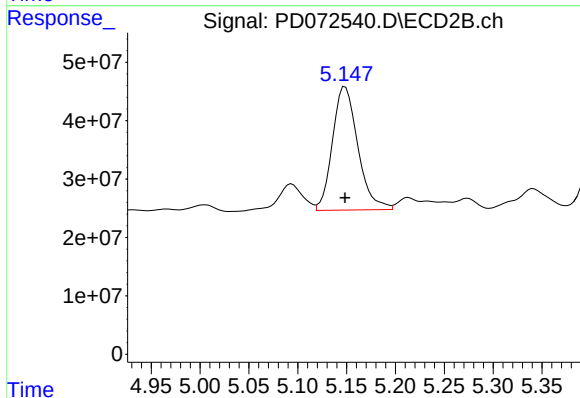


#24 Chlordane-2

R.T.: 5.149 min
Delta R.T.: 0.000 min
Response: 382697055
Conc: 500.00 ng/ml

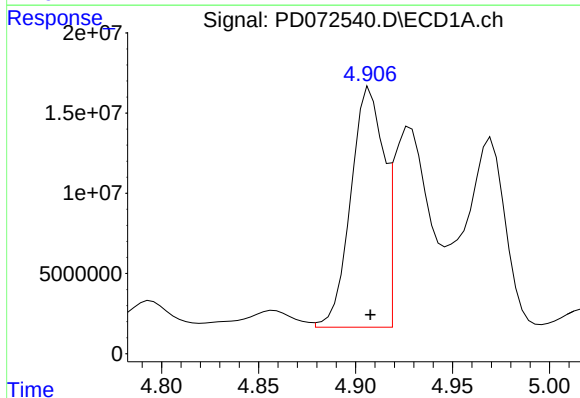


#25 Chlordane-3

R.T.: 4.908 min
Delta R.T.: 0.000 min
Response: 175265482
Conc: 500.00 ng/ml

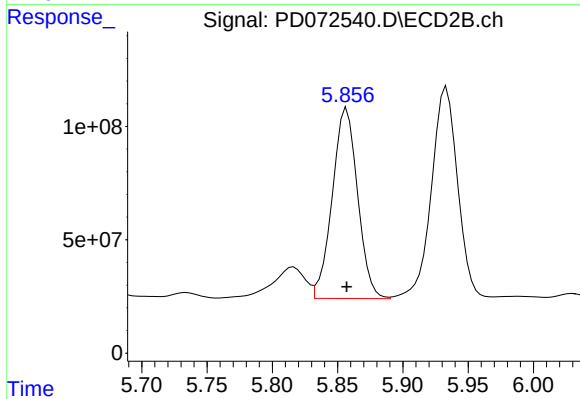

#25 Chlordane-3


R.T.: 5.857 min
Delta R.T.: 0.000 min
Response: 1135353767
Conc: 500.00 ng/ml

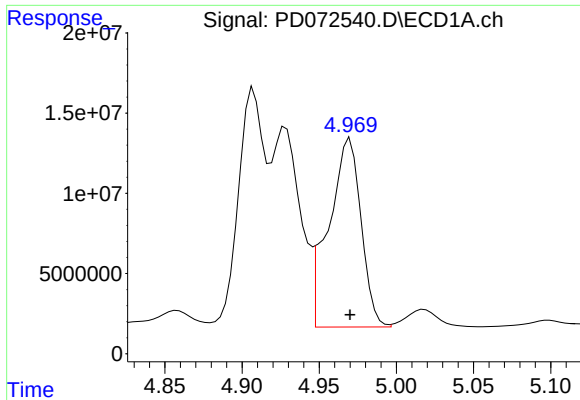

#26 Chlordane-4


R.T.: 4.970 min
Delta R.T.: 0.000 min
Response: 171188883
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

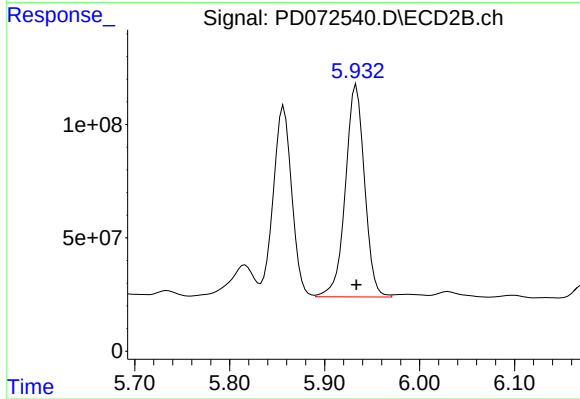


#26 Chlordane-4

R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 1311977682
Conc: 500.00 ng/ml

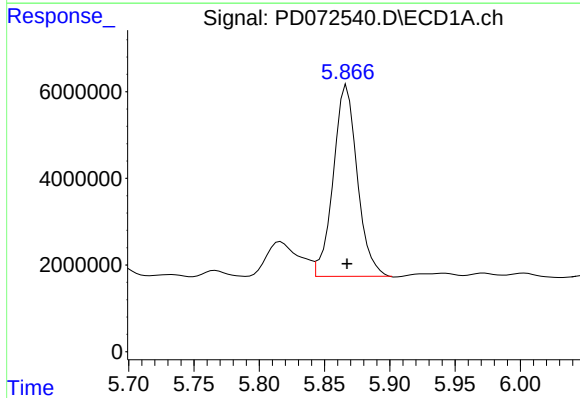


#27 Chlordane-5

R.T.: 5.867 min
Delta R.T.: 0.000 min
Response: 56532799
Conc: 500.00 ng/ml

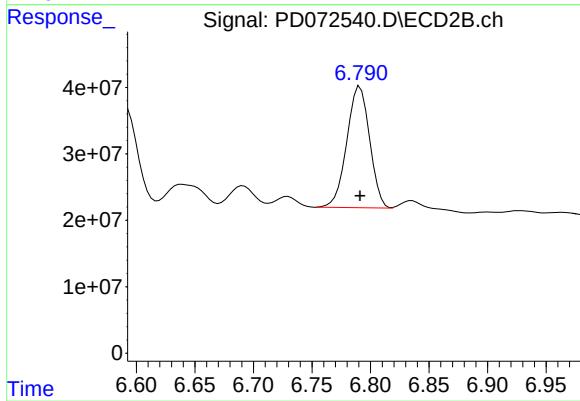

#27 Chlordane-5


R.T.: 6.791 min
Delta R.T.: 0.000 min
Response: 248177237
Conc: 500.00 ng/ml

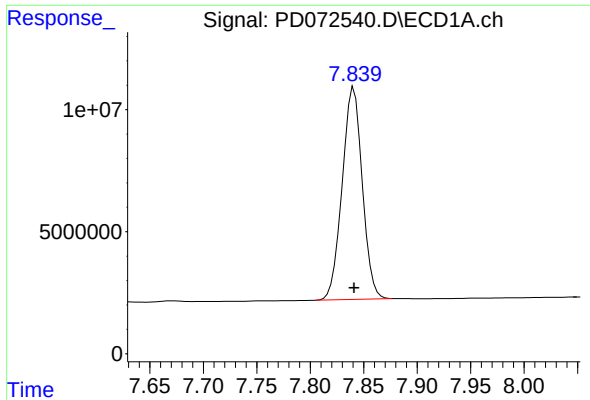

#28 Decachlorobiphenyl

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 113790771
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

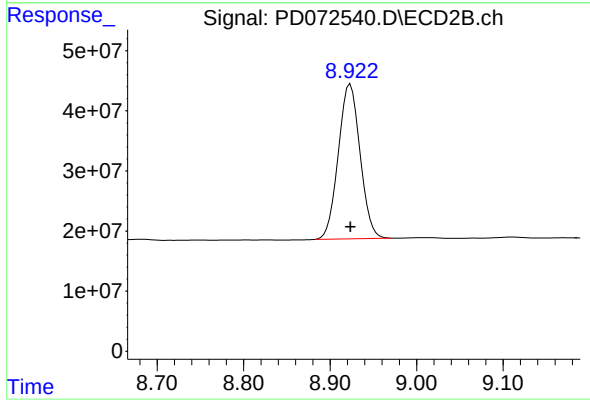

#28 Decachlorobiphenyl

R.T.: 8.923 min
Delta R.T.: 0.000 min
Response: 448382293
Conc: 50.00 ng/ml