

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102022\
 Data File : PD072541.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2022 19:47
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 01:04:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 01:03:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.705	3.466	71876582	857.4E6	24.678	26.592
28)	SA Decachlor...	7.840	8.924	58042406	231.2E6	26.166	26.523
Target Compounds							
23)	Chlordane-1	3.699	4.617	24230449	267.7E6	259.900	275.101
24)	Chlordane-2	4.277	5.149	30151085	209.5E6	270.814	282.368
25)	Chlordane-3	4.907	5.857	83234911	588.4E6	243.523	265.739
26)	Chlordane-4	4.970	5.934	83913407	682.1E6	247.987	266.727
27)	Chlordane-5	5.867	6.791	28396048	126.6E6	255.807	263.372



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102022\
Data File : PD072541.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2022 19:47
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 01:04:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 01:03:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

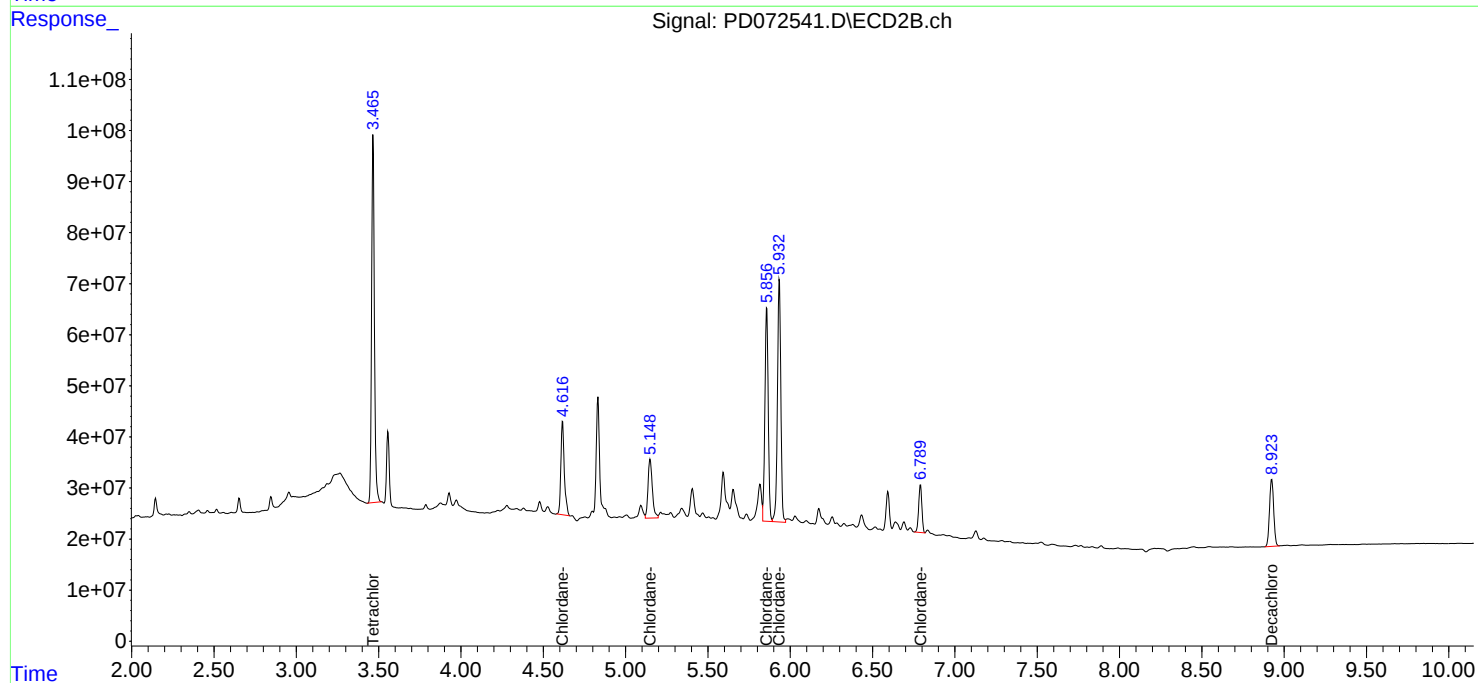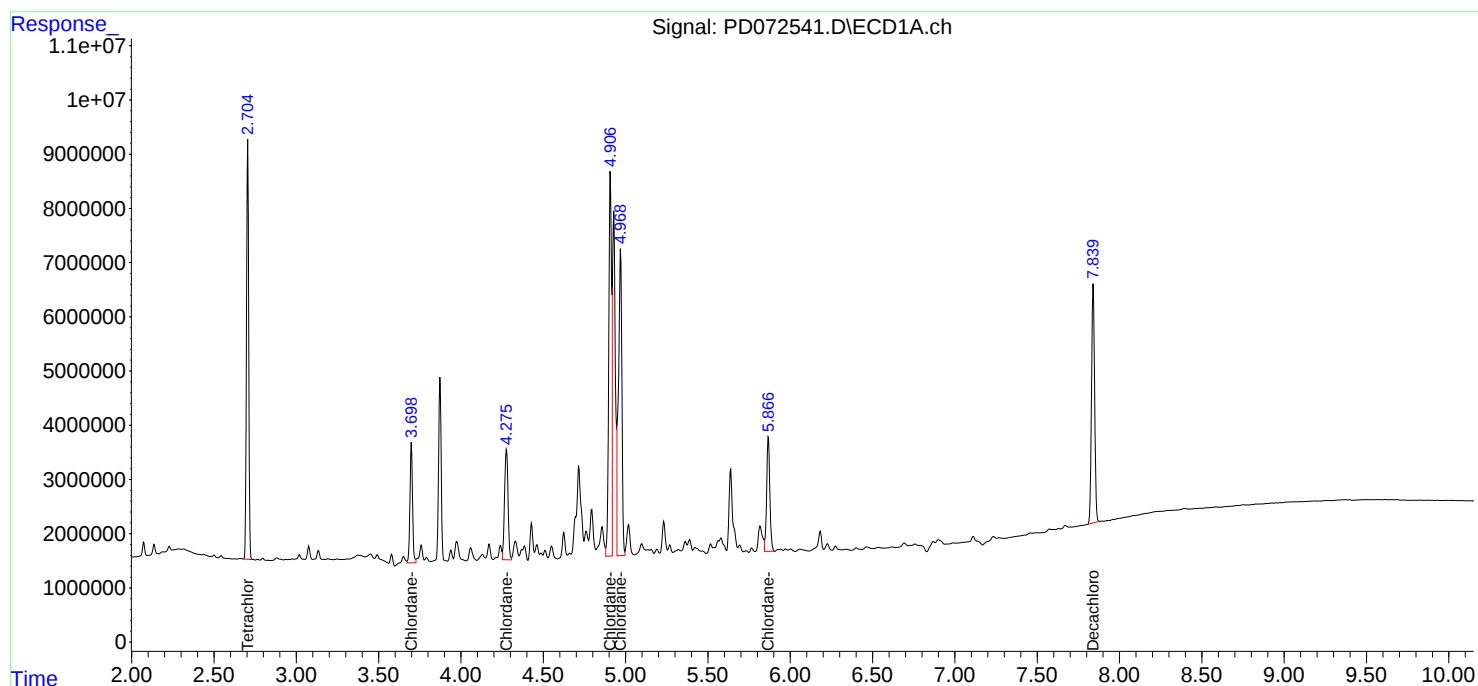


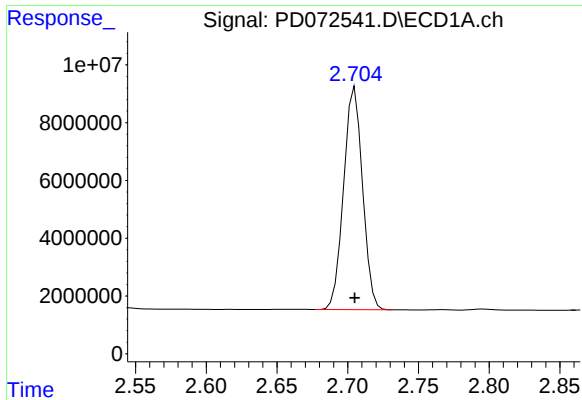

#1 Tetrachloro-m-xylene


R.T.: 2.705 min
Delta R.T.: 0.000 min
Response: 71876582
Conc: 24.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

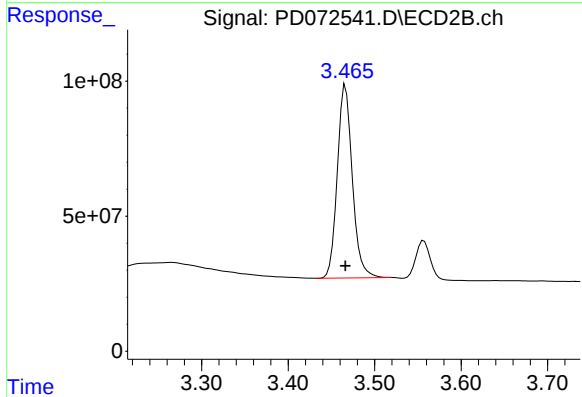


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 857383421
Conc: 26.59 ng/ml

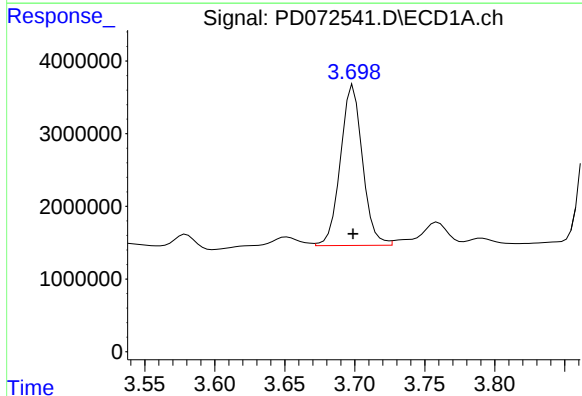


#23 Chlordane-1

R.T.: 3.699 min
Delta R.T.: 0.000 min
Response: 24230449
Conc: 259.90 ng/ml

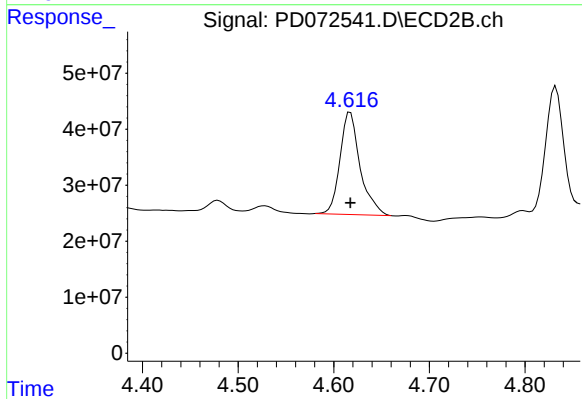

#23 Chlordane-1


R.T.: 4.617 min
Delta R.T.: 0.000 min
Response: 267655741
Conc: 275.10 ng/ml

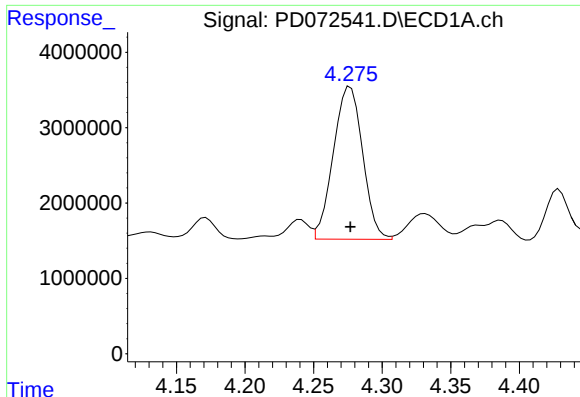

#24 Chlordane-2


R.T.: 4.277 min
Delta R.T.: 0.000 min
Response: 30151085
Conc: 270.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

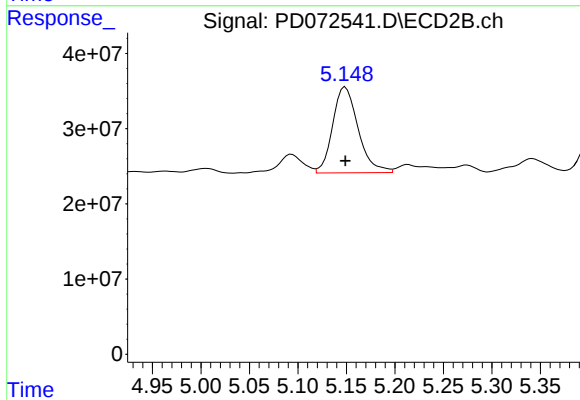


#24 Chlordane-2

R.T.: 5.149 min
Delta R.T.: 0.000 min
Response: 209480218
Conc: 282.37 ng/ml

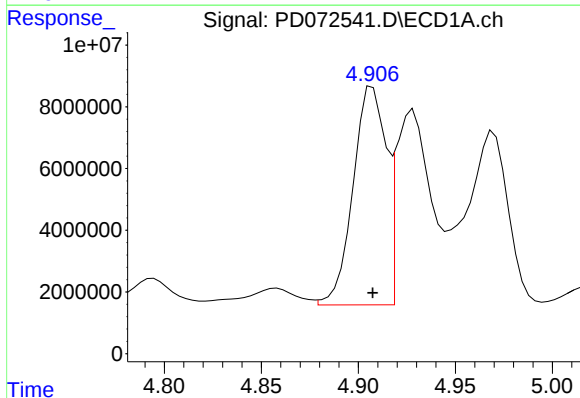


#25 Chlordane-3

R.T.: 4.907 min
Delta R.T.: 0.000 min
Response: 83234911
Conc: 243.52 ng/ml

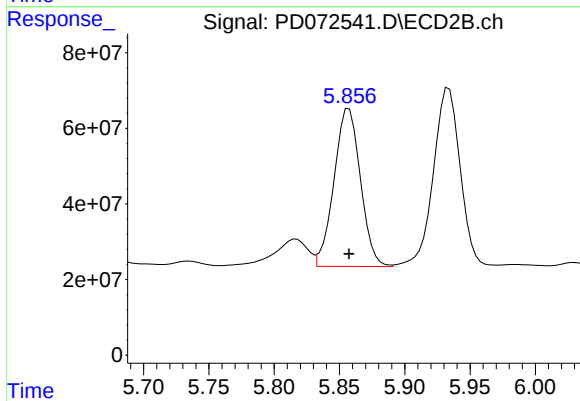

#25 Chlordane-3


R.T.: 5.857 min
Delta R.T.: 0.000 min
Response: 588379313
Conc: 265.74 ng/ml

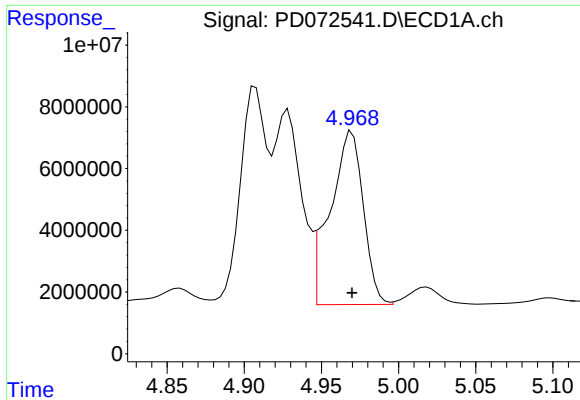

#26 Chlordane-4


R.T.: 4.970 min
Delta R.T.: 0.000 min
Response: 83913407
Conc: 247.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

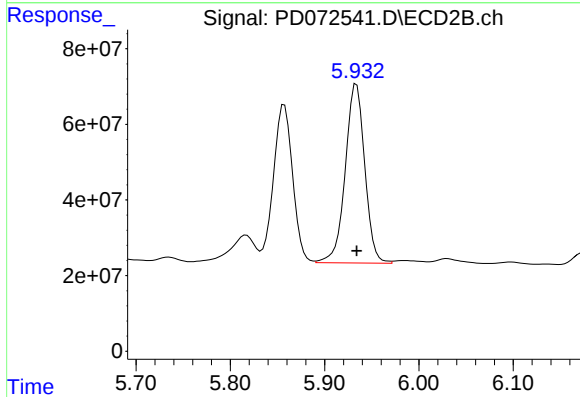


#26 Chlordane-4

R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 682062255
Conc: 266.73 ng/ml

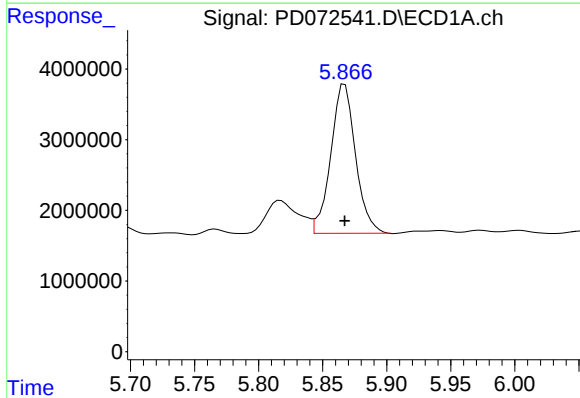


#27 Chlordane-5

R.T.: 5.867 min
Delta R.T.: 0.000 min
Response: 28396048
Conc: 255.81 ng/ml

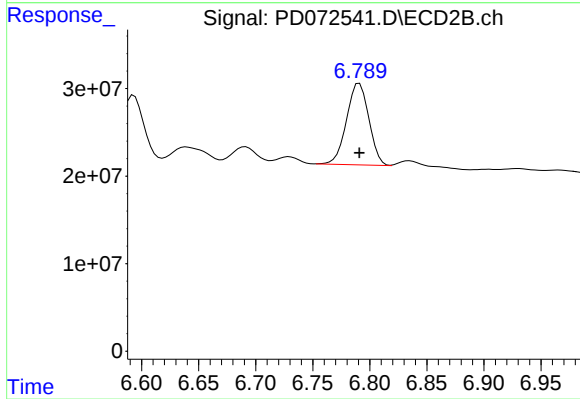

#27 Chlordane-5

R.T.: 6.791 min
Delta R.T.: 0.000 min
Response: 126558961
Conc: 263.37 ng/ml

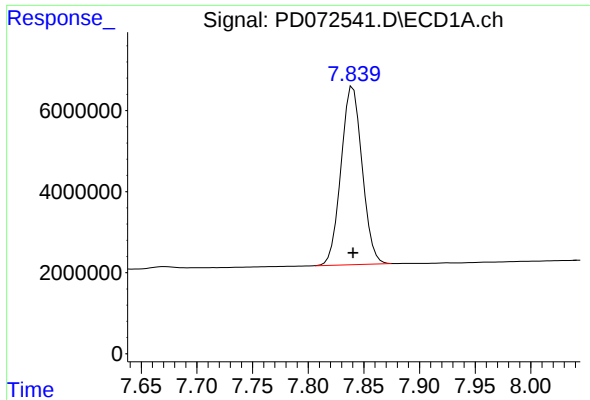

#28 Decachlorobiphenyl


R.T.: 7.840 min

Delta R.T.: 0.000 min

Response: 58042406

Conc: 26.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

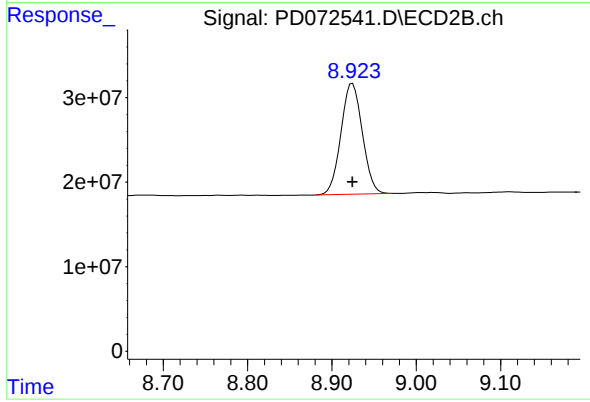

#28 Decachlorobiphenyl

R.T.: 8.924 min

Delta R.T.: 0.000 min

Response: 231204240

Conc: 26.52 ng/ml