

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102023\
 Data File : PD078995.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2023 19:41
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 02:01:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 01:59:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	110.0E6	190.1E6	75.313	75.612
28)	SA Decachlor...	9.115	7.955	129.8E6	163.5E6	73.916	72.822
Target Compounds							
23)	Chlordane-1	4.737	3.809	55832656	63176482	750.492	744.316
24)	Chlordane-2	5.267	4.386	54944543	62909768	725.848	718.964
25)	Chlordane-3	5.977	5.017	228.0E6	199.2E6	759.068	758.206
26)	Chlordane-4	6.060	5.081	270.0E6	176.8E6	755.945	738.205
27)	Chlordane-5	6.912	5.976	49757779	72520705	739.720	743.107



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102023\
Data File : PD078995.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2023 19:41
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 02:01:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 01:59:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

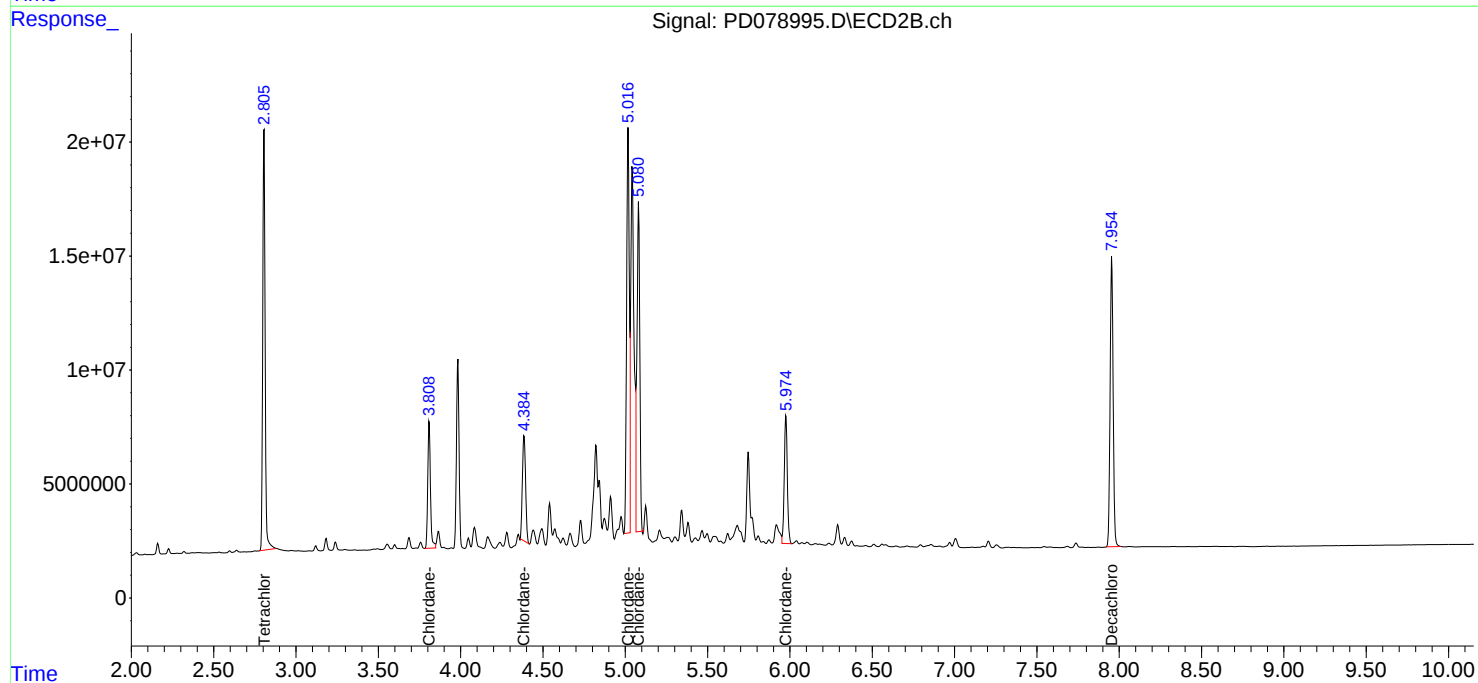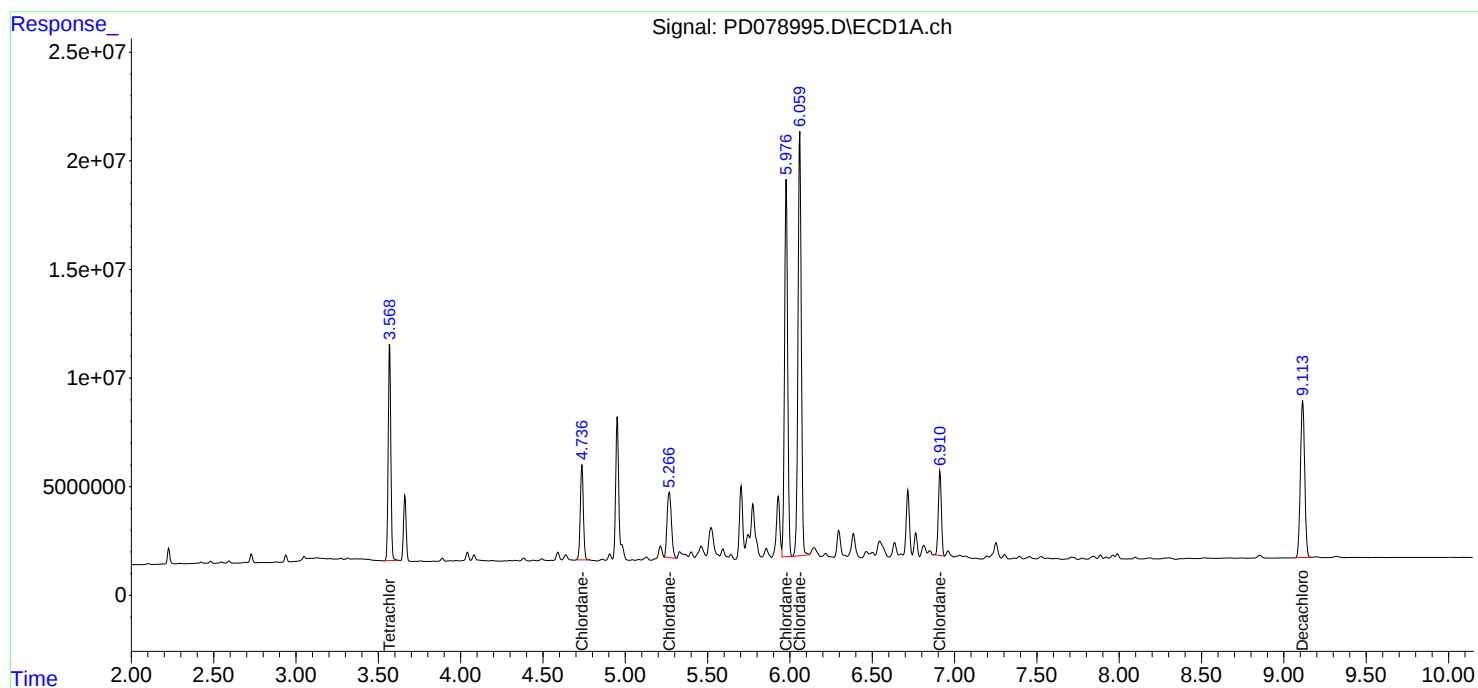


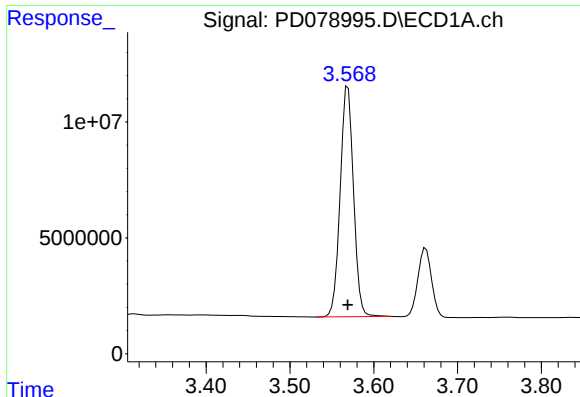

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 110033452
Conc: 75.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

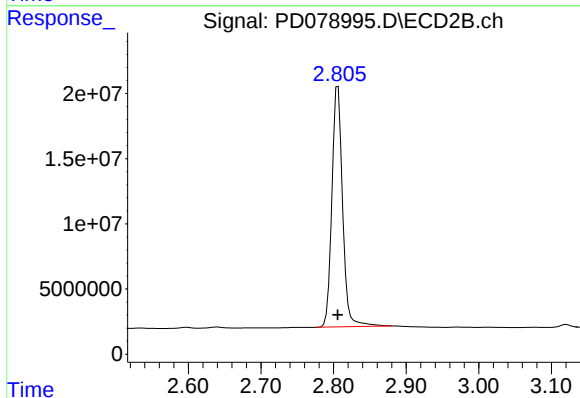


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 190104772
Conc: 75.61 ng/ml

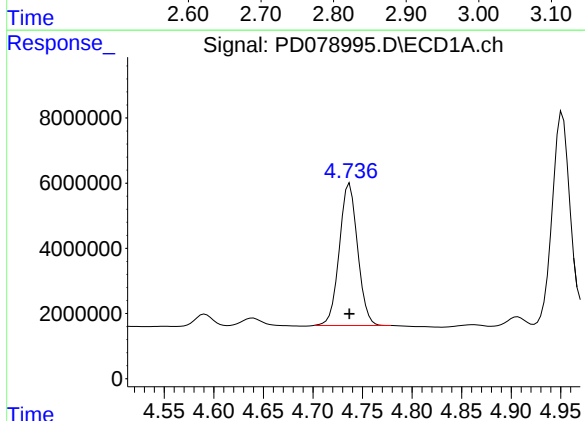


#23 Chlordane-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 55832656
Conc: 750.49 ng/ml

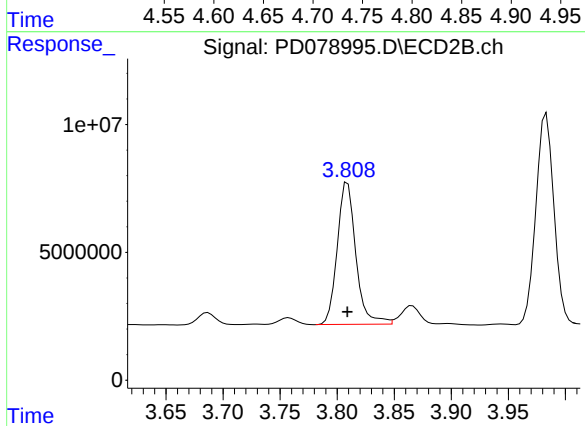

#23 Chlordane-1


R.T.: 3.809 min
Delta R.T.: 0.000 min
Response: 63176482
Conc: 744.32 ng/ml

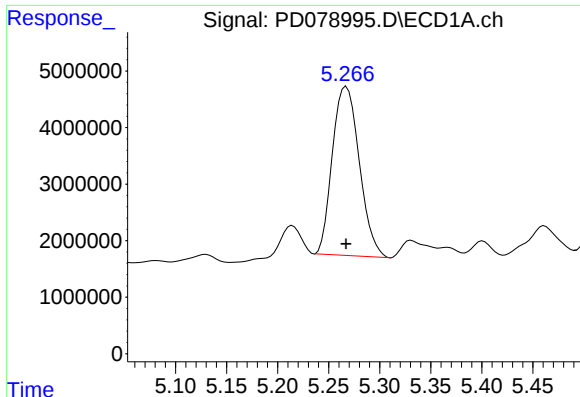

#24 Chlordane-2


R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 54944543
Conc: 725.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

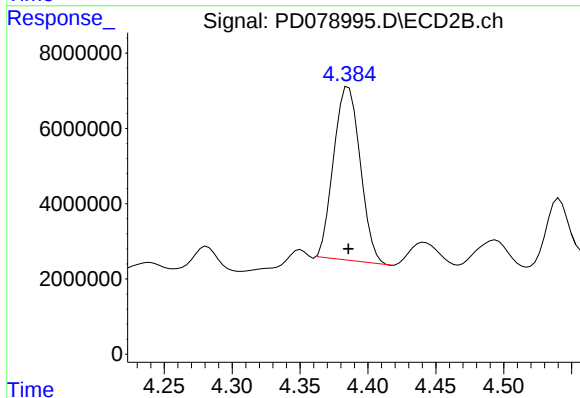


#24 Chlordane-2

R.T.: 4.386 min
Delta R.T.: 0.000 min
Response: 62909768
Conc: 718.96 ng/ml

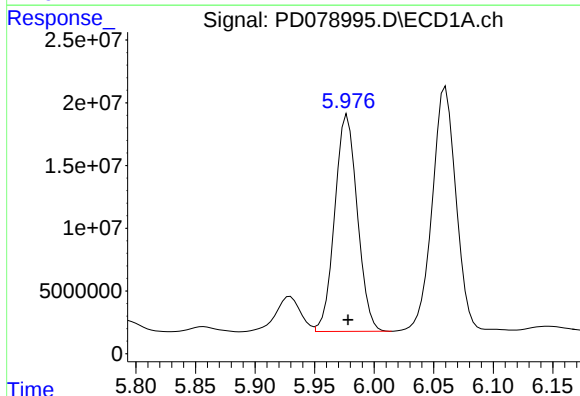


#25 Chlordane-3

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 227967007
Conc: 759.07 ng/ml

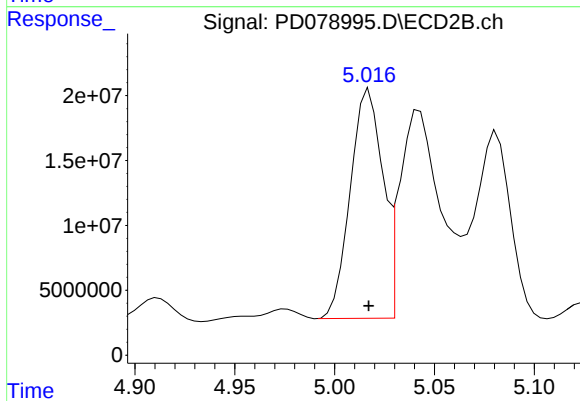

#25 Chlordane-3


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 199238052
Conc: 758.21 ng/ml

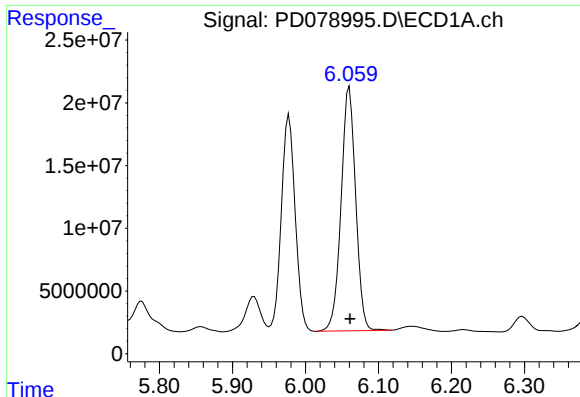

#26 Chlordane-4


R.T.: 6.060 min
Delta R.T.: 0.000 min
Response: 270018863
Conc: 755.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

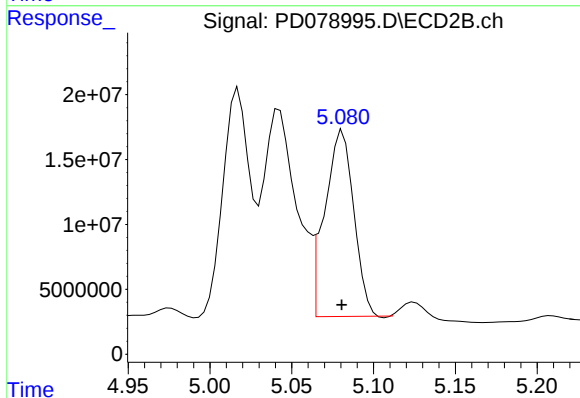


#26 Chlordane-4

R.T.: 5.081 min
Delta R.T.: 0.000 min
Response: 176826478
Conc: 738.20 ng/ml

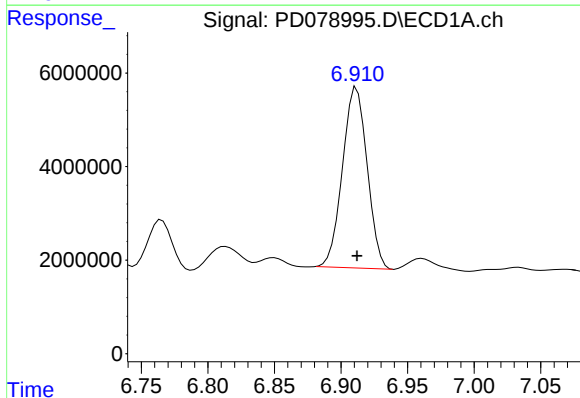


#27 Chlordane-5

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 49757779
Conc: 739.72 ng/ml

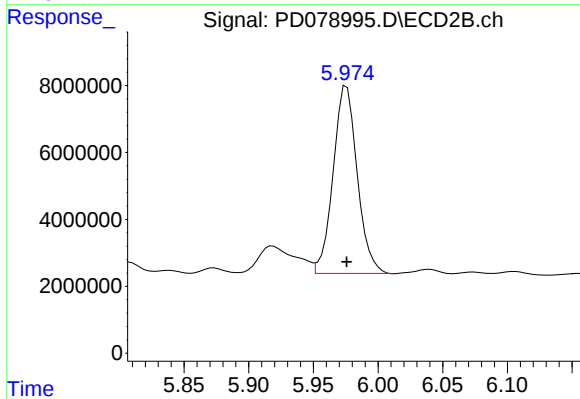

#27 Chlordane-5


R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 72520705
Conc: 743.11 ng/ml

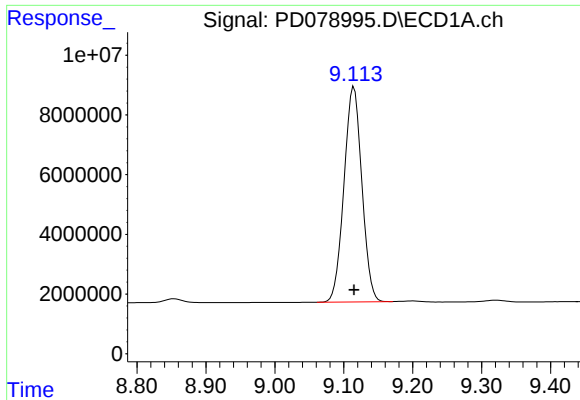

#28 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.000 min
Response: 129822607
Conc: 73.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

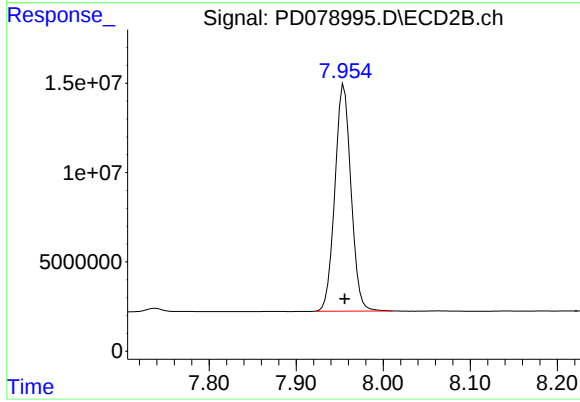

#28 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: 0.000 min
Response: 163469104
Conc: 72.82 ng/ml