

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102023\
 Data File : PD078988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2023 18:08
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 04:46:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.807	29278399	40629254	18.134	17.548
28)	SA Decachlor...	9.116	7.956	37889761	44313225	18.888	18.180
Target Compounds							
9)	A Endosulfan I	6.109	5.137	20471541	23863042	9.443	9.013
10)	B gamma-Chl...	5.978	5.016	21870067	26463831	9.539	9.223
12)	B 4,4'-DDE	6.228	5.270	38029392	47690008	17.997	17.912
13)	MA Dieldrin	6.384	5.401	41189243	51885830	17.687	17.471
19)	B Endosulfa...	7.196	6.371	35938721	42517978	18.077	18.210
20)	A Methoxychlor	7.534	6.651	88577993	114.7E6	80.836	84.483
21)	B Endrin ke...	7.683	6.878	39928591	49606882	18.314	17.744



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102023\
Data File : PD078988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2023 18:08
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 04:46:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

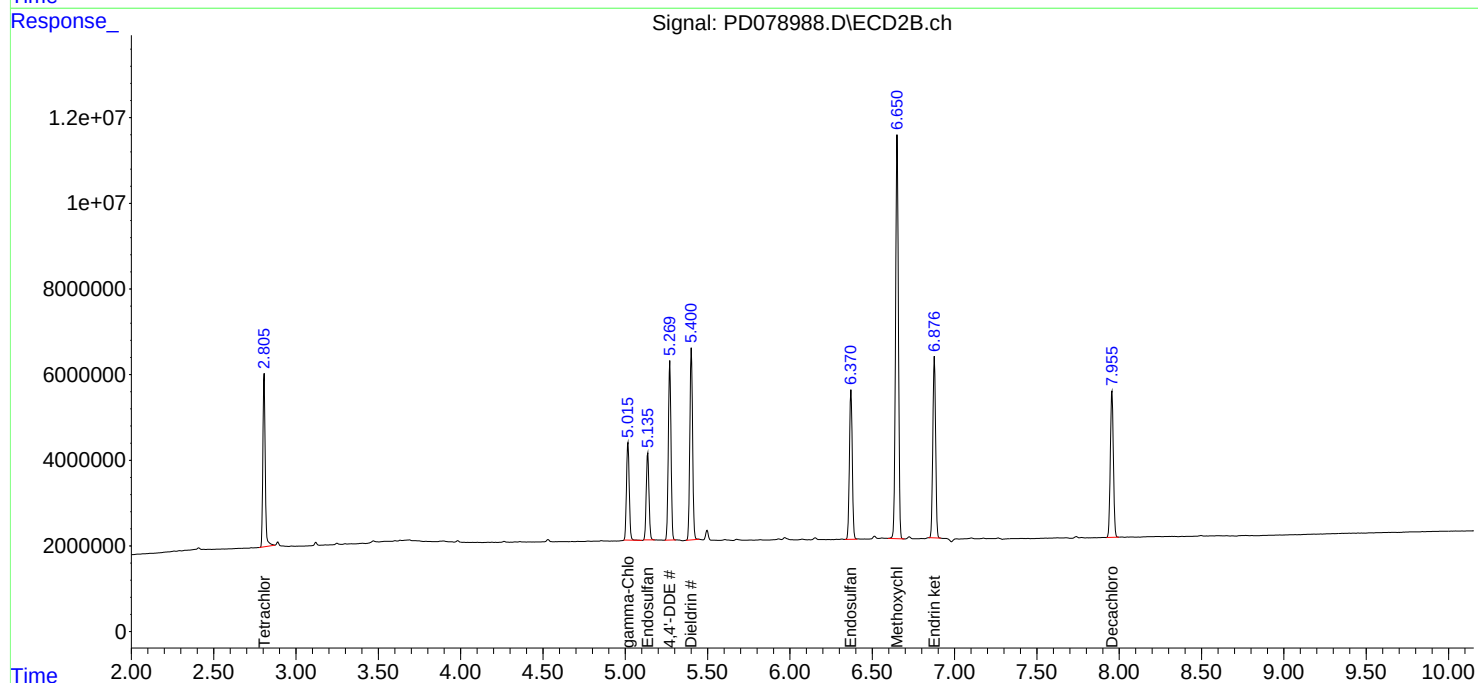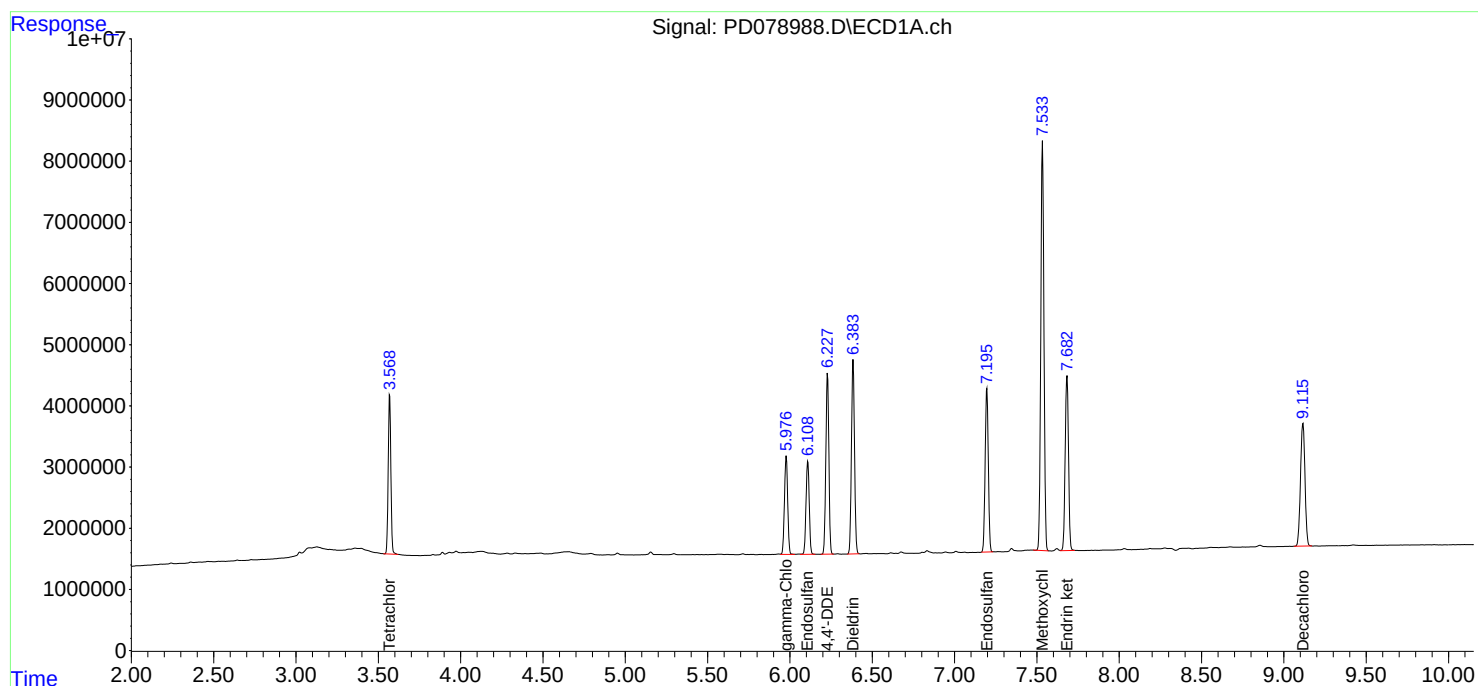


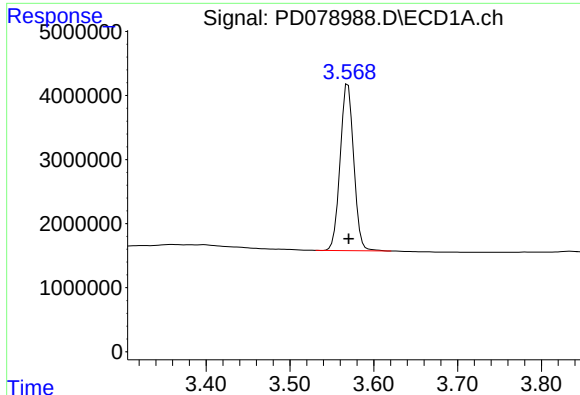

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 29278399
Conc: 18.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

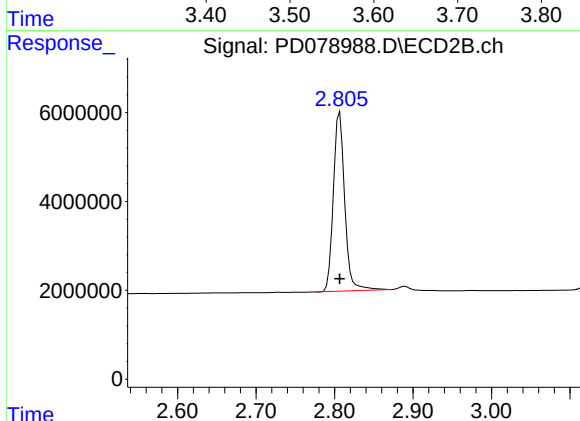


#1 Tetrachloro-m-xylene

R.T.: 2.807 min
Delta R.T.: 0.000 min
Response: 40629254
Conc: 17.55 ng/ml

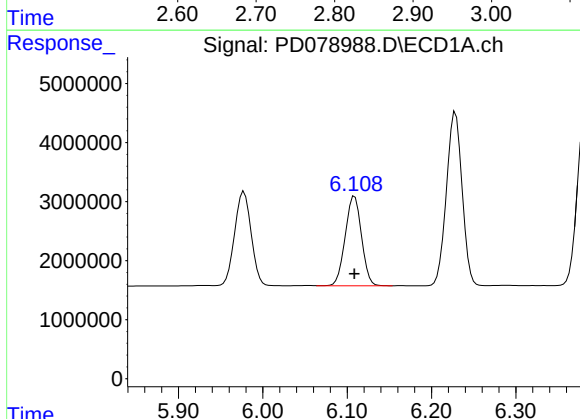


#9 Endosulfan I

R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 20471541
Conc: 9.44 ng/ml

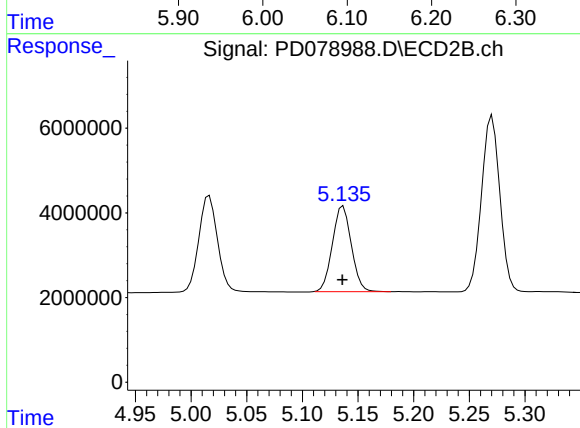

#9 Endosulfan I


R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 23863042
Conc: 9.01 ng/ml

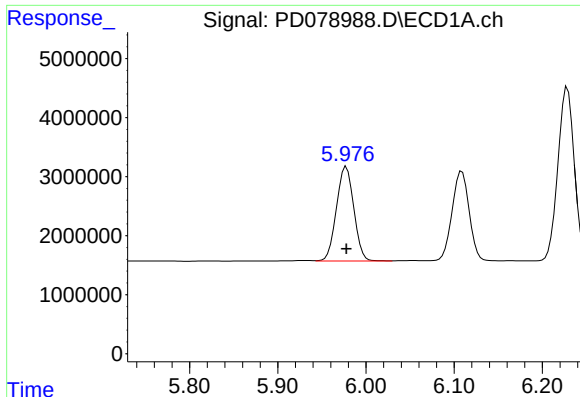

#10 gamma-Chlordane


R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 21870067
Conc: 9.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

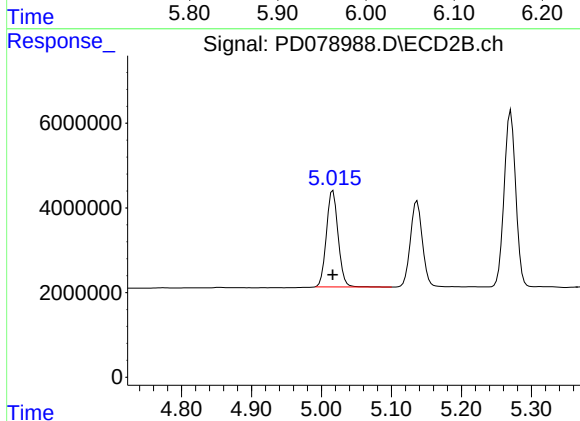


#10 gamma-Chlordane

R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 26463831
Conc: 9.22 ng/ml

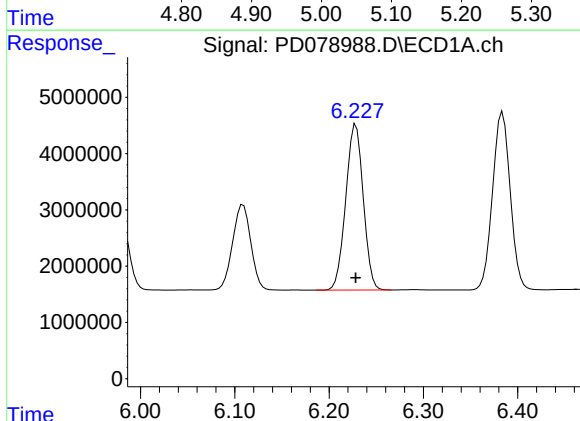


#12 4,4'-DDE

R.T.: 6.228 min
Delta R.T.: 0.000 min
Response: 38029392
Conc: 18.00 ng/ml

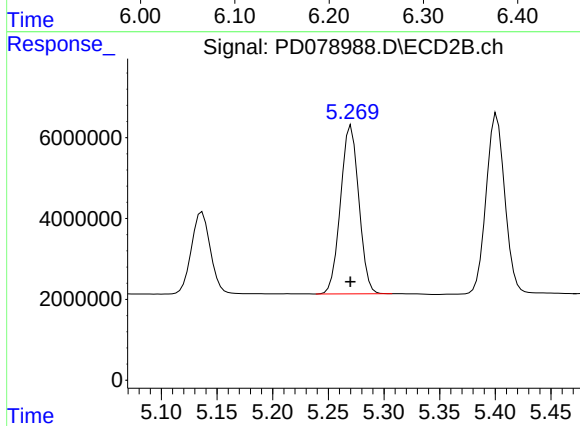

#12 4,4'-DDE


R.T.: 5.270 min
Delta R.T.: 0.000 min
Response: 47690008
Conc: 17.91 ng/ml

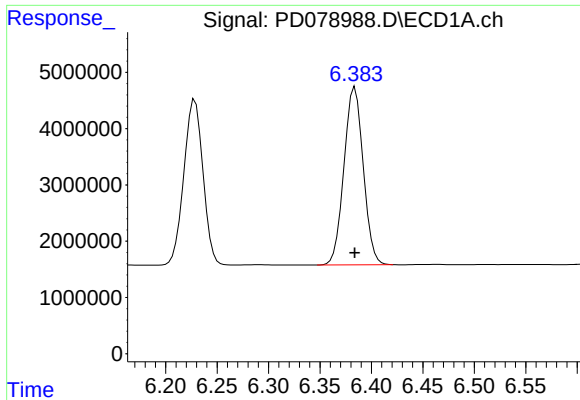

#13 Dieldrin


R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 41189243
Conc: 17.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

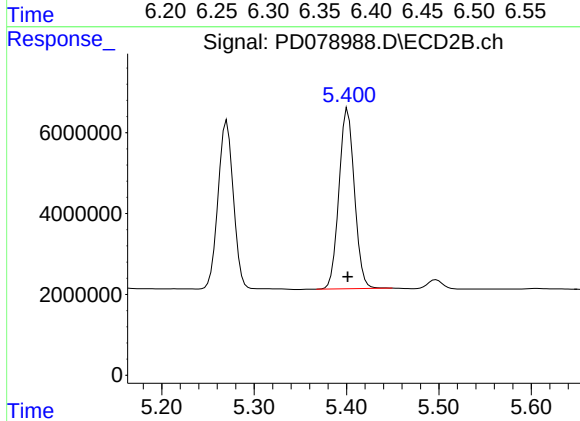


#13 Dieldrin

R.T.: 5.401 min
Delta R.T.: 0.000 min
Response: 51885830
Conc: 17.47 ng/ml

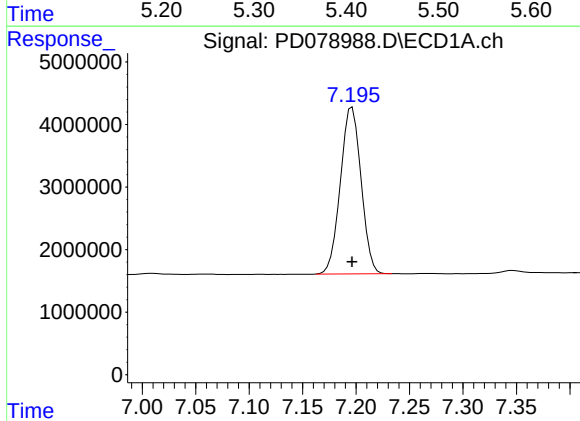


#19 Endosulfan Sulfate

R.T.: 7.196 min
Delta R.T.: 0.000 min
Response: 35938721
Conc: 18.08 ng/ml

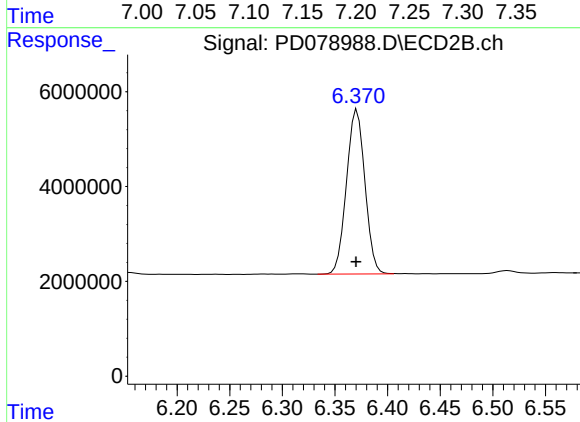

#19 Endosulfan Sulfate


R.T.: 6.371 min
Delta R.T.: 0.001 min
Response: 42517978
Conc: 18.21 ng/ml

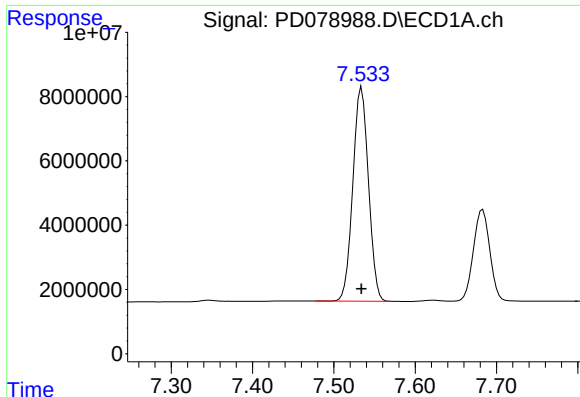

#20 Methoxychlor


R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 88577993
Conc: 80.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

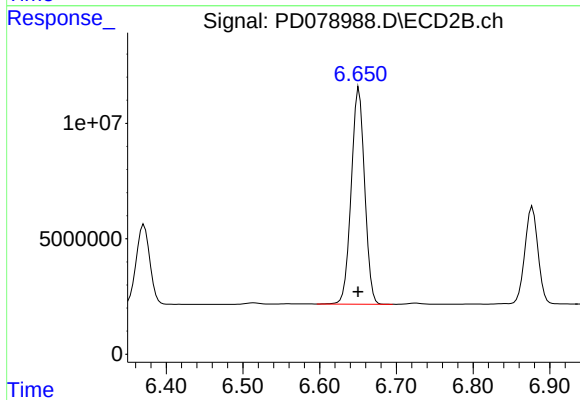


#20 Methoxychlor

R.T.: 6.651 min
Delta R.T.: 0.001 min
Response: 114696456
Conc: 84.48 ng/ml

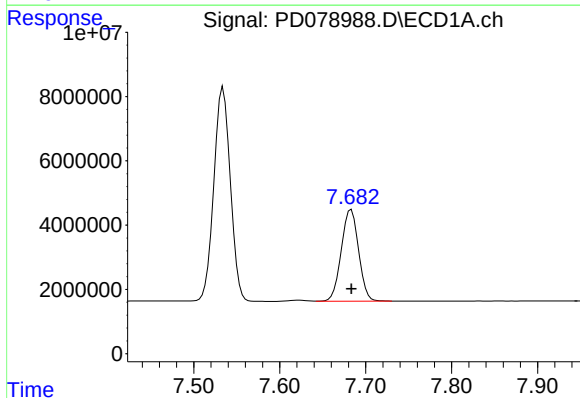


#21 Endrin ketone

R.T.: 7.683 min
Delta R.T.: 0.000 min
Response: 39928591
Conc: 18.31 ng/ml

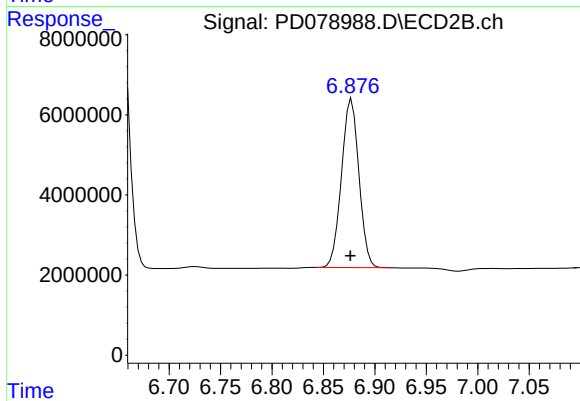

#21 Endrin ketone


R.T.: 6.878 min
Delta R.T.: 0.001 min
Response: 49606882
Conc: 17.74 ng/ml

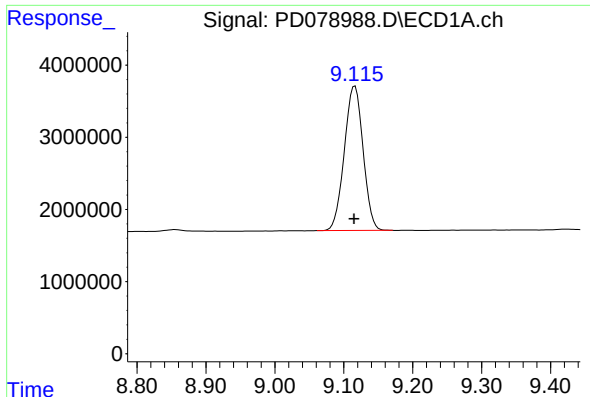

#28 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: 0.001 min
Response: 37889761
Conc: 18.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

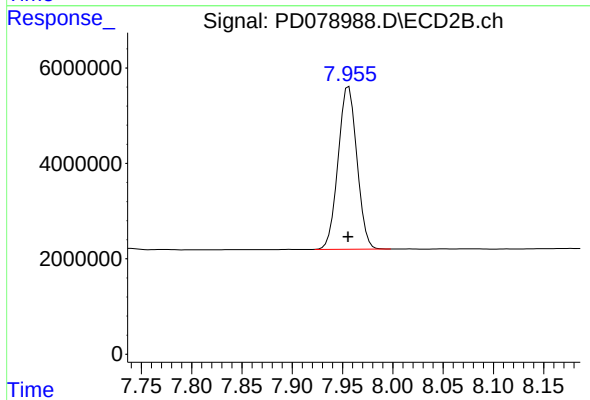

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 44313225
Conc: 18.18 ng/ml