

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102023\
 Data File : PD078995.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2023 19:41
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 02:05:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 02:05:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	110.0E6	190.1E6	75.344	75.407
28)	SA Decachlor...	9.115	7.955	129.8E6	163.5E6	75.507	74.566
Target Compounds							
23)	Chlordane-1	4.737	3.809	55832656	63176482	748.080	749.343
24)	Chlordane-2	5.267	4.386	54944543	62909768	748.882	744.165
25)	Chlordane-3	5.977	5.017	228.0E6	199.2E6	751.200	753.830
26)	Chlordane-4	6.060	5.081	270.0E6	176.8E6	752.182	735.618
27)	Chlordane-5	6.912	5.976	49757779	72520705	748.116	749.268



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102023\
Data File : PD078995.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2023 19:41
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 02:05:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 02:05:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

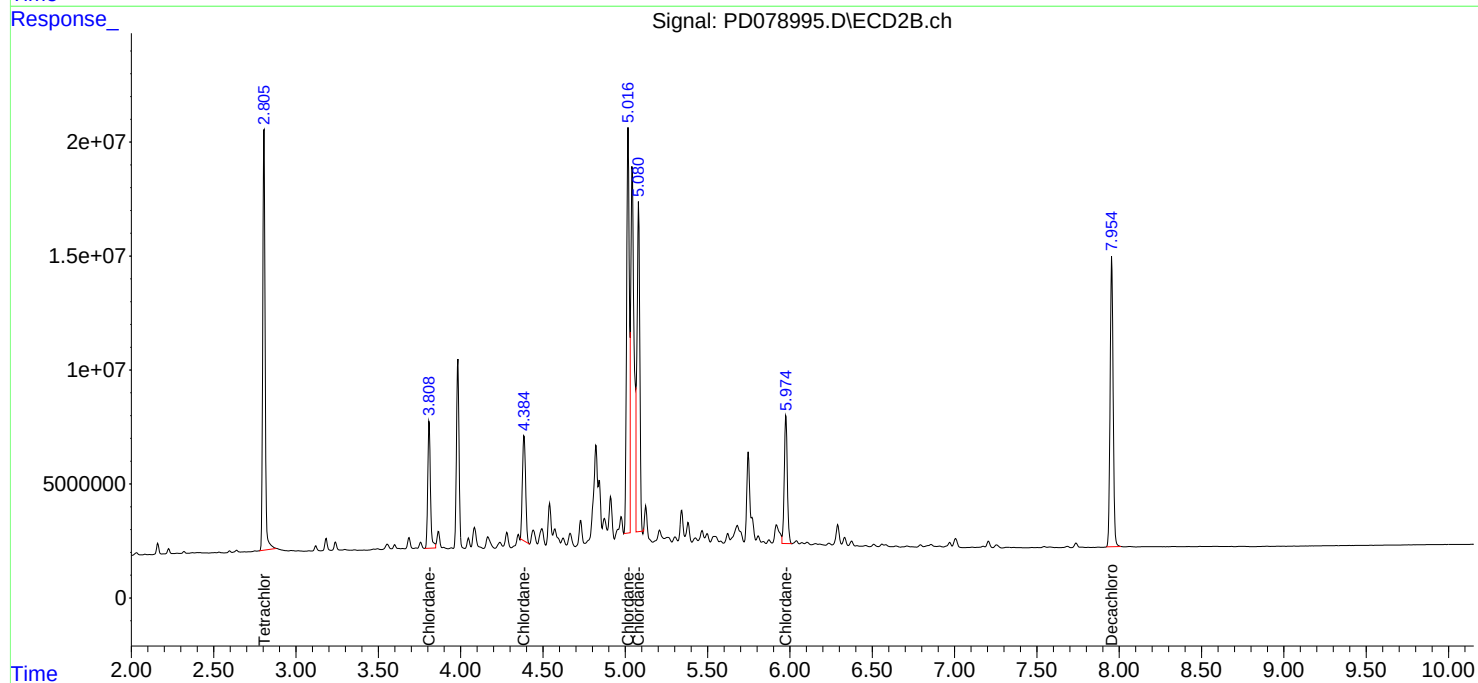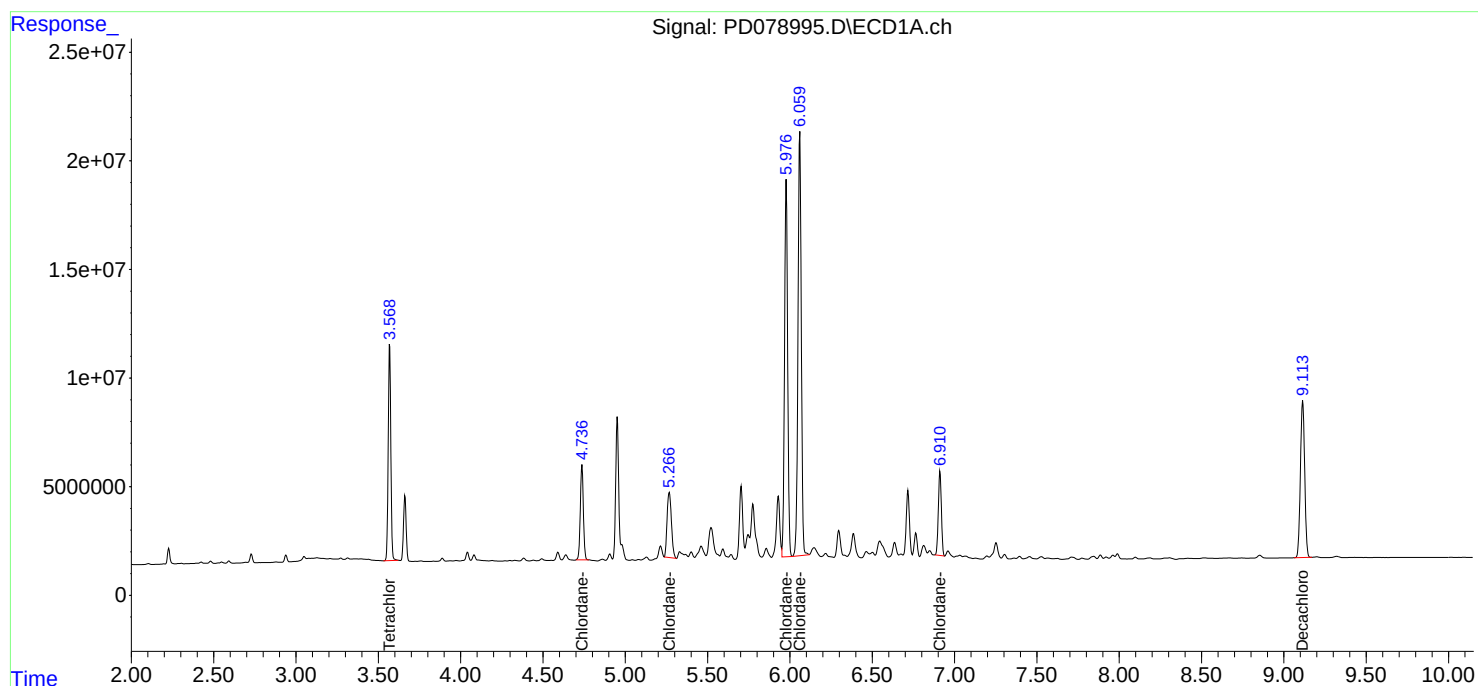


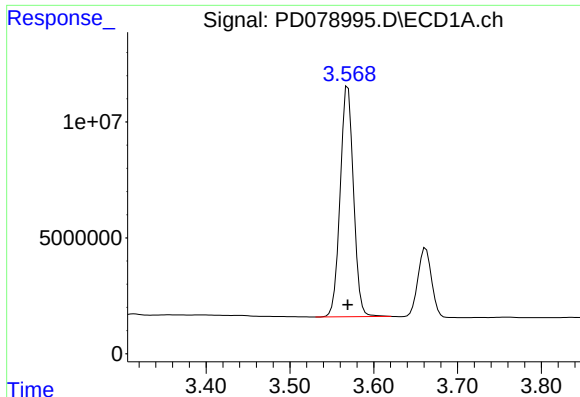

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 110033452
Conc: 75.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

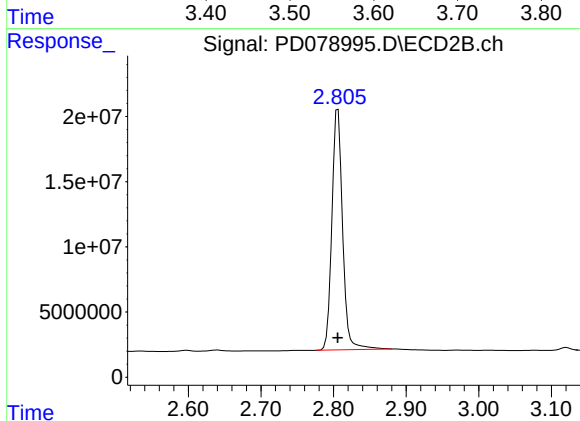


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 190104772
Conc: 75.41 ng/ml

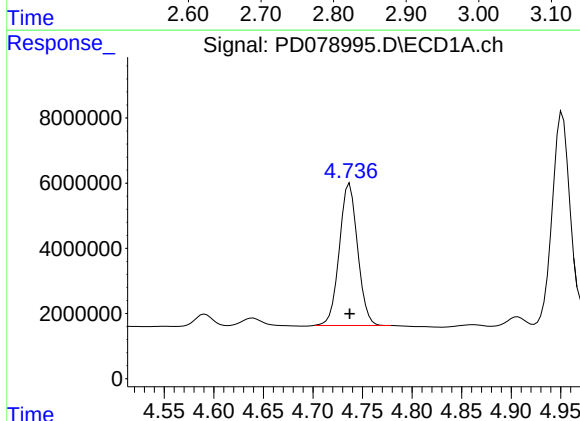


#23 Chlordane-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 55832656
Conc: 748.08 ng/ml

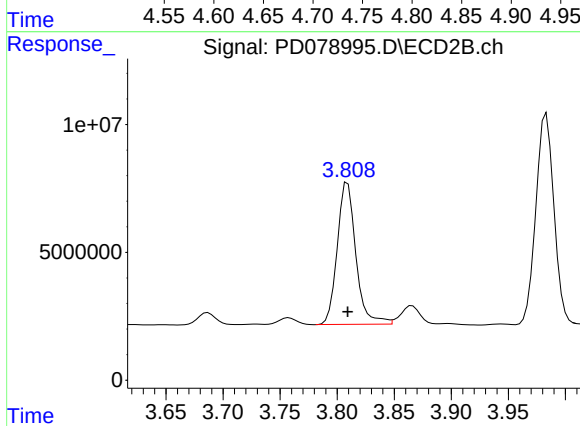

#23 Chlordane-1


R.T.: 3.809 min
Delta R.T.: 0.000 min
Response: 63176482
Conc: 749.34 ng/ml

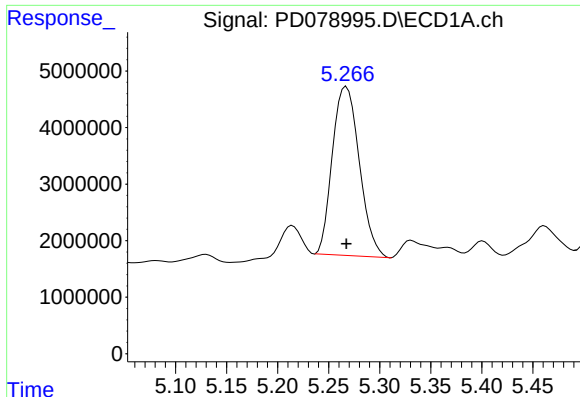

#24 Chlordane-2


R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 54944543
Conc: 748.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

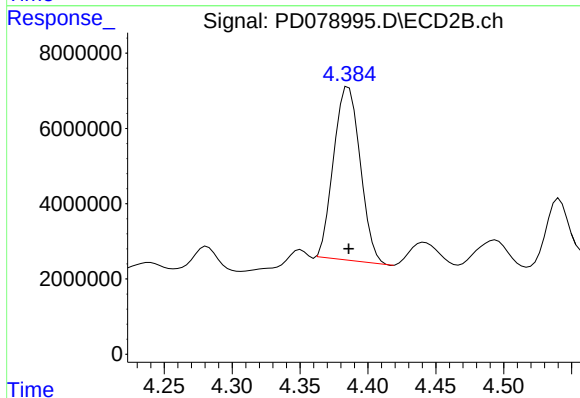


#24 Chlordane-2

R.T.: 4.386 min
Delta R.T.: 0.000 min
Response: 62909768
Conc: 744.17 ng/ml

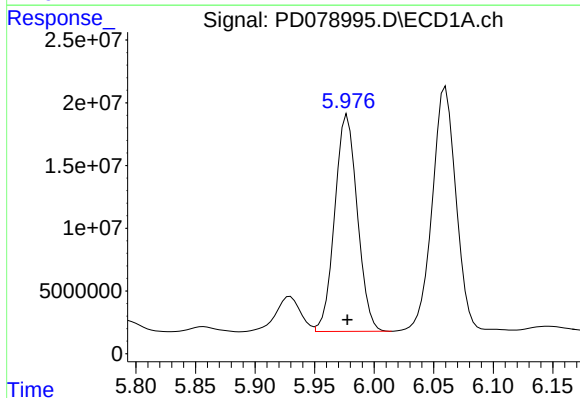


#25 Chlordane-3

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 227967007
Conc: 751.20 ng/ml

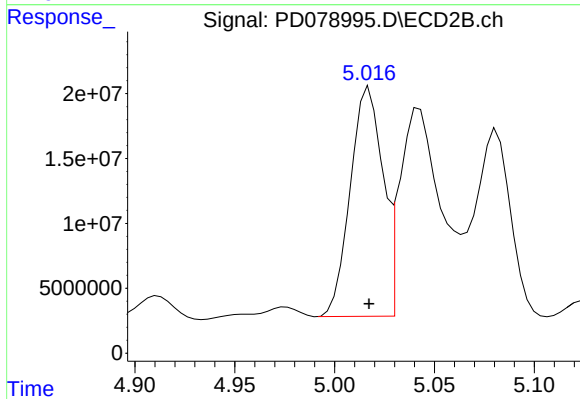

#25 Chlordane-3


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 199238052
Conc: 753.83 ng/ml

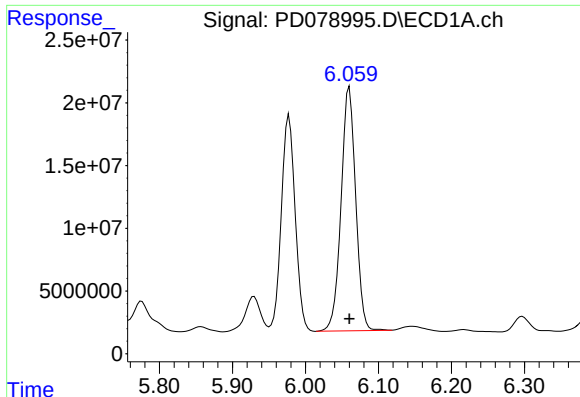

#26 Chlordane-4


R.T.: 6.060 min
Delta R.T.: 0.000 min
Response: 270018863
Conc: 752.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

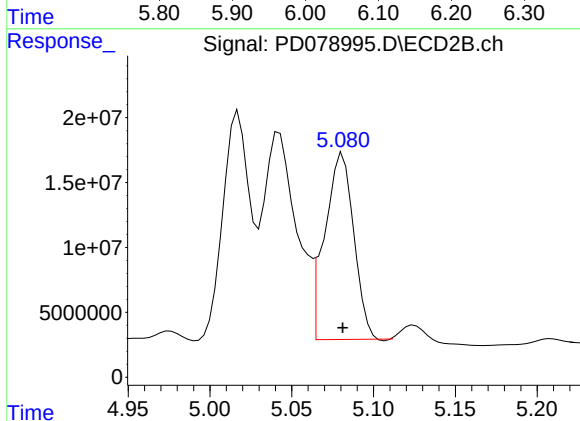


#26 Chlordane-4

R.T.: 5.081 min
Delta R.T.: 0.000 min
Response: 176826478
Conc: 735.62 ng/ml

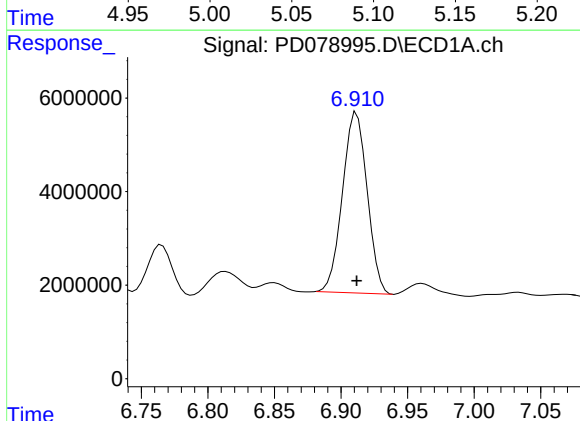


#27 Chlordane-5

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 49757779
Conc: 748.12 ng/ml

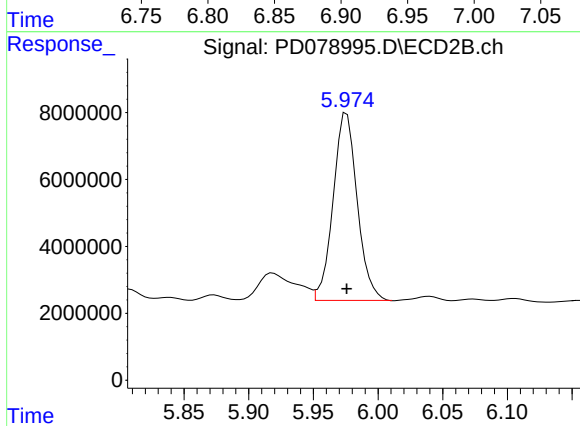

#27 Chlordane-5


R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 72520705
Conc: 749.27 ng/ml

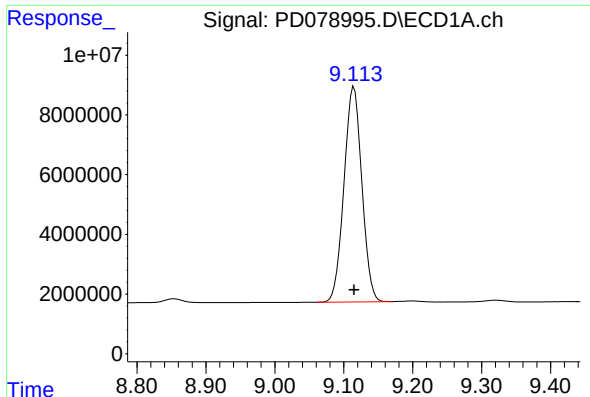

#28 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.000 min
Response: 129822607
Conc: 75.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

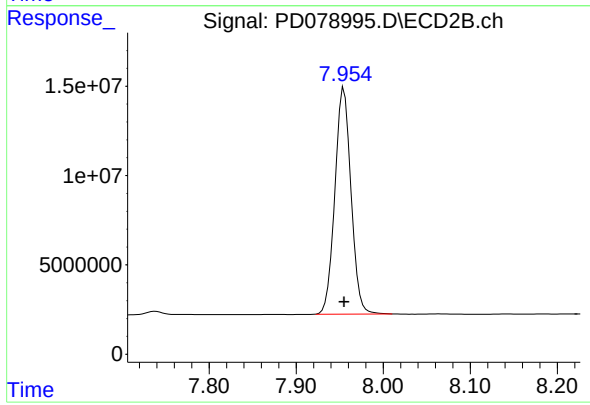

#28 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: 0.000 min
Response: 163469104
Conc: 74.57 ng/ml