

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102023\
 Data File : PD078996.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2023 19:55
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 02:01:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 01:59:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	73050432	125.7E6	50.000	50.000
28)	SA Decachlor...	9.115	7.956	87817231	112.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.737	3.809	37197379	42439279	500.000	500.000
24)	Chlordane-2	5.267	4.386	37848519	43750294	500.000	500.000
25)	Chlordane-3	5.978	5.017	150.2E6	131.4E6	500.000	500.000
26)	Chlordane-4	6.061	5.081	178.6E6	119.8E6	500.000	500.000
27)	Chlordane-5	6.912	5.976	33632859	48795587	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102023\
Data File : PD078996.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2023 19:55
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 02:01:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 01:59:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

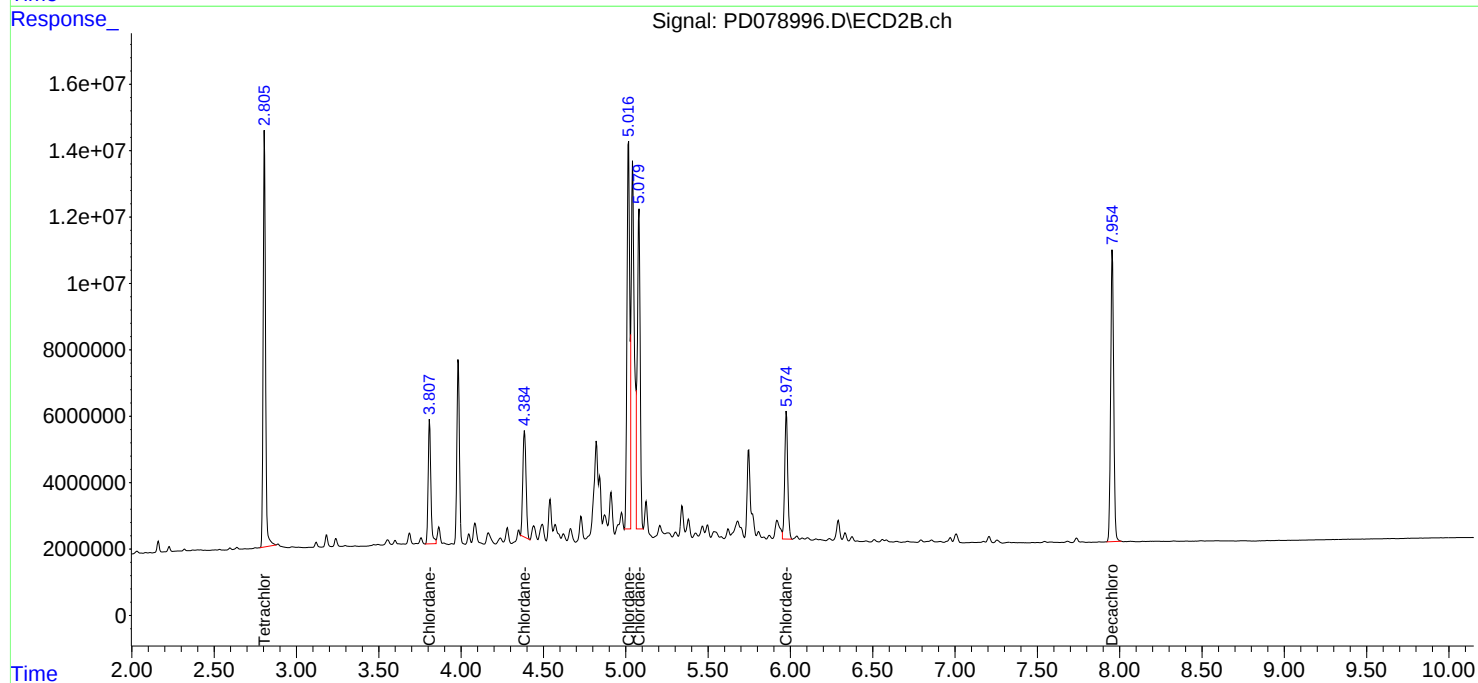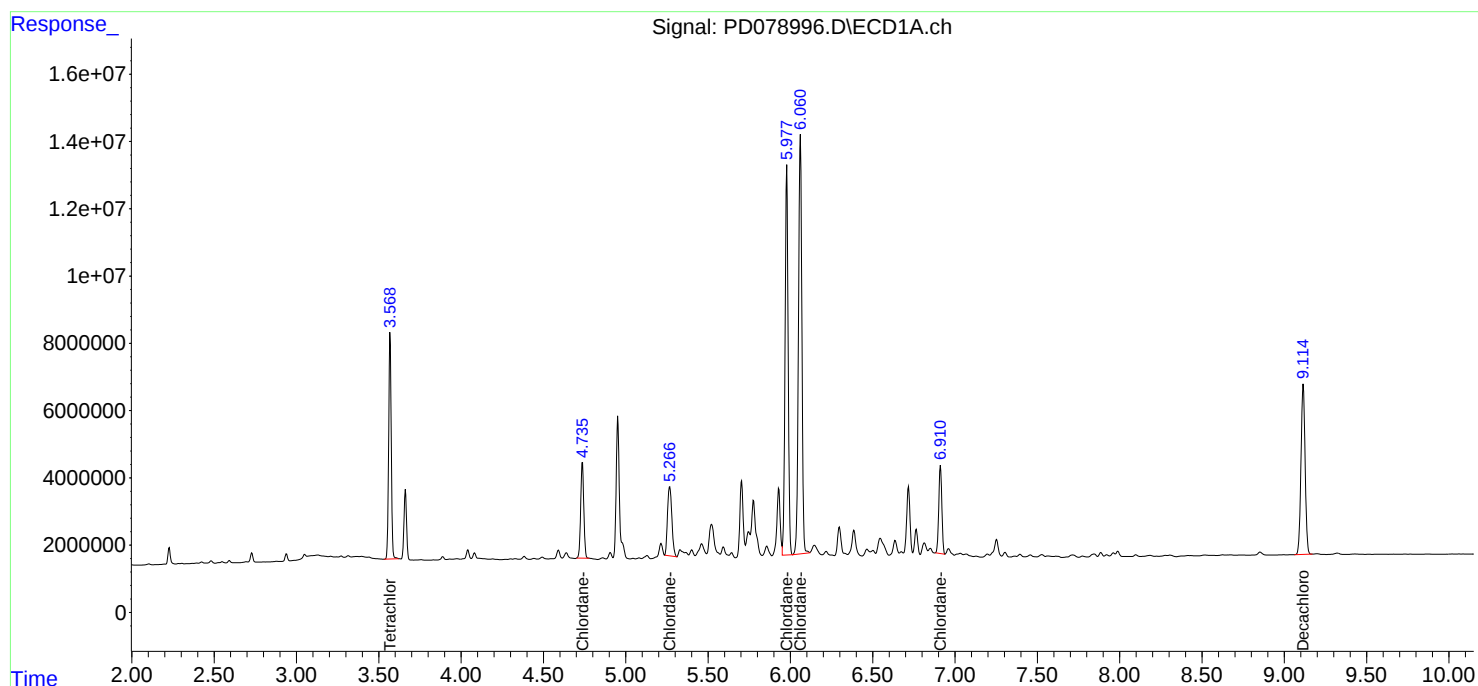


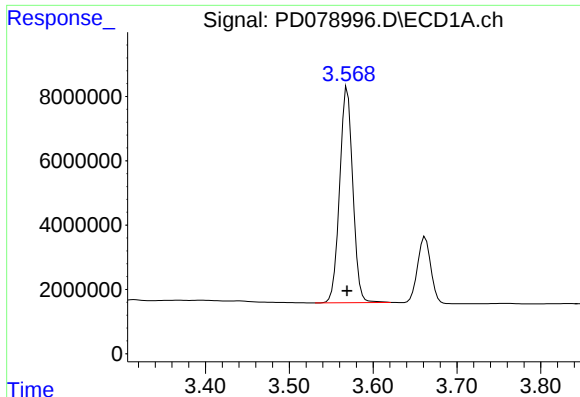

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 73050432
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

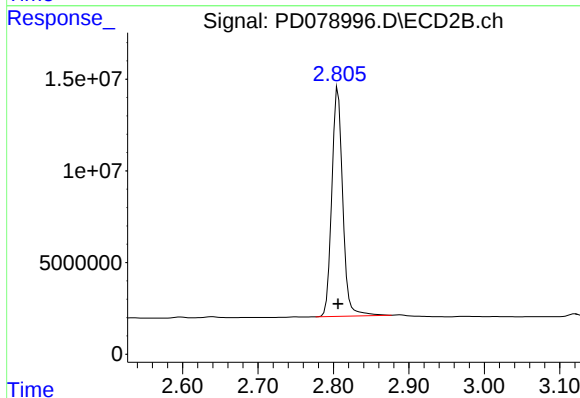


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 125711180
Conc: 50.00 ng/ml

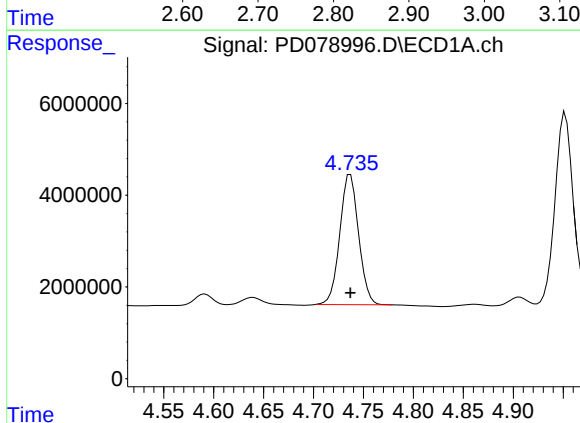


#23 Chlordane-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 37197379
Conc: 500.00 ng/ml

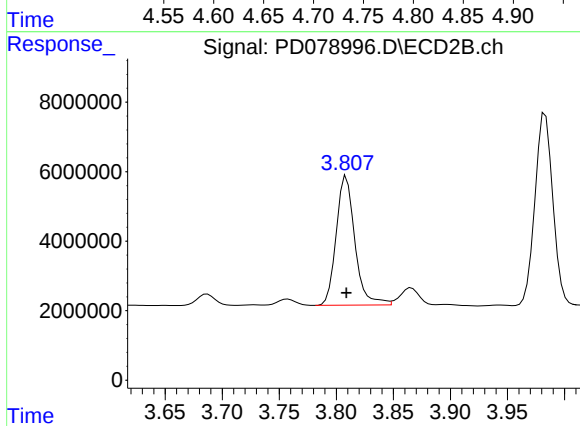

#23 Chlordane-1


R.T.: 3.809 min
Delta R.T.: 0.000 min
Response: 42439279
Conc: 500.00 ng/ml

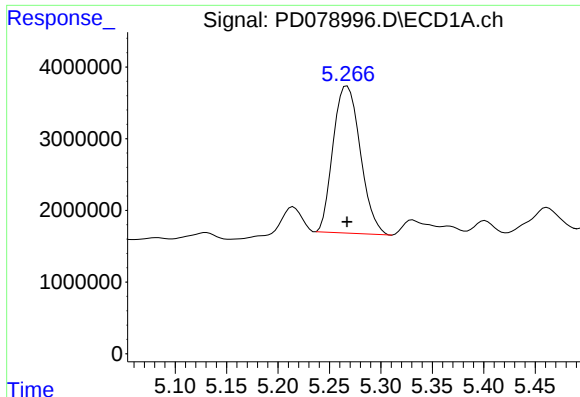

#24 Chlordane-2


R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 37848519
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

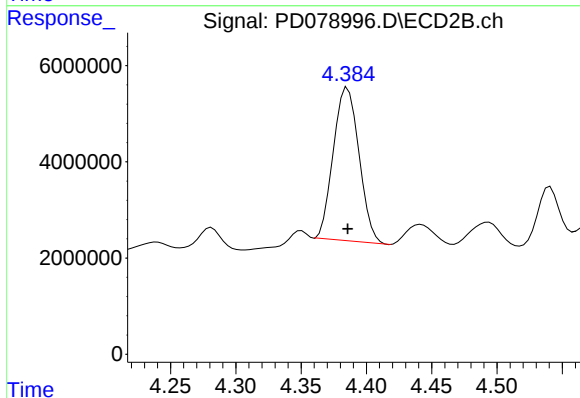


#24 Chlordane-2

R.T.: 4.386 min
Delta R.T.: 0.000 min
Response: 43750294
Conc: 500.00 ng/ml

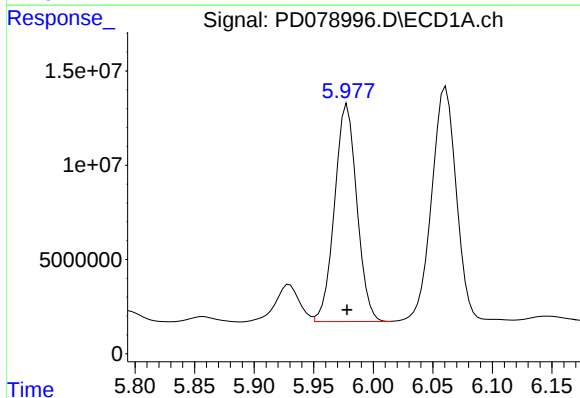


#25 Chlordane-3

R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 150162539
Conc: 500.00 ng/ml

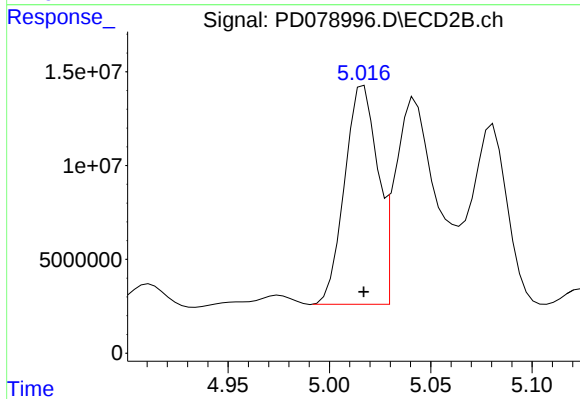

#25 Chlordane-3


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 131387791
Conc: 500.00 ng/ml

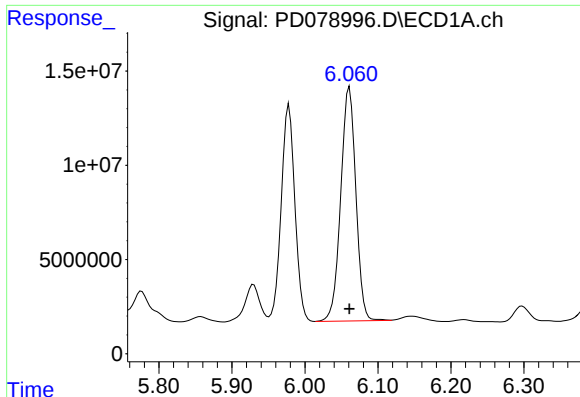

#26 Chlordane-4


R.T.: 6.061 min
Delta R.T.: 0.000 min
Response: 178596953
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

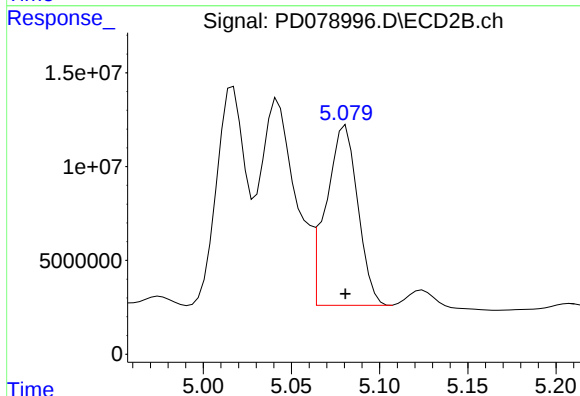


#26 Chlordane-4

R.T.: 5.081 min
Delta R.T.: 0.000 min
Response: 119767900
Conc: 500.00 ng/ml

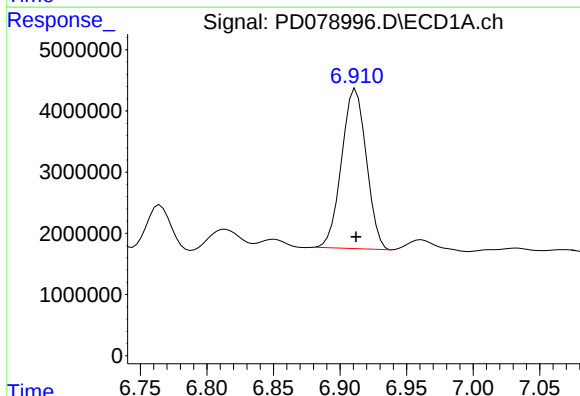


#27 Chlordane-5

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 33632859
Conc: 500.00 ng/ml

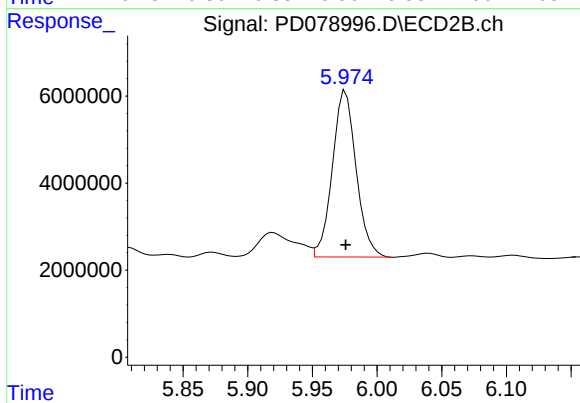

#27 Chlordane-5


R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 48795587
Conc: 500.00 ng/ml

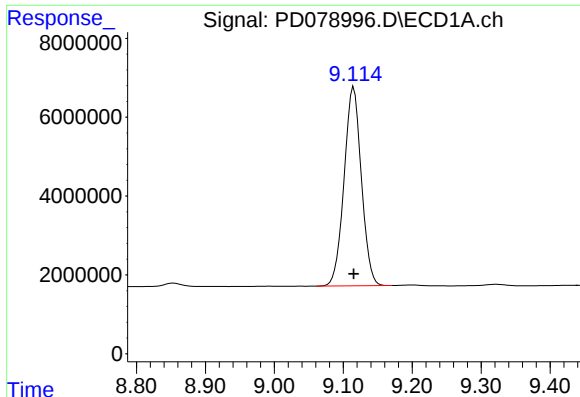

#28 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.000 min
Response: 87817231
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

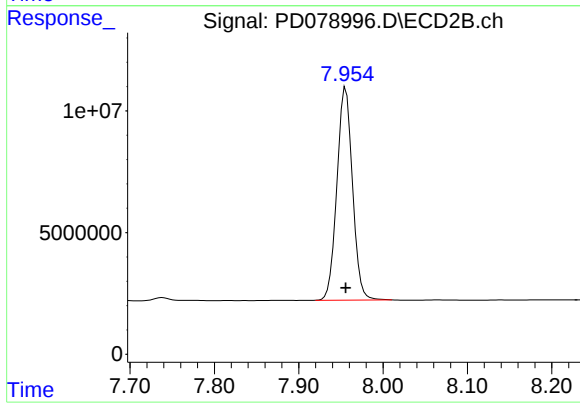

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 112238153
Conc: 50.00 ng/ml