

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102023\
 Data File : PD078997.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2023 20:08
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 02:09:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 02:09:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.806	36549186	62813465	25.020	24.937
28)	SA Decachlor...	9.115	7.956	48326330	58701763	27.260	26.309
Target Compounds							
23)	Chlordane-1	4.737	3.809	19494355	21407068	258.305	252.922
24)	Chlordane-2	5.267	4.386	20286515	22842511	269.362	264.854
25)	Chlordane-3	5.978	5.017	75236072	64334833	248.436	245.028
26)	Chlordane-4	6.061	5.082	91119370	59302337	252.860	247.520
27)	Chlordane-5	6.913	5.976	17606292	24642895	260.875	253.438



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102023\
Data File : PD078997.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2023 20:08
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 02:09:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 02:09:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

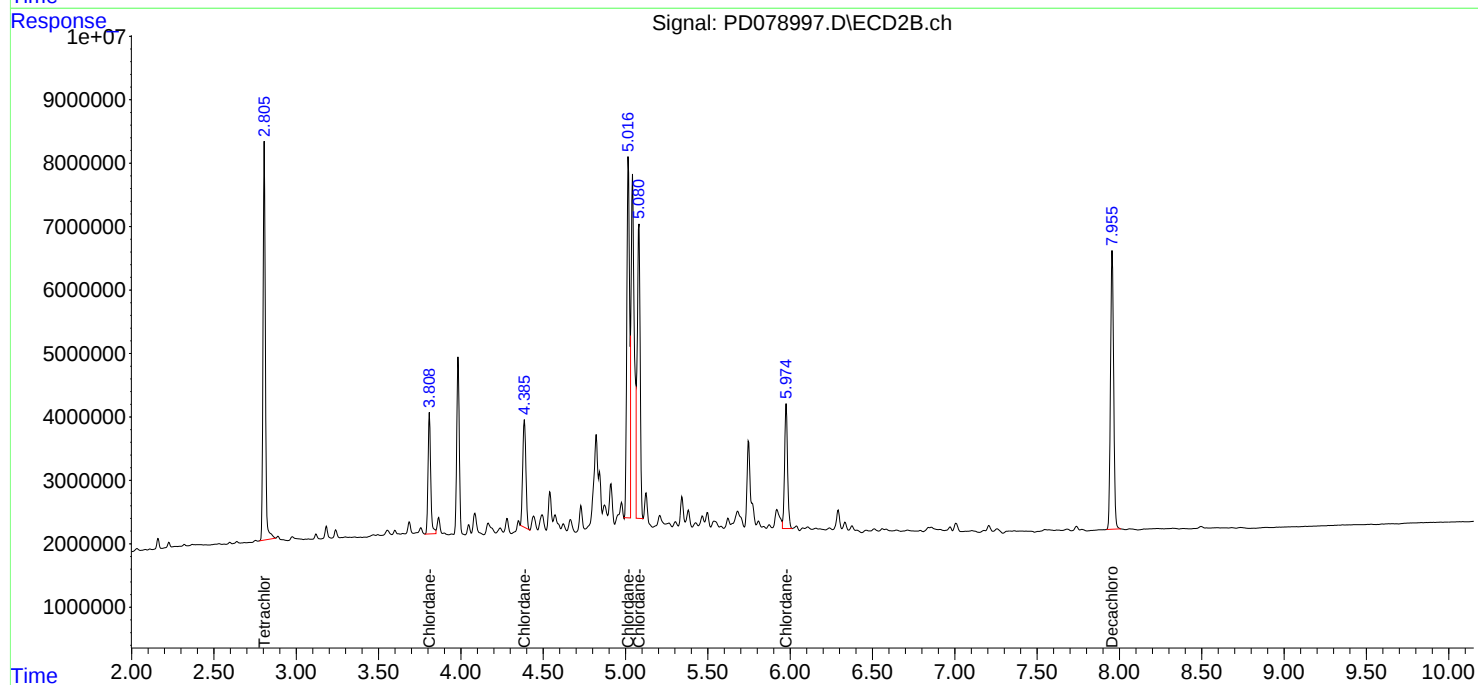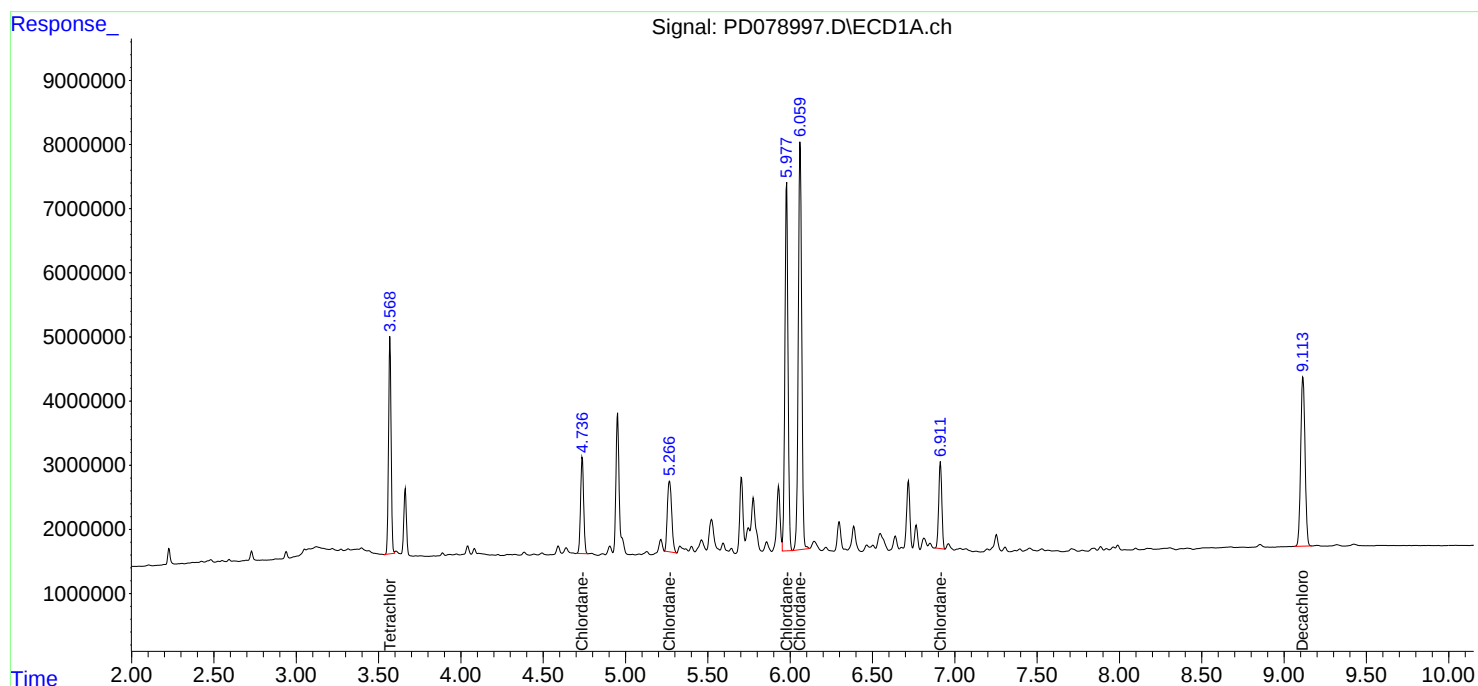


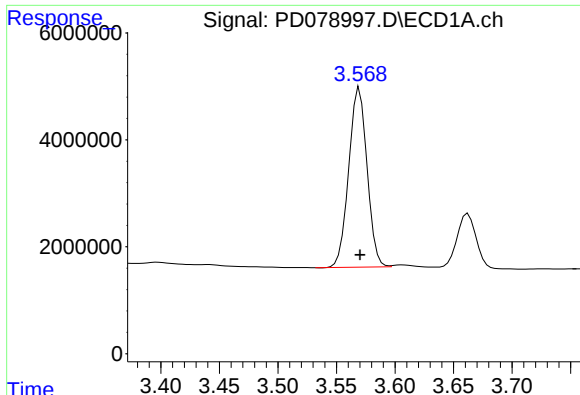

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 36549186
Conc: 25.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

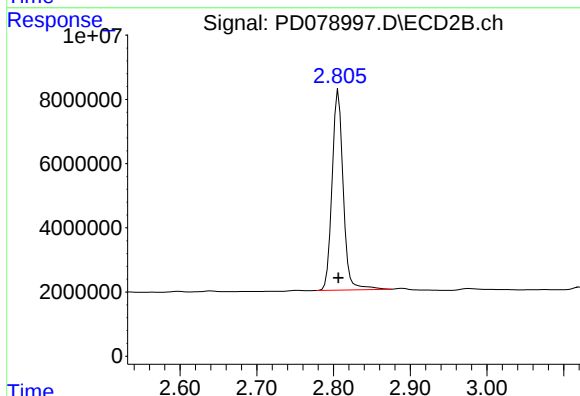


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 62813465
Conc: 24.94 ng/ml

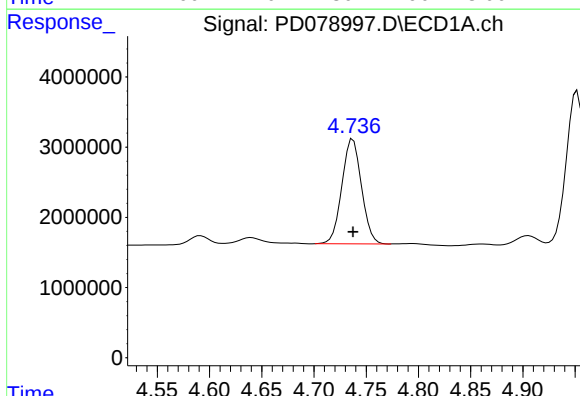


#23 Chlordane-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 19494355
Conc: 258.31 ng/ml

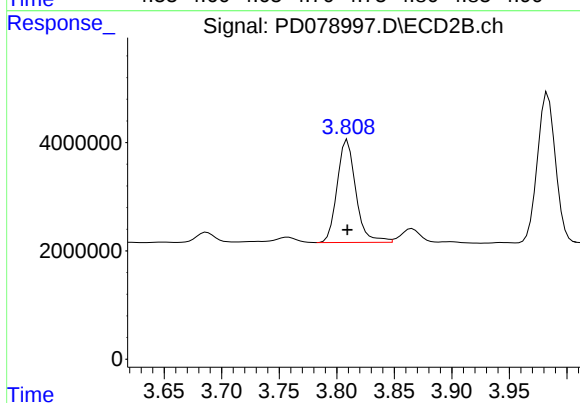

#23 Chlordane-1


R.T.: 3.809 min
Delta R.T.: 0.000 min
Response: 21407068
Conc: 252.92 ng/ml

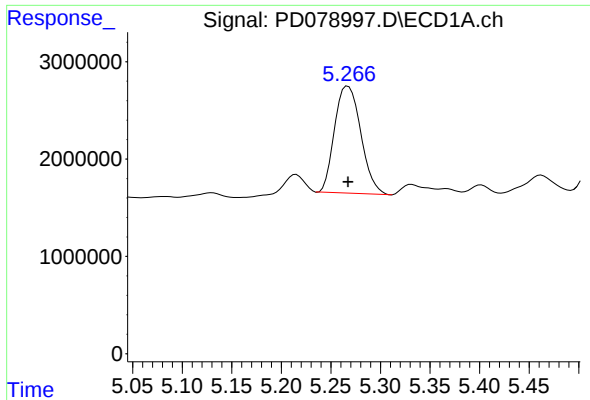

#24 Chlordane-2


R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 20286515
Conc: 269.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

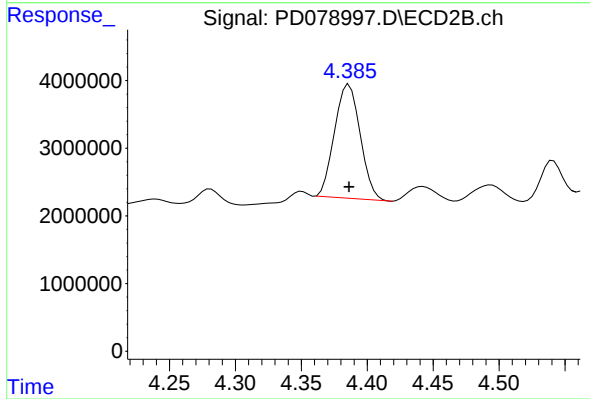


#24 Chlordane-2

R.T.: 4.386 min
Delta R.T.: 0.000 min
Response: 22842511
Conc: 264.85 ng/ml

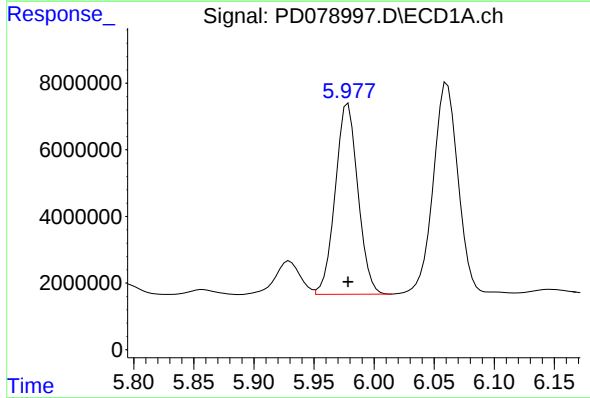


#25 Chlordane-3

R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 75236072
Conc: 248.44 ng/ml

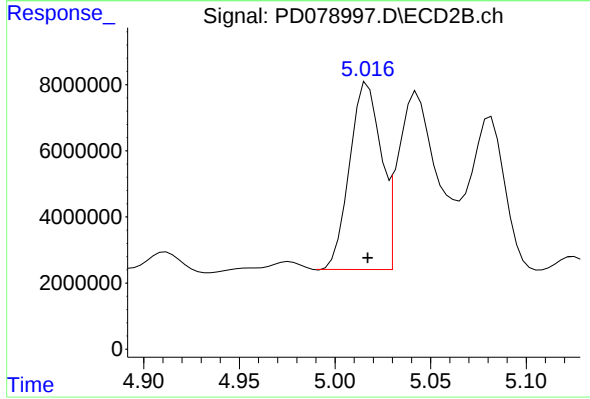

#25 Chlordane-3


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 64334833
Conc: 245.03 ng/ml

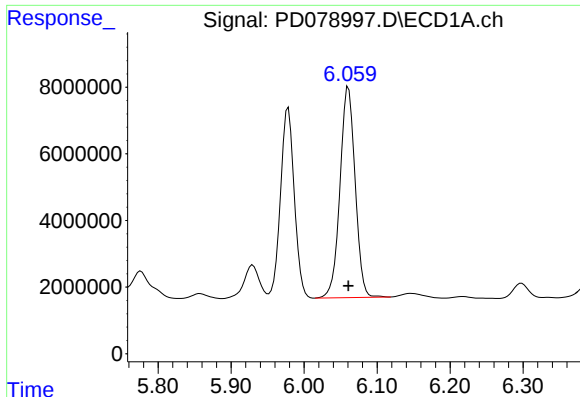

#26 Chlordane-4


R.T.: 6.061 min
Delta R.T.: 0.000 min
Response: 91119370
Conc: 252.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

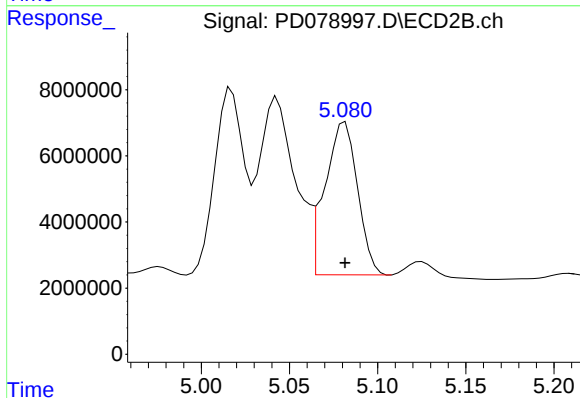


#26 Chlordane-4

R.T.: 5.082 min
Delta R.T.: 0.000 min
Response: 59302337
Conc: 247.52 ng/ml

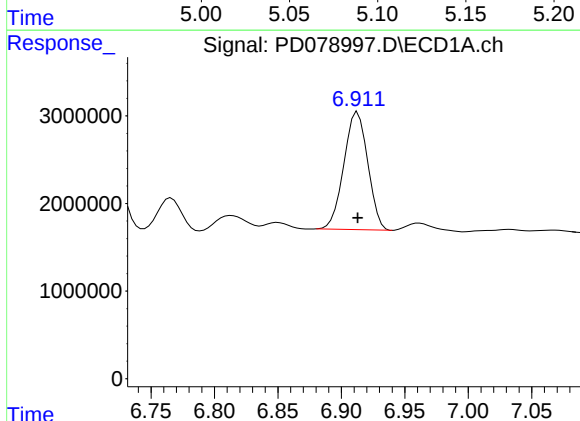


#27 Chlordane-5

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 17606292
Conc: 260.87 ng/ml

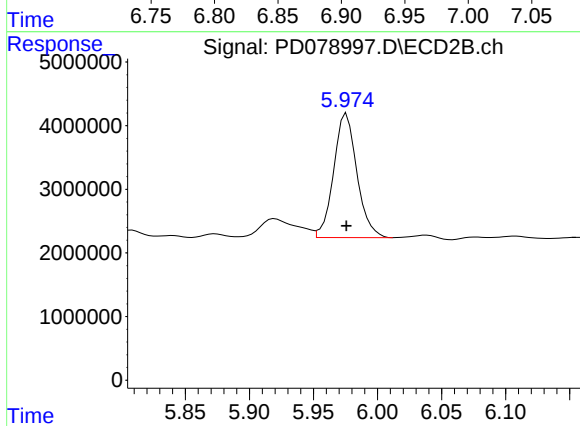

#27 Chlordane-5


R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 24642895
Conc: 253.44 ng/ml

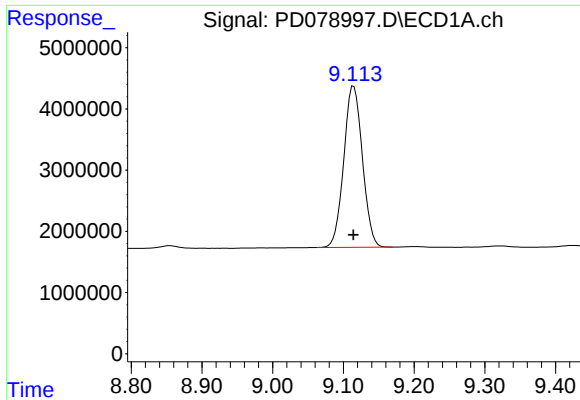

#28 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.000 min
Response: 48326330
Conc: 27.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

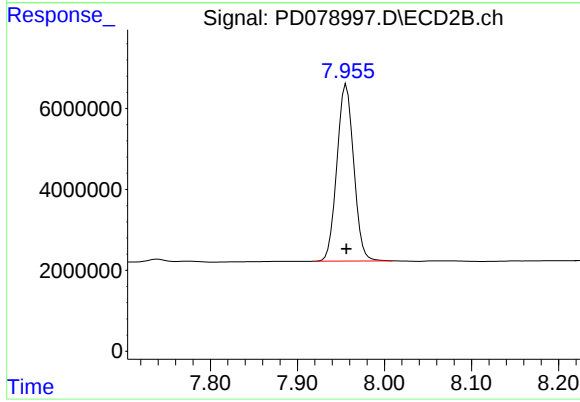

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 58701763
Conc: 26.31 ng/ml