

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102023\
 Data File : PD078998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2023 20:21
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 02:11:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 02:11:08 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	8330911	14046547	5.547	5.451
28)	SA Decachlor...	9.114	7.954	11648101	13798587	6.182	5.905
Target Compounds							
23)	Chlordane-1	4.737	3.809	4343033	4785970	55.860	55.103
24)	Chlordane-2	5.268	4.386	4894369	5465637	61.311	60.155
25)	Chlordane-3	5.978	5.017	16933399	14170833	54.623	53.128
26)	Chlordane-4	6.061	5.081	20810062	13427575	56.013	54.722
27)	Chlordane-5	6.912	5.976	4068456	5469151	57.901	54.876



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102023\
Data File : PD078998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2023 20:21
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 02:11:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 02:11:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

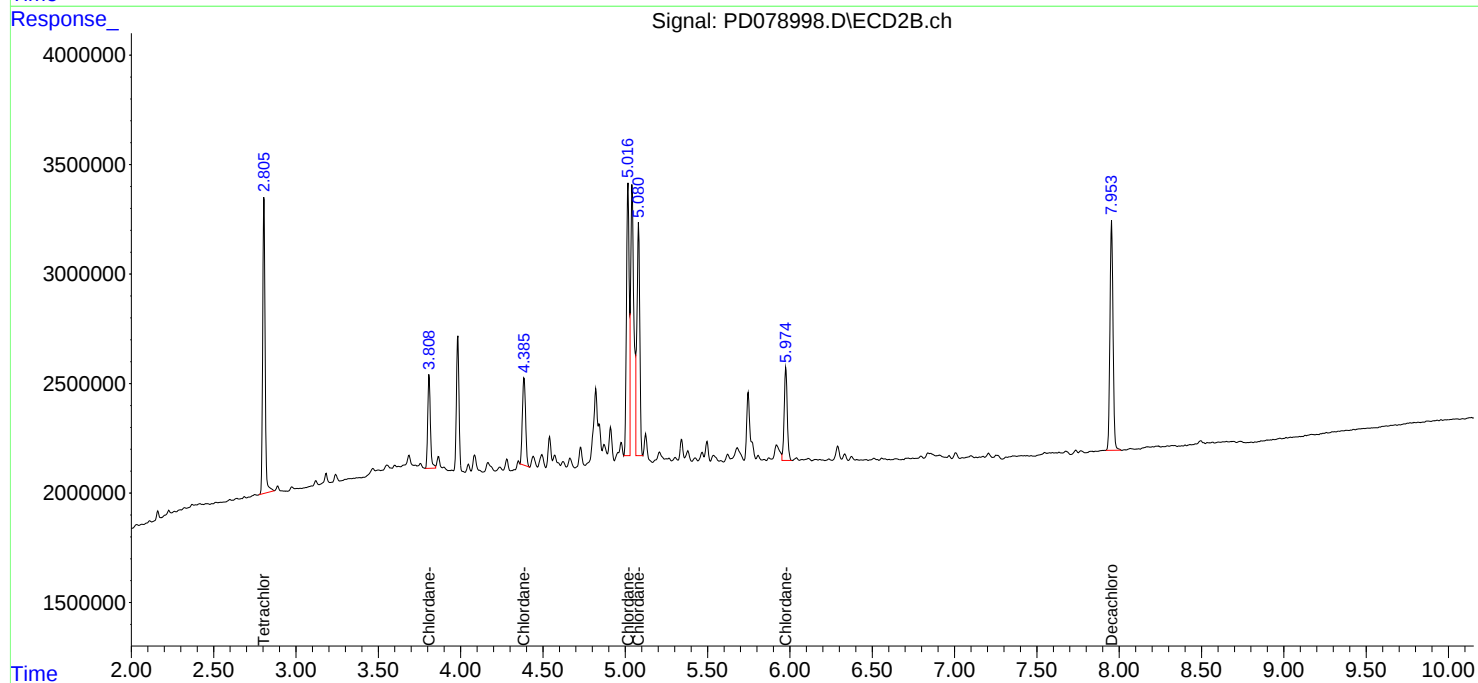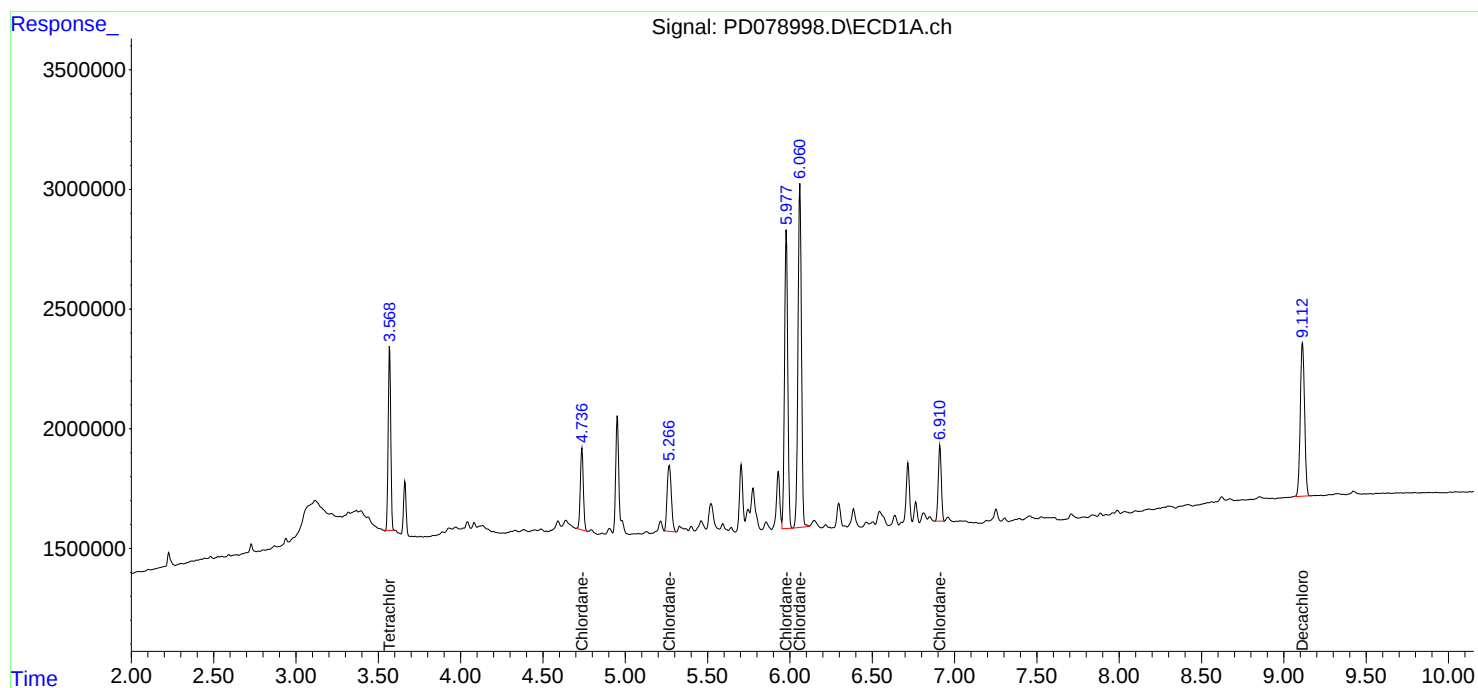


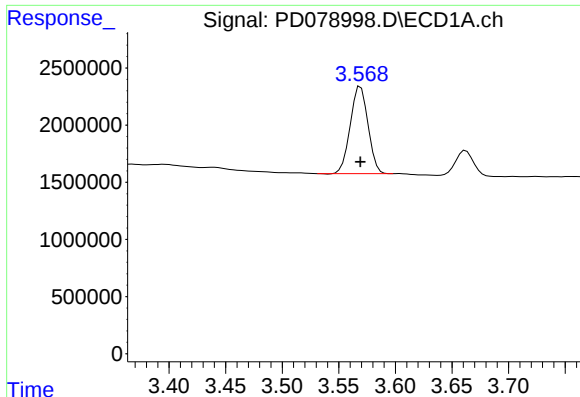

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 8330911
Conc: 5.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

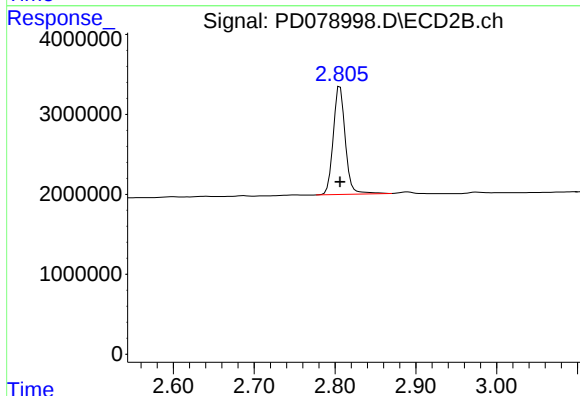


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 14046547
Conc: 5.45 ng/ml

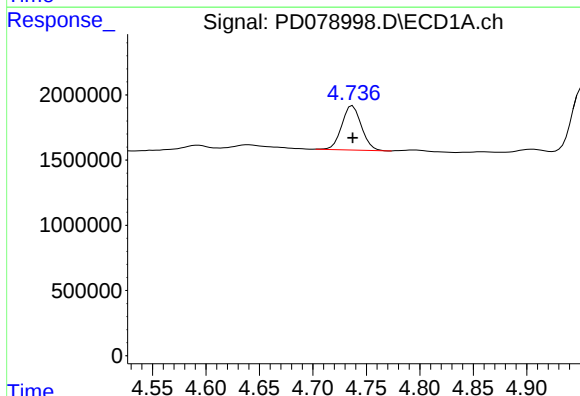


#23 Chlordane-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 4343033
Conc: 55.86 ng/ml

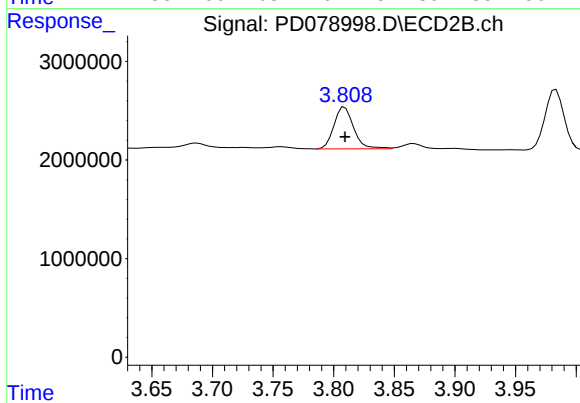

#23 Chlordane-1


R.T.: 3.809 min
Delta R.T.: 0.000 min
Response: 4785970
Conc: 55.10 ng/ml

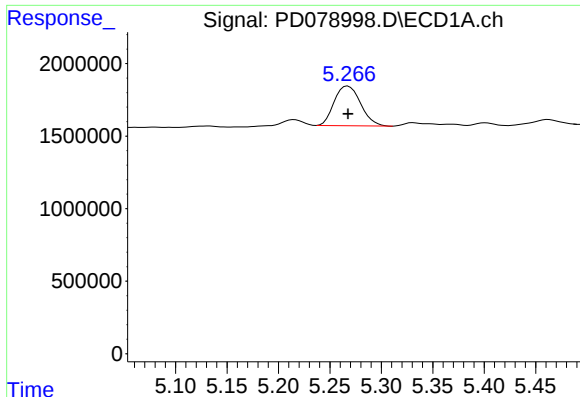

#24 Chlordane-2


R.T.: 5.268 min
Delta R.T.: 0.000 min
Response: 4894369
Conc: 61.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

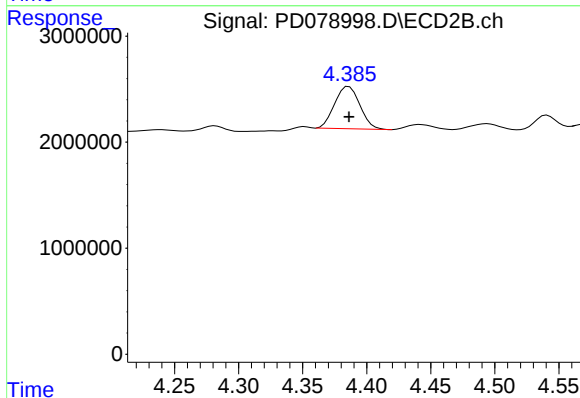


#24 Chlordane-2

R.T.: 4.386 min
Delta R.T.: 0.000 min
Response: 5465637
Conc: 60.16 ng/ml

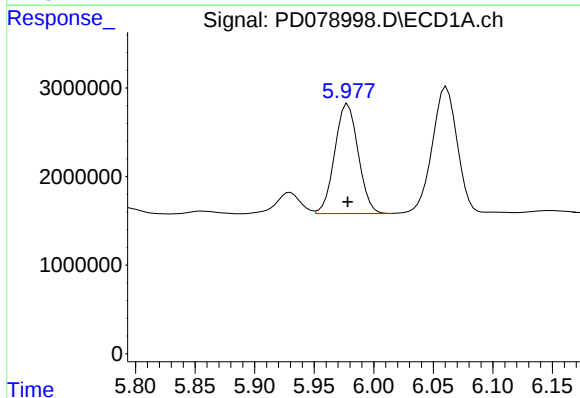


#25 Chlordane-3

R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 16933399
Conc: 54.62 ng/ml

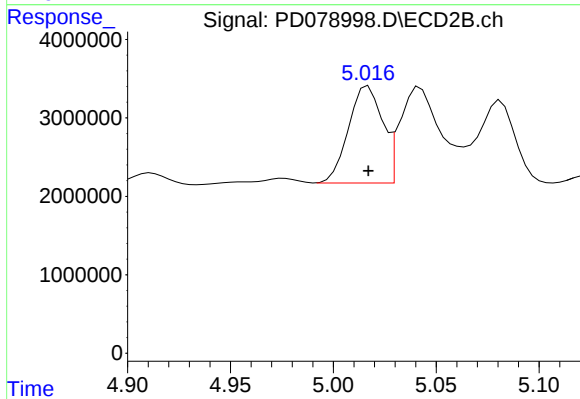

#25 Chlordane-3


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 14170833
Conc: 53.13 ng/ml

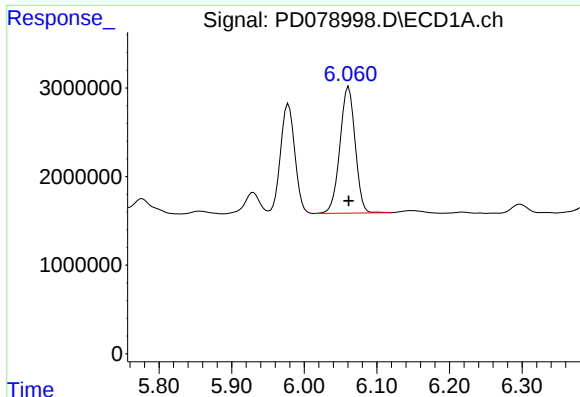

#26 Chlordane-4


R.T.: 6.061 min
Delta R.T.: 0.000 min
Response: 20810062
Conc: 56.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

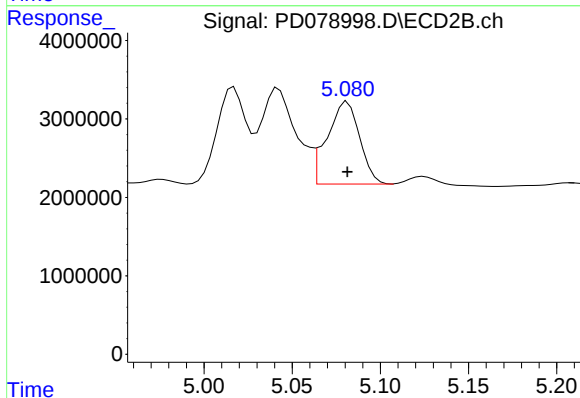


#26 Chlordane-4

R.T.: 5.081 min
Delta R.T.: 0.000 min
Response: 13427575
Conc: 54.72 ng/ml

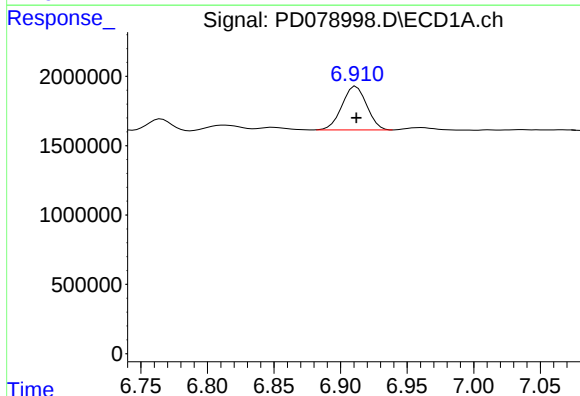


#27 Chlordane-5

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 4068456
Conc: 57.90 ng/ml

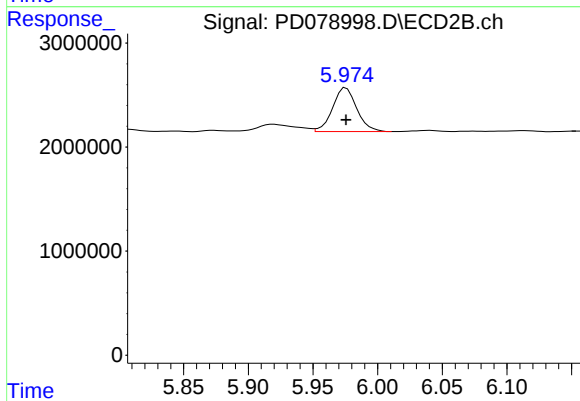

#27 Chlordane-5


R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 5469151
Conc: 54.88 ng/ml

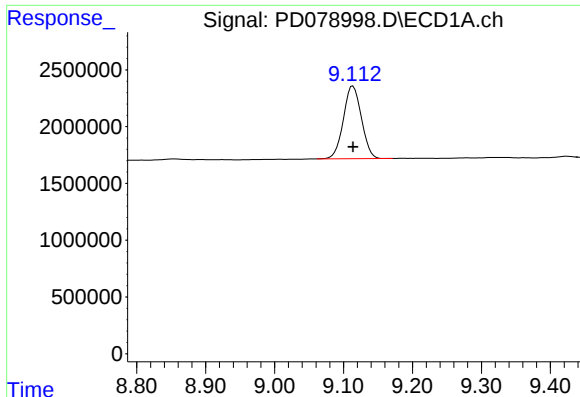

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 11648101
Conc: 6.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

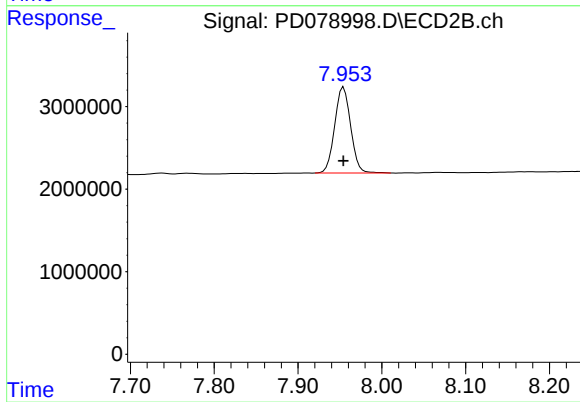

#28 Decachlorobiphenyl

R.T.: 7.954 min
Delta R.T.: 0.000 min
Response: 13798587
Conc: 5.90 ng/ml