

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102120\
 Data File : PD059859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 00:49
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 07:36:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:13:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	5.924f	0	7354014	N.D. 2.679 #
22)	Mirex	7.423	0.000	2936482	0	2.050 N.D. #
27)	Chlordane-5	0.000	7.027	0	634407	N.D. 7.704 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102120\
Data File : PD059859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 00:49
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 07:36:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:13:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

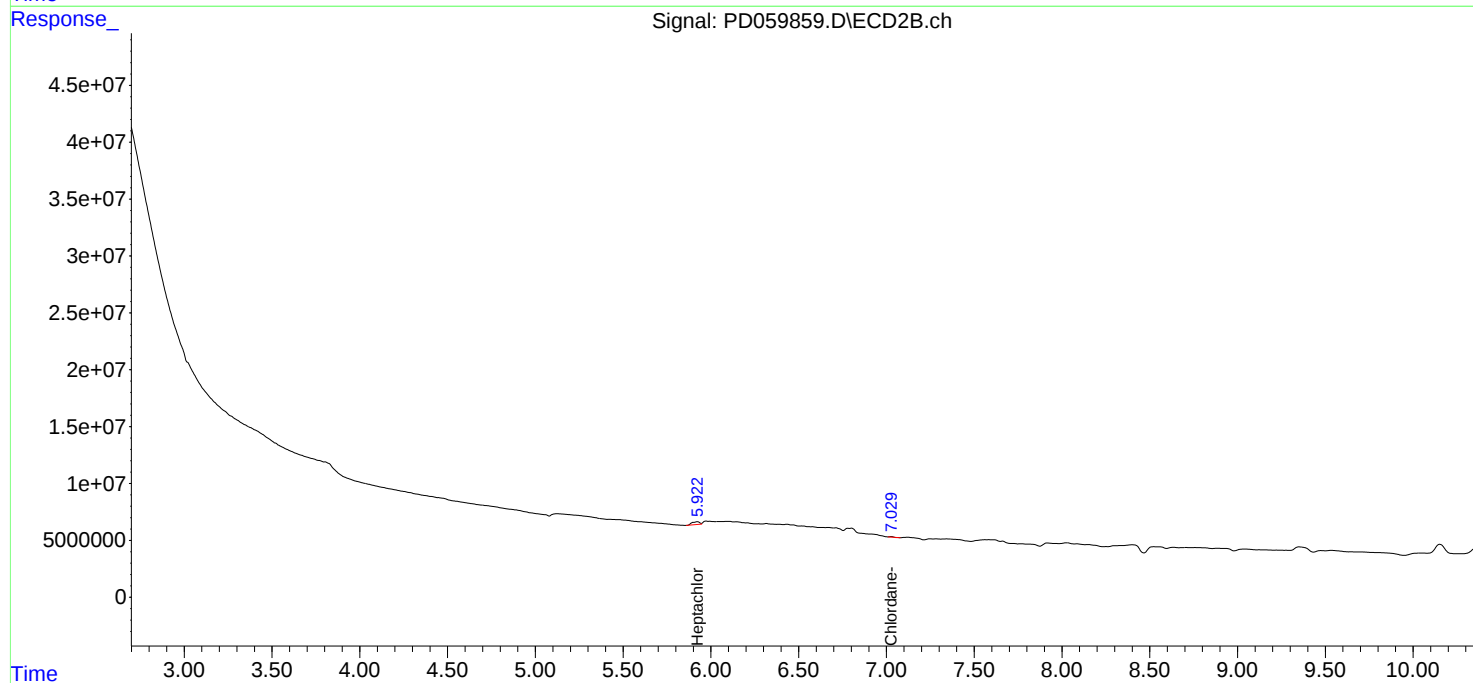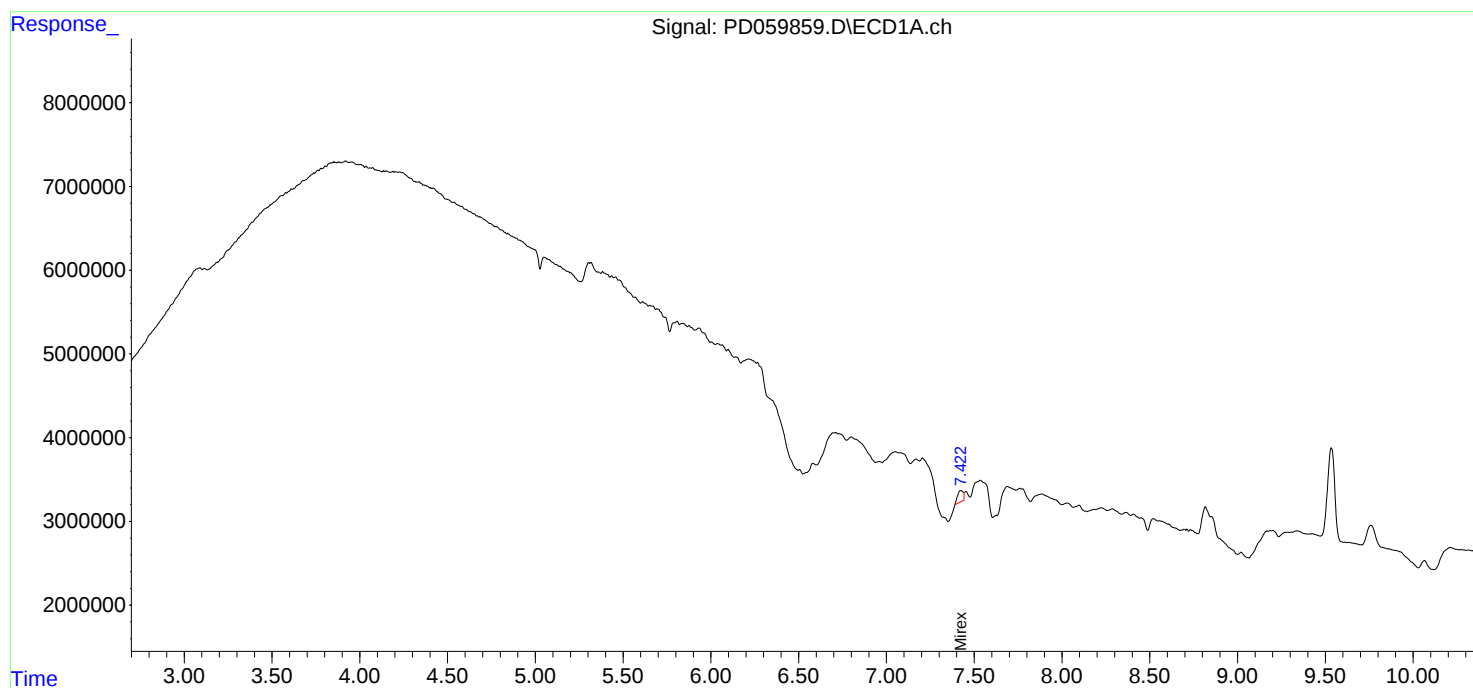


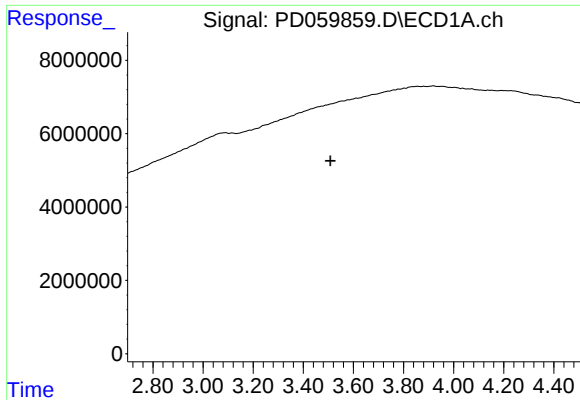

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

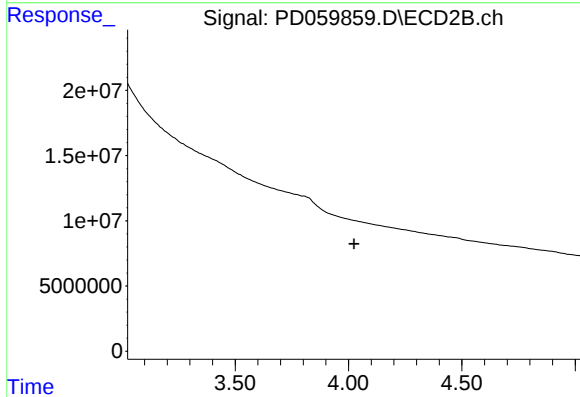


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.024 min
Response: 0
Conc: N.D.

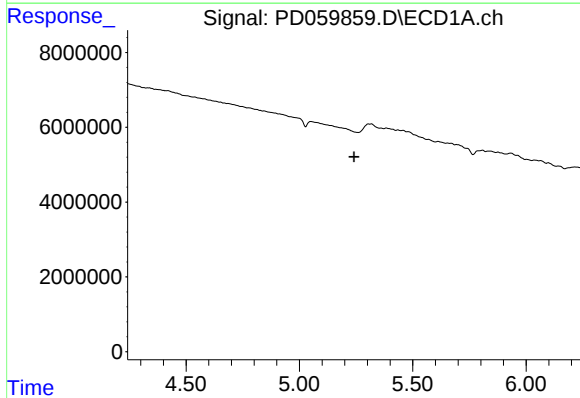


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.242 min
Response: 0
Conc: N.D.

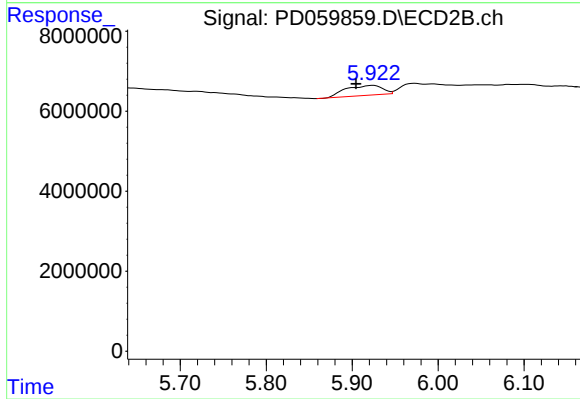

#8 Heptachlor epoxide


R.T.: 5.924 min
Delta R.T.: 0.020 min
Response: 7354014
Conc: 2.68 ng/ml

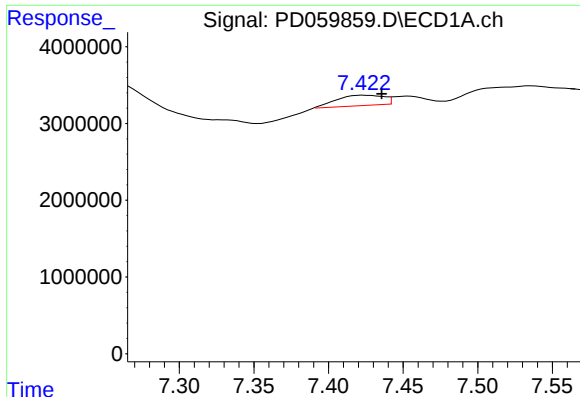

#22 Mirex


R.T.: 7.423 min
Delta R.T.: -0.012 min
Response: 2936482
Conc: 2.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

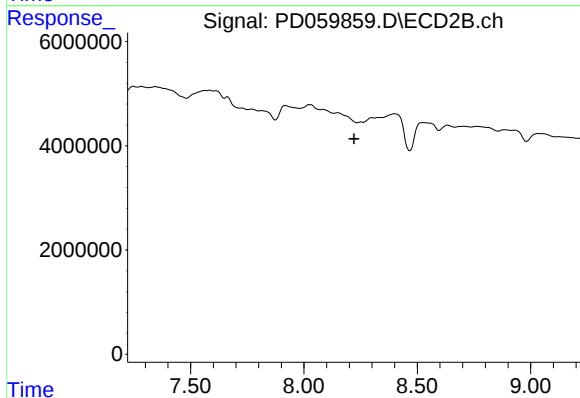


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.221 min
Response: 0
Conc: N.D.

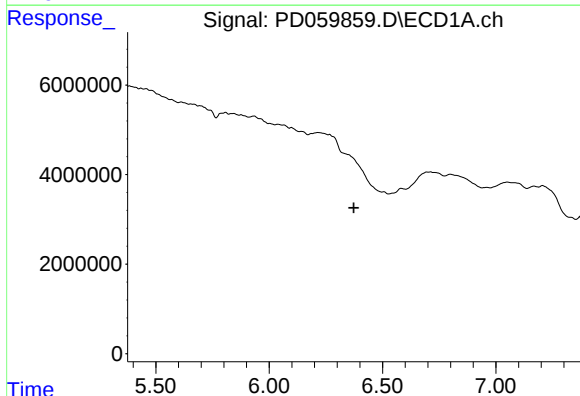


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.373 min
Response: 0
Conc: N.D.

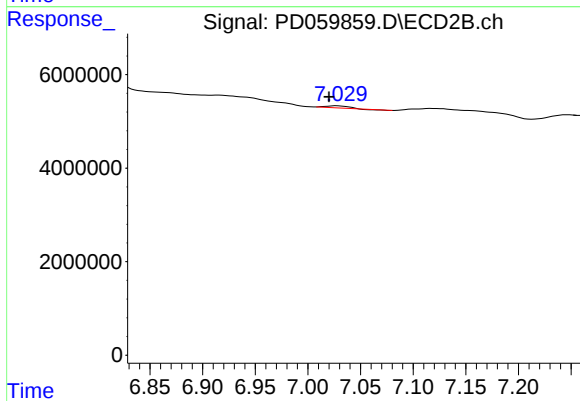

#27 Chlordane-5


R.T.: 7.027 min
Delta R.T.: 0.007 min
Response: 634407
Conc: 7.70 ng/ml

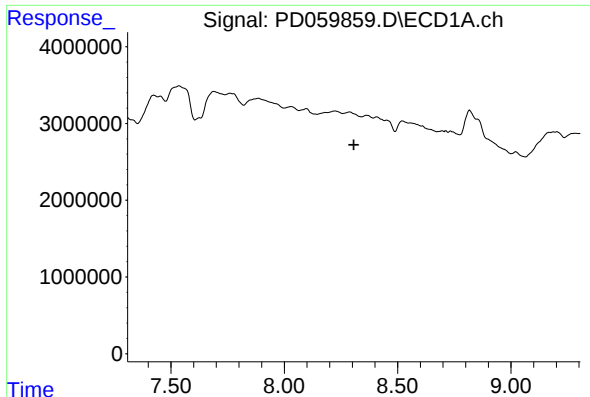

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.307 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

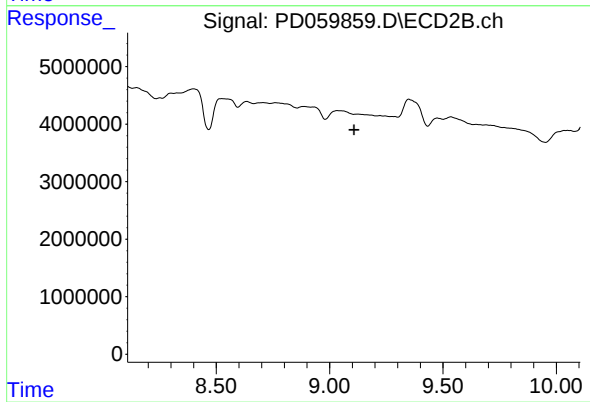

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.108 min
Response: 0
Conc: N.D.