

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102120\
 Data File : PD059860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 01:03
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 07:37:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:13:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.024	30699808	49881241	20.675	20.323
28)	SA Decachlor...	8.308	9.108	36409511	40095162	23.549	22.141
Target Compounds							
5)	MB Aldrin	0.000	5.517	0	1517702	N.D.	0.483 #
8)	B Heptachlo...	0.000	5.892	0	872607	N.D.	0.318 #
15)	B Endosulfa...	0.000	6.951	0	442980	N.D.	0.171 #
16)	A 4,4'-DDD	0.000	6.886f	0	238180	N.D.	0.103 #
18)	B Endrin al...	0.000	7.065	0	134982	N.D.	0.065 #
19)	B Endosulfa...	6.758	0.000	269682	0	0.167	N.D. #
21)	B Endrin ke...	0.000	7.779	0	3022481	N.D.	1.216 #
23)	Chlordane-1	4.415f	0.000	1472841	0	23.960	N.D. #
24)	Chlordane-2	0.000	5.517f	0	1517702	N.D.	15.401 #
27)	Chlordane-5	0.000	7.032	0	489098	N.D.	5.939 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102120\
Data File : PD059860.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 01:03
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 07:37:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:13:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

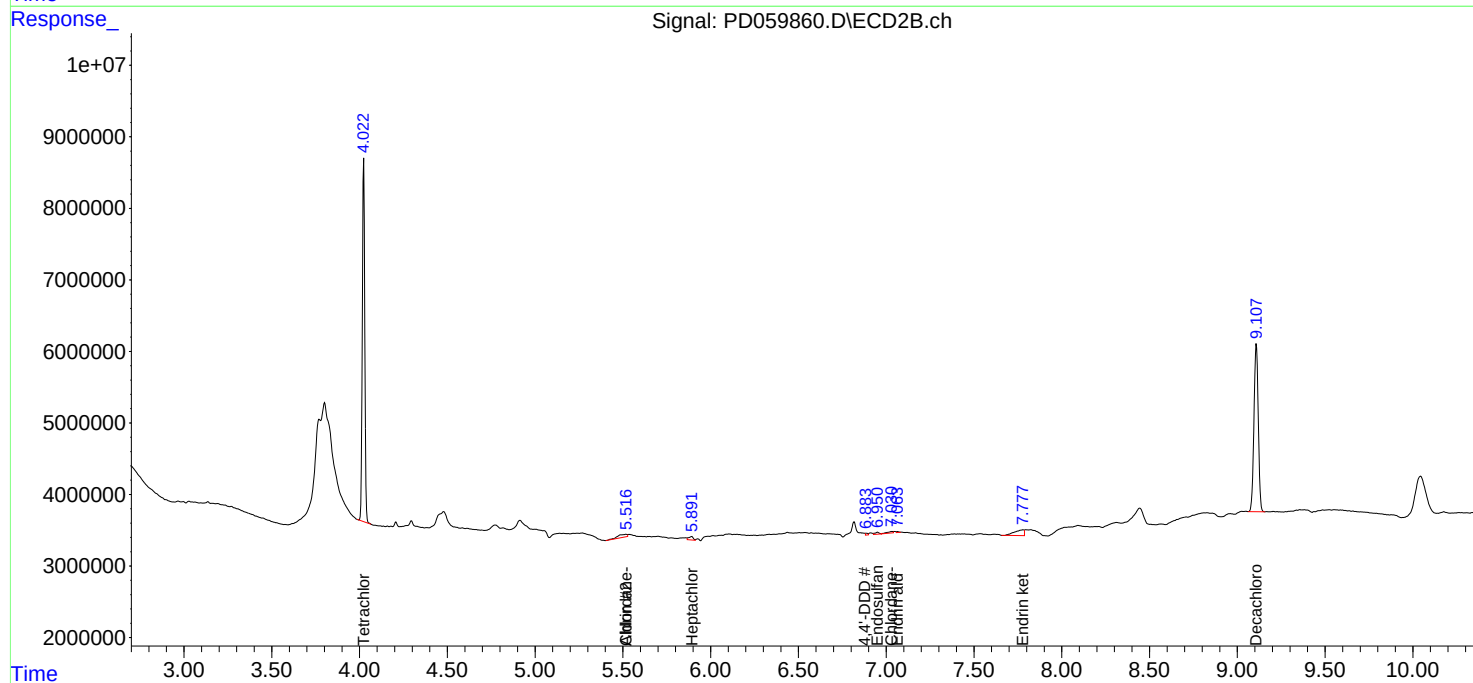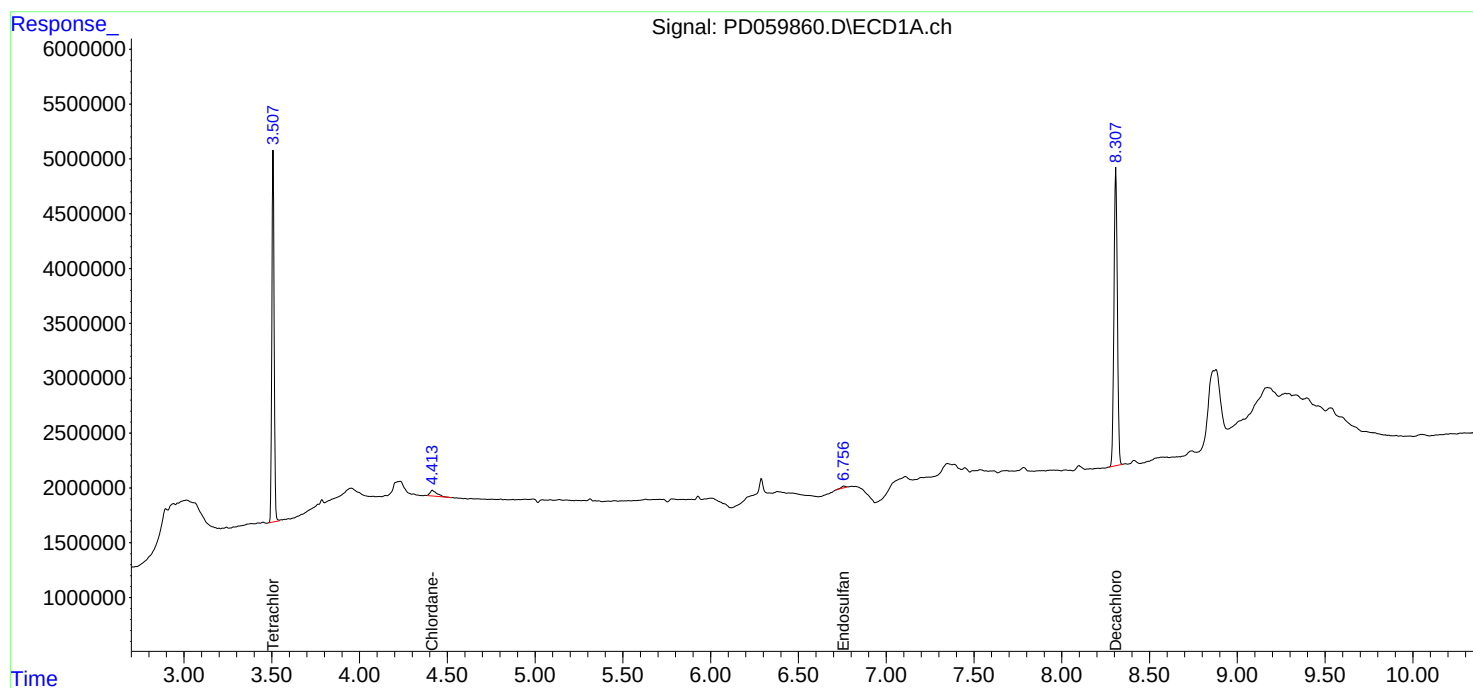


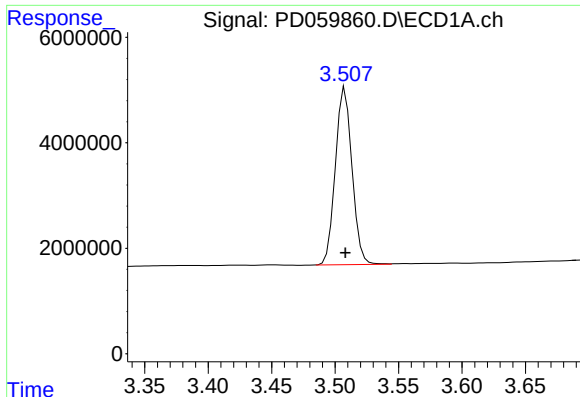

#1 Tetrachloro-m-xylene


R.T.: 3.508 min
Delta R.T.: 0.000 min
Response: 30699808
Conc: 20.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

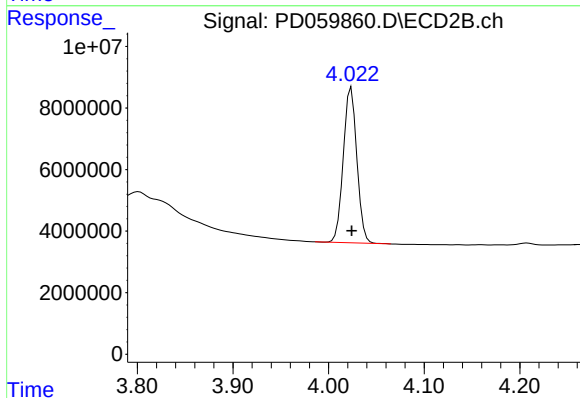


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 49881241
Conc: 20.32 ng/ml

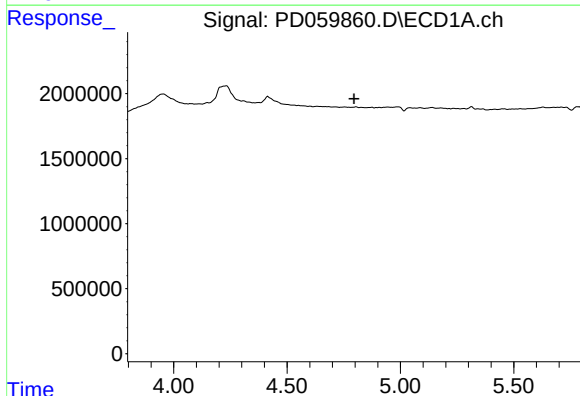


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.795 min
Response: 0
Conc: N.D.

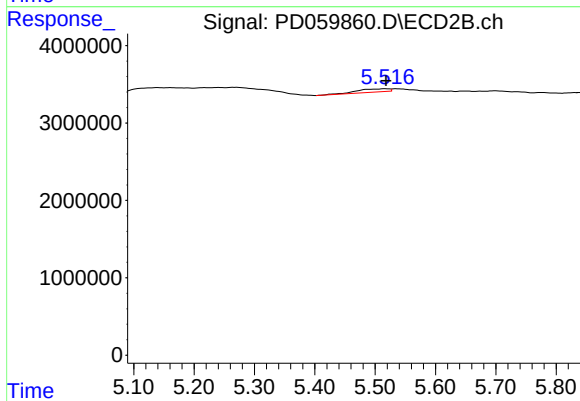

#5 Aldrin


R.T.: 5.517 min
Delta R.T.: -0.001 min
Response: 1517702
Conc: 0.48 ng/ml

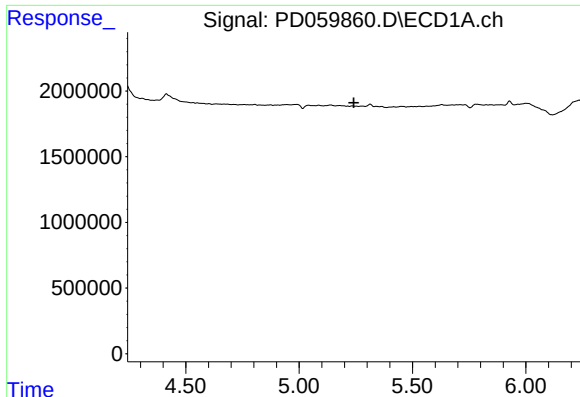

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

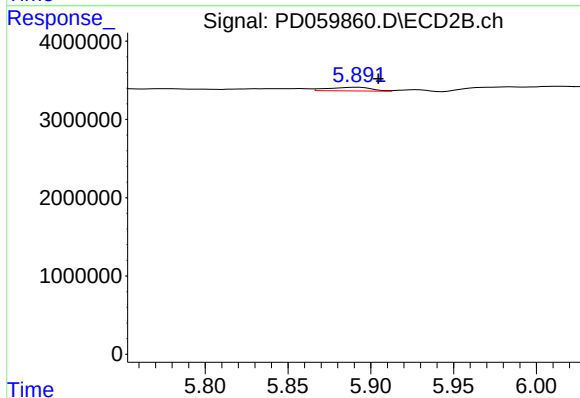


#8 Heptachlor epoxide

R.T.: 5.892 min
Delta R.T.: -0.012 min
Response: 872607
Conc: 0.32 ng/ml

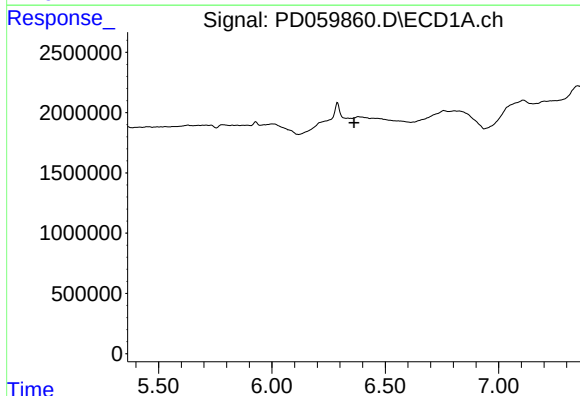


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.362 min
Response: 0
Conc: N.D.

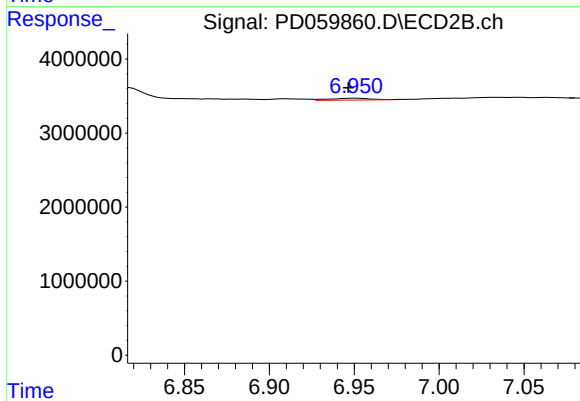

#15 Endosulfan II


R.T.: 6.951 min
Delta R.T.: 0.004 min
Response: 442980
Conc: 0.17 ng/ml

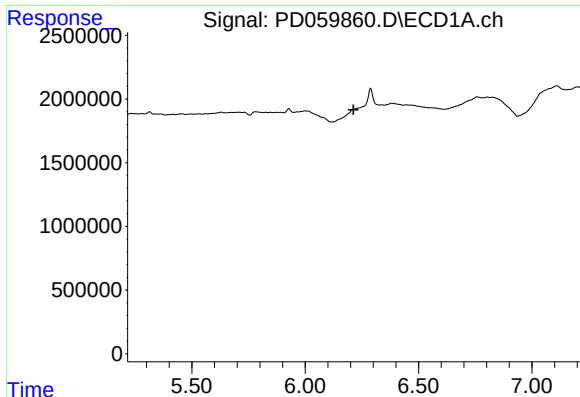

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

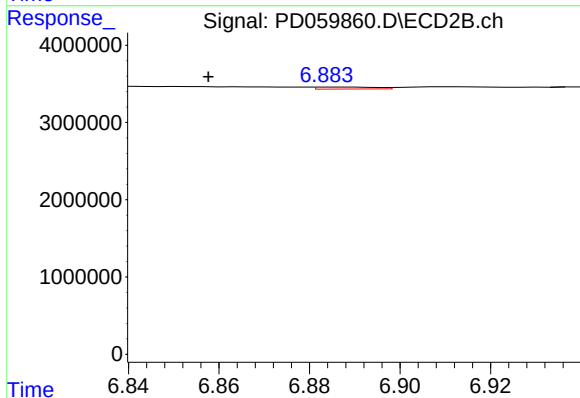


#16 4,4'-DDD

R.T.: 6.886 min
Delta R.T.: 0.029 min
Response: 238180
Conc: 0.10 ng/ml

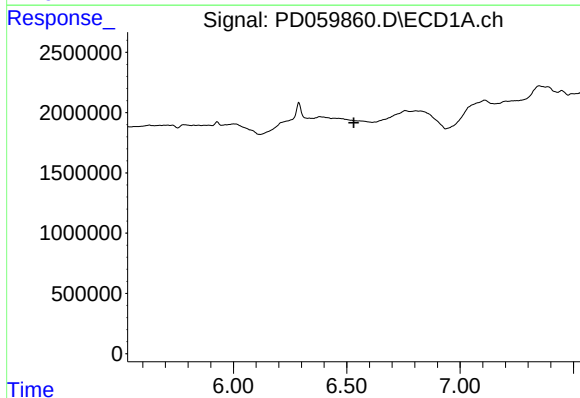


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

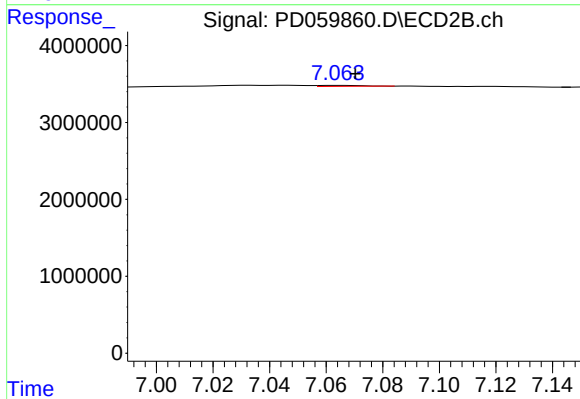

#18 Endrin aldehyde


R.T.: 7.065 min
Delta R.T.: -0.006 min
Response: 134982
Conc: 0.07 ng/ml

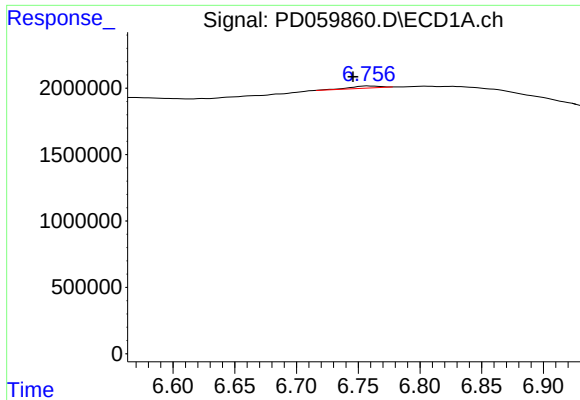

#19 Endosulfan Sulfate


R.T.: 6.758 min
Delta R.T.: 0.012 min
Response: 269682
Conc: 0.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

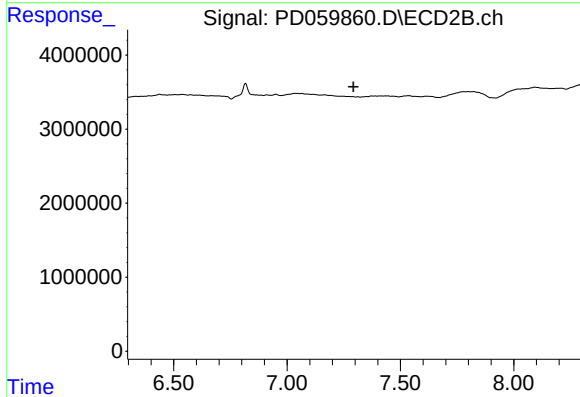


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.294 min
Response: 0
Conc: N.D.

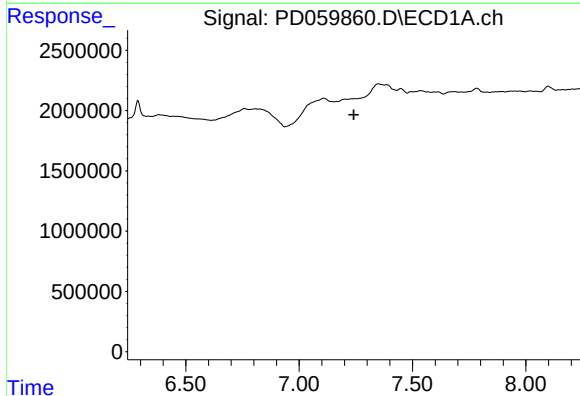


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.242 min
Response: 0
Conc: N.D.

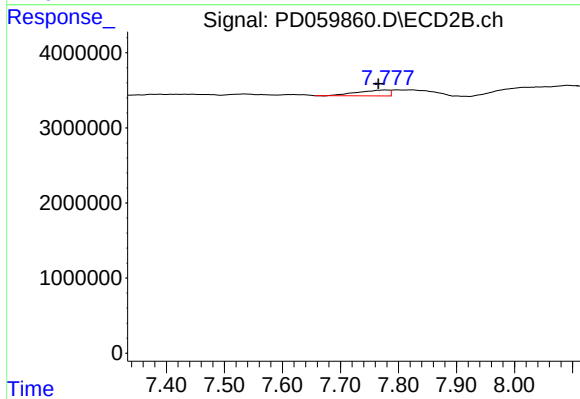

#21 Endrin ketone


R.T.: 7.779 min
Delta R.T.: 0.013 min
Response: 3022481
Conc: 1.22 ng/ml

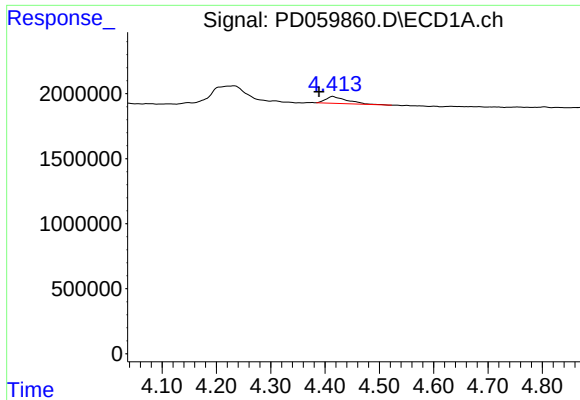

#23 Chlordane-1


R.T.: 4.415 min
Delta R.T.: 0.026 min
Response: 1472841
Conc: 23.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

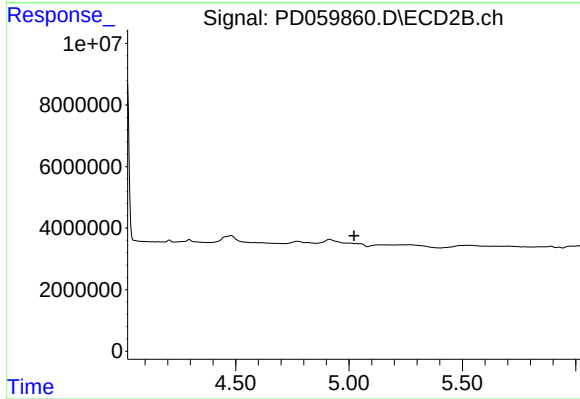


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.023 min
Response: 0
Conc: N.D.

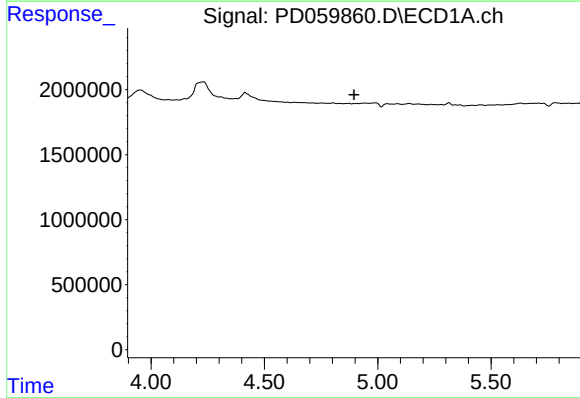


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.896 min
Response: 0
Conc: N.D.

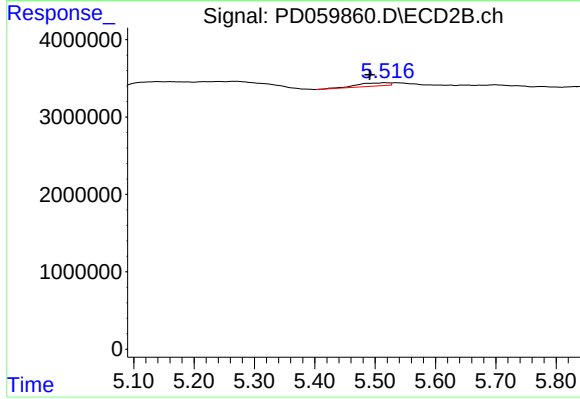

#24 Chlordane-2


R.T.: 5.517 min
Delta R.T.: 0.026 min
Response: 1517702
Conc: 15.40 ng/ml

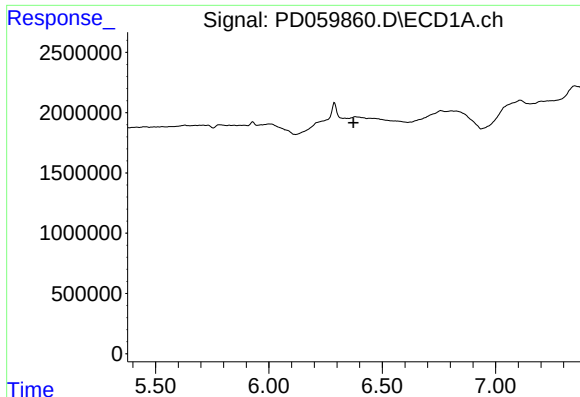

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.373 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

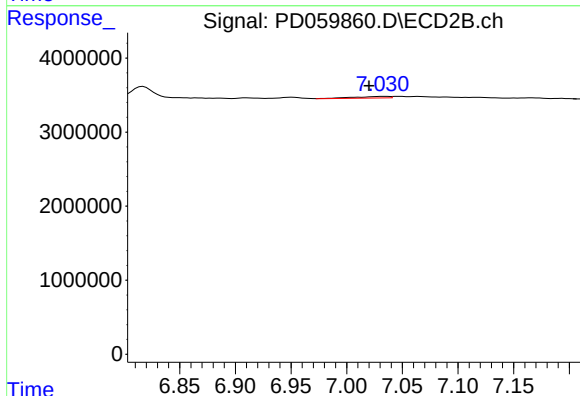


#27 Chlordane-5

R.T.: 7.032 min
Delta R.T.: 0.012 min
Response: 489098
Conc: 5.94 ng/ml

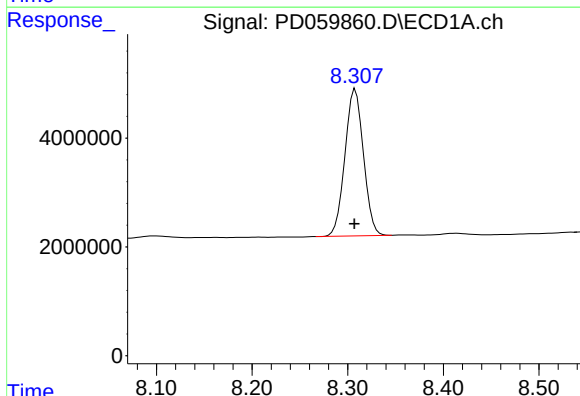

#28 Decachlorobiphenyl

R.T.: 8.308 min
Delta R.T.: 0.000 min
Response: 36409511
Conc: 23.55 ng/ml

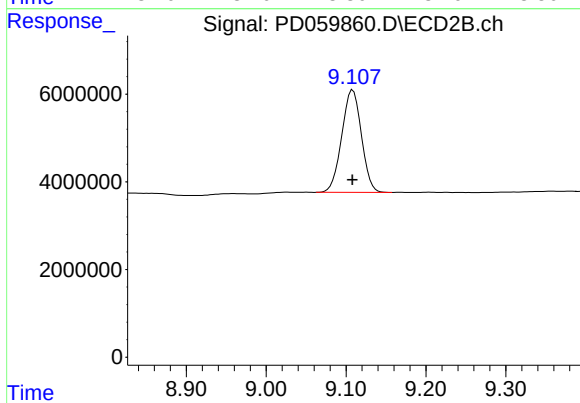

#28 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: 0.000 min
Response: 40095162
Conc: 22.14 ng/ml