

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102120\
 Data File : PD059876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 04:50
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 07:42:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:13:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.024	30469175	50675559	20.520	20.646
28)	SA Decachlor...	8.306	9.107	38282982	42544136	24.761	23.493
Target Compounds							
2)	A alpha-BHC	3.962	0.000	702486	0	0.291	N.D. #
5)	MB Aldrin	0.000	5.508	0	770072	N.D.	0.245 #
8)	B Heptachlo...	0.000	5.895	0	1852760	N.D.	0.675 #
15)	B Endosulfa...	0.000	6.952	0	828533	N.D.	0.319 #
18)	B Endrin al...	0.000	7.059	0	126847	N.D.	0.061 #
22)	Mirex	7.448	0.000	1042509	0	0.728	N.D. #
23)	Chlordane-1	4.414f	0.000	3851629	0	62.658	N.D. #
24)	Chlordane-2	0.000	5.486	0	1013777	N.D.	10.287 #
27)	Chlordane-5	0.000	6.998f	0	522411	N.D.	6.344 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102120\
Data File : PD059876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 04:50
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 07:42:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:13:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

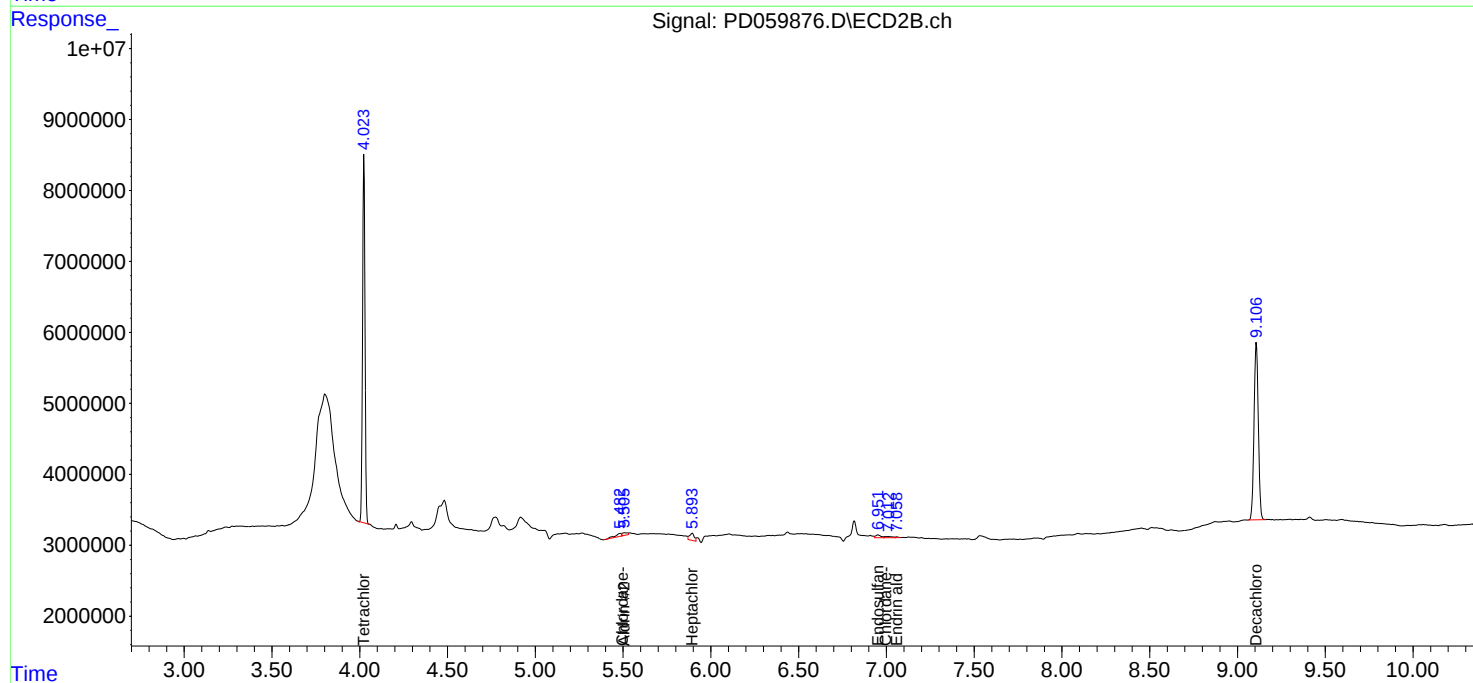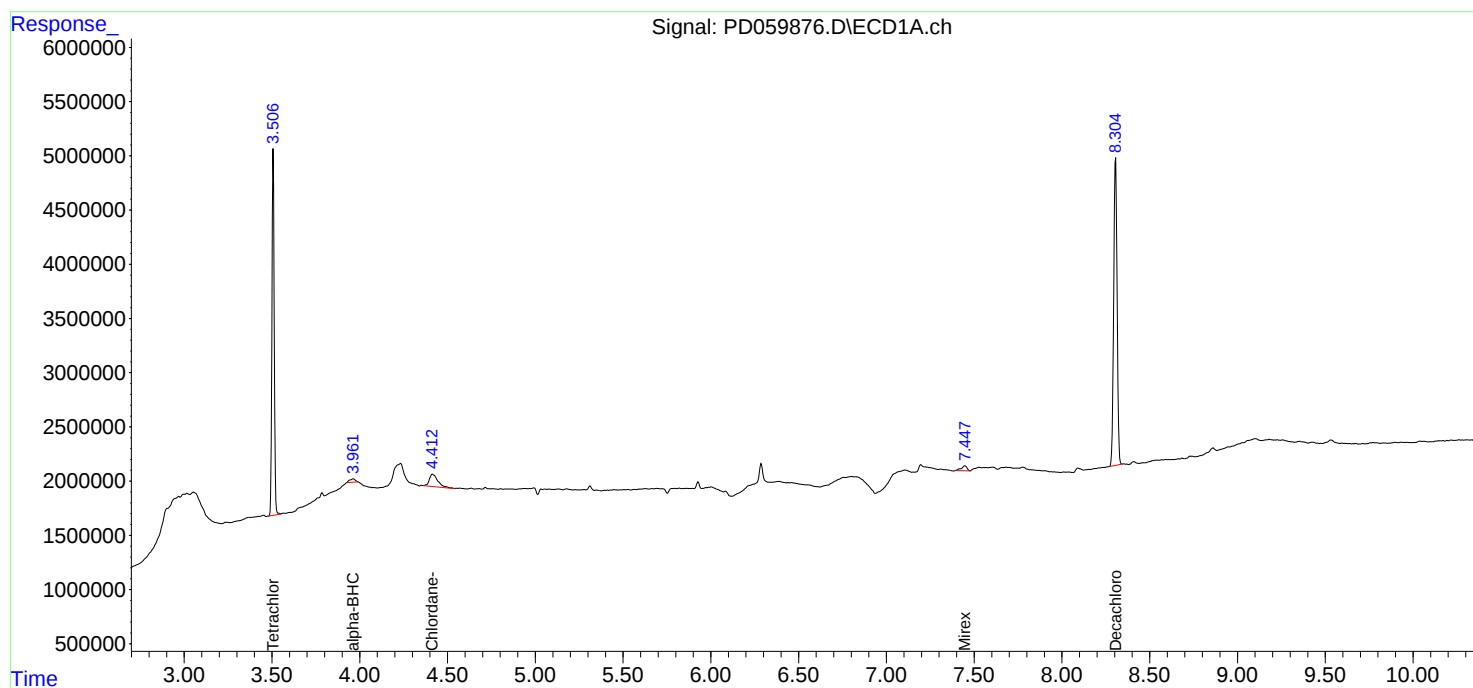


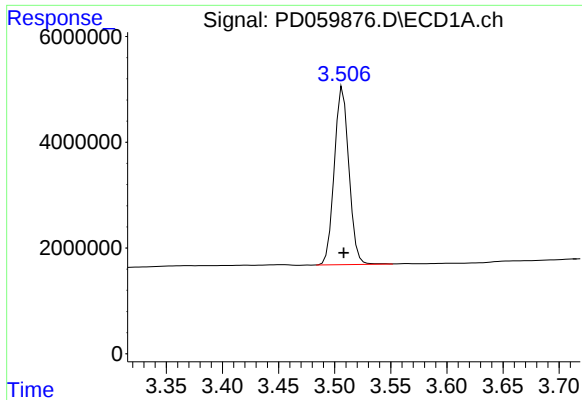

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 30469175
Conc: 20.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

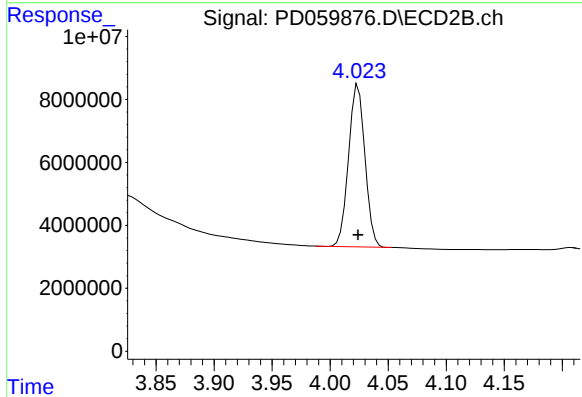


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 50675559
Conc: 20.65 ng/ml

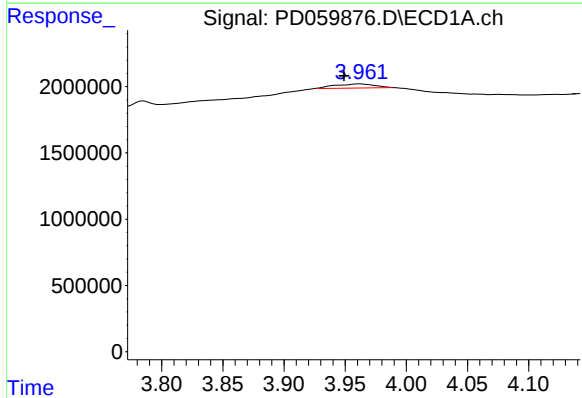


#2 alpha-BHC

R.T.: 3.962 min
Delta R.T.: 0.013 min
Response: 702486
Conc: 0.29 ng/ml

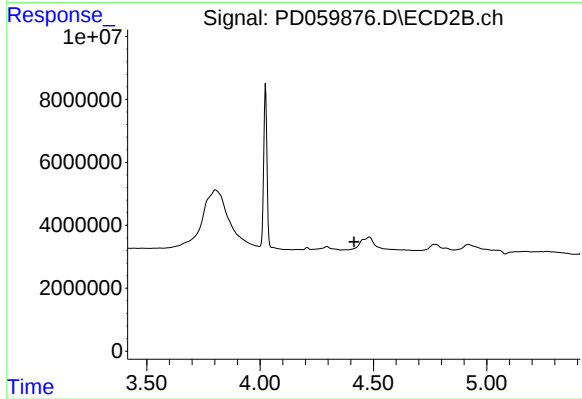

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.415 min
Response: 0
Conc: N.D.

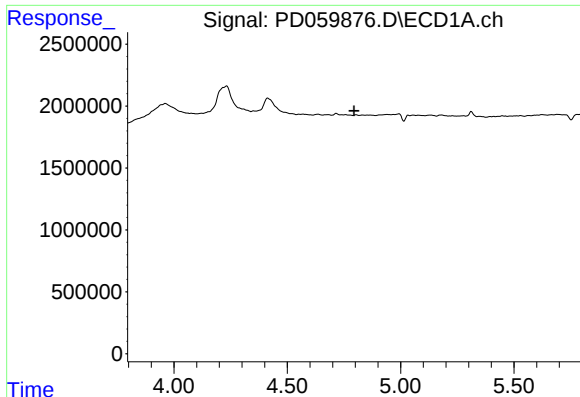

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

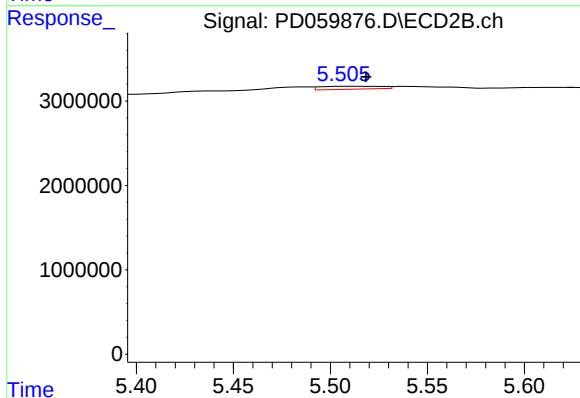


#5 Aldrin

R.T.: 5.508 min
Delta R.T.: -0.010 min
Response: 770072
Conc: 0.25 ng/ml

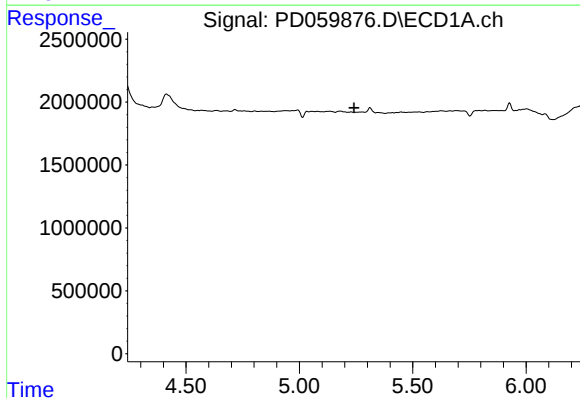


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.242 min
Response: 0
Conc: N.D.

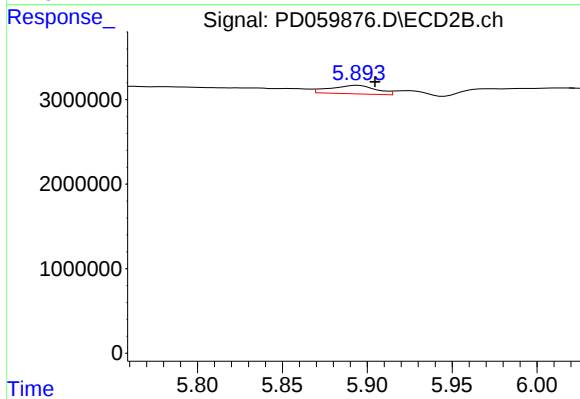

#8 Heptachlor epoxide


R.T.: 5.895 min
Delta R.T.: -0.010 min
Response: 1852760
Conc: 0.67 ng/ml

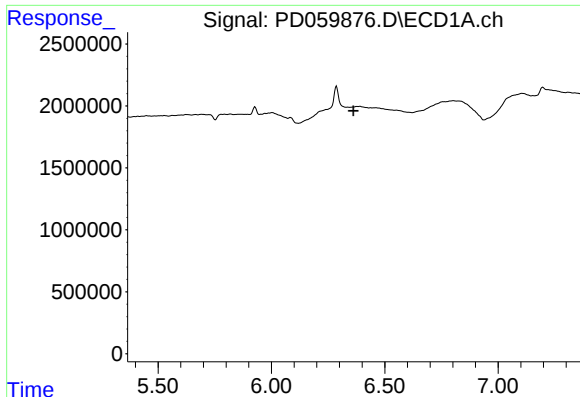

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

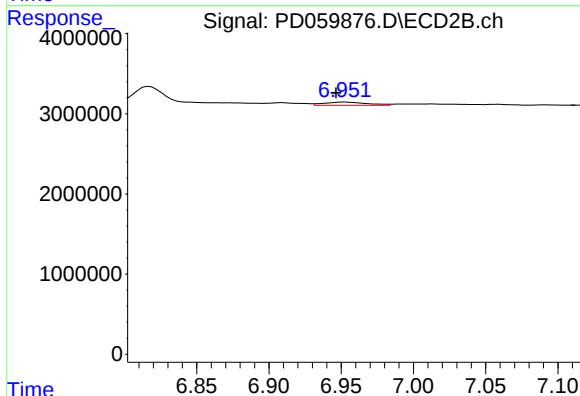


#15 Endosulfan II

R.T.: 6.952 min
Delta R.T.: 0.006 min
Response: 828533
Conc: 0.32 ng/ml

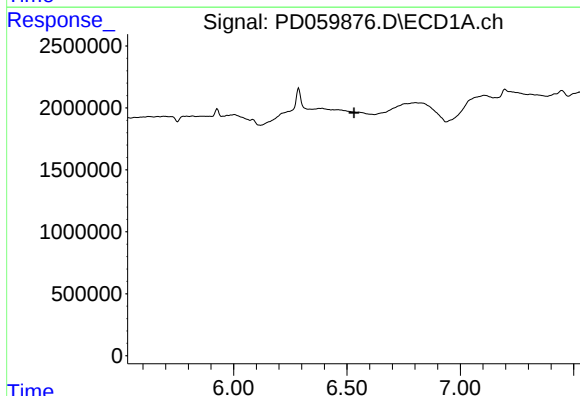


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

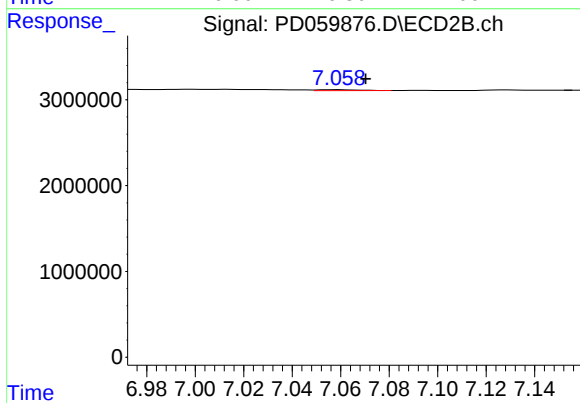

#18 Endrin aldehyde


R.T.: 7.059 min
Delta R.T.: -0.011 min
Response: 126847
Conc: 0.06 ng/ml

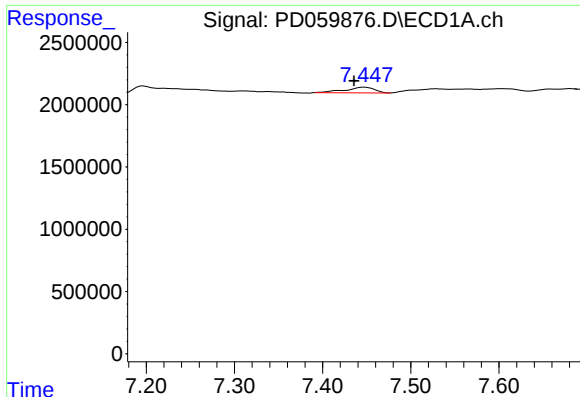

#22 Mirex


R.T.: 7.448 min
Delta R.T.: 0.012 min
Response: 1042509
Conc: 0.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

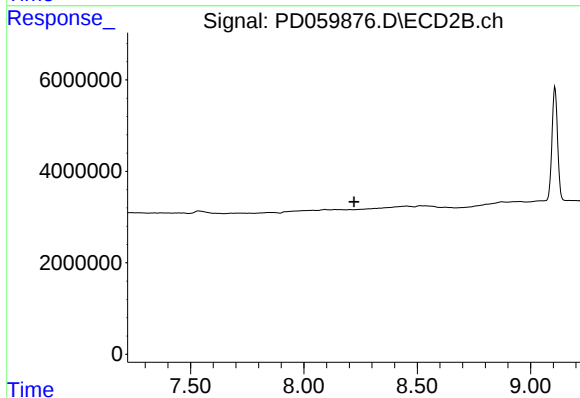


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.221 min
Response: 0
Conc: N.D.

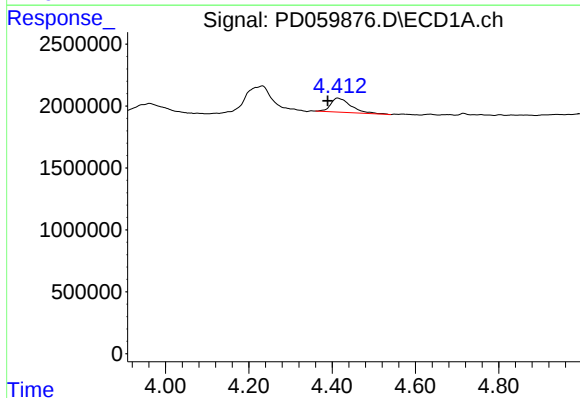


#23 Chlordane-1

R.T.: 4.414 min
Delta R.T.: 0.024 min
Response: 3851629
Conc: 62.66 ng/ml

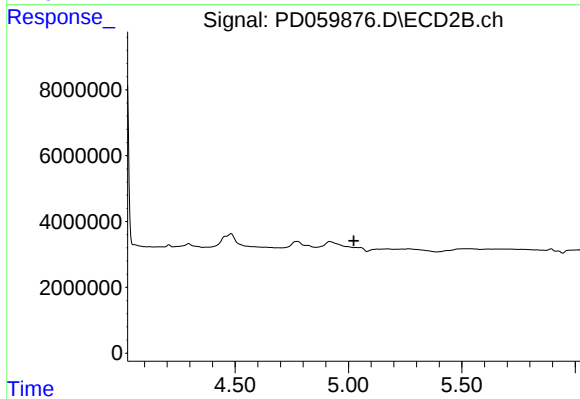

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.023 min
Response: 0
Conc: N.D.

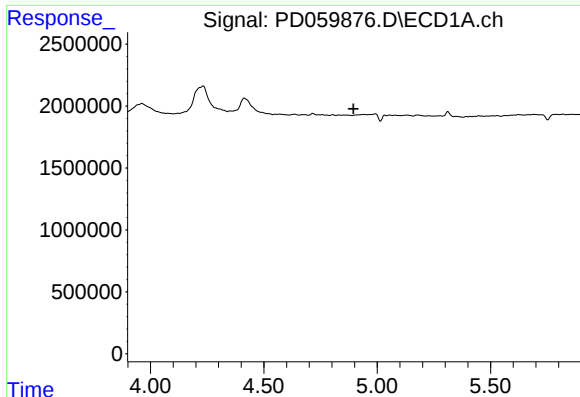

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.896 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

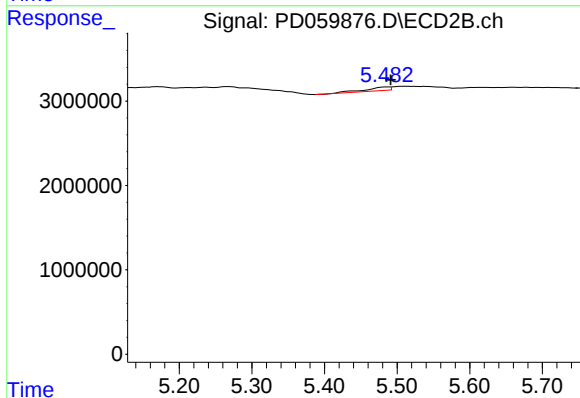


#24 Chlordane-2

R.T.: 5.486 min
Delta R.T.: -0.006 min
Response: 1013777
Conc: 10.29 ng/ml

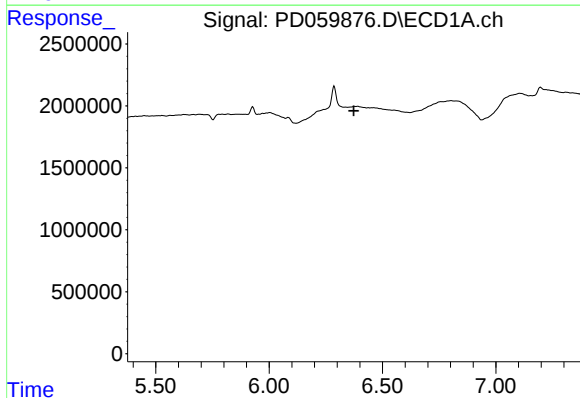


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.373 min
Response: 0
Conc: N.D.

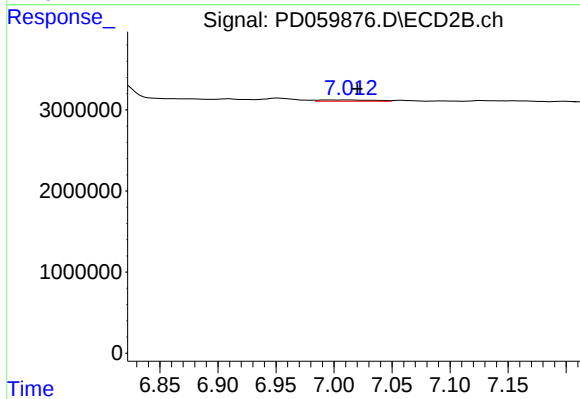

#27 Chlordane-5

R.T.: 6.998 min
Delta R.T.: -0.023 min
Response: 522411
Conc: 6.34 ng/ml

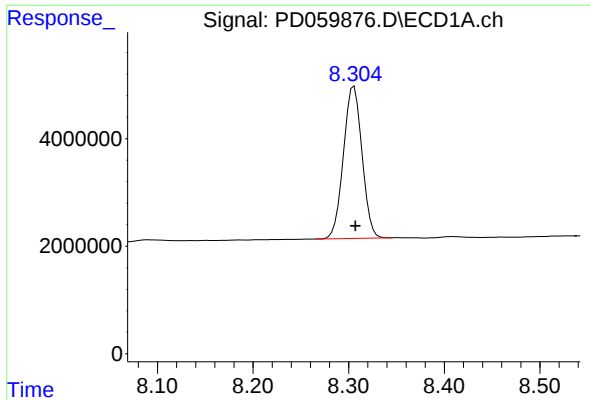

#28 Decachlorobiphenyl


R.T.: 8.306 min

Delta R.T.: -0.001 min

Response: 38282982

Conc: 24.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

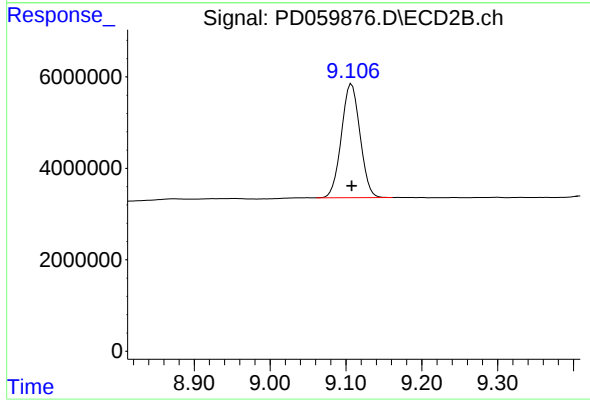

#28 Decachlorobiphenyl

R.T.: 9.107 min

Delta R.T.: 0.000 min

Response: 42544136

Conc: 23.49 ng/ml