

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102120\
 Data File : PD059875.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 04:36
 Operator : DD\AJ
 Sample : L4214-09
 Misc : TOX MDL 25PPB (Sig #1); TOX MDL 25 PPB (Sig #2)
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-03-QT4-2020

Manual Integrations
 APPROVED

Ankita
 10/21/2020 2:02:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 08:26:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:47:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.507	4.024	30247882	50767895	20.500	20.813
7) SA Decachlor...	8.306	9.107	38521418	42812457	24.546	23.400
Target Compounds						
2) Toxaphene-1	6.006	6.608	1542265	1588085	80.055	60.731m
3) Toxaphene-2	6.395	6.909	1994282	1349694	60.679	51.398m
4) Toxaphene-3	6.645	7.193	1744111	3836210	57.273	62.130
5) Toxaphene-4	6.789	7.279	672023	2315728	58.609	59.998
6) Toxaphene-5	7.068	7.693	851771	1769925	65.078m	64.106

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102120\
Data File : PD059875.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 04:36
Operator : DD\AJ
Sample : L4214-09
Misc : TOX MDL 25PPB (Sig #1); TOX MDL 25 PPB (Sig #2)
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 08:26:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:47:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

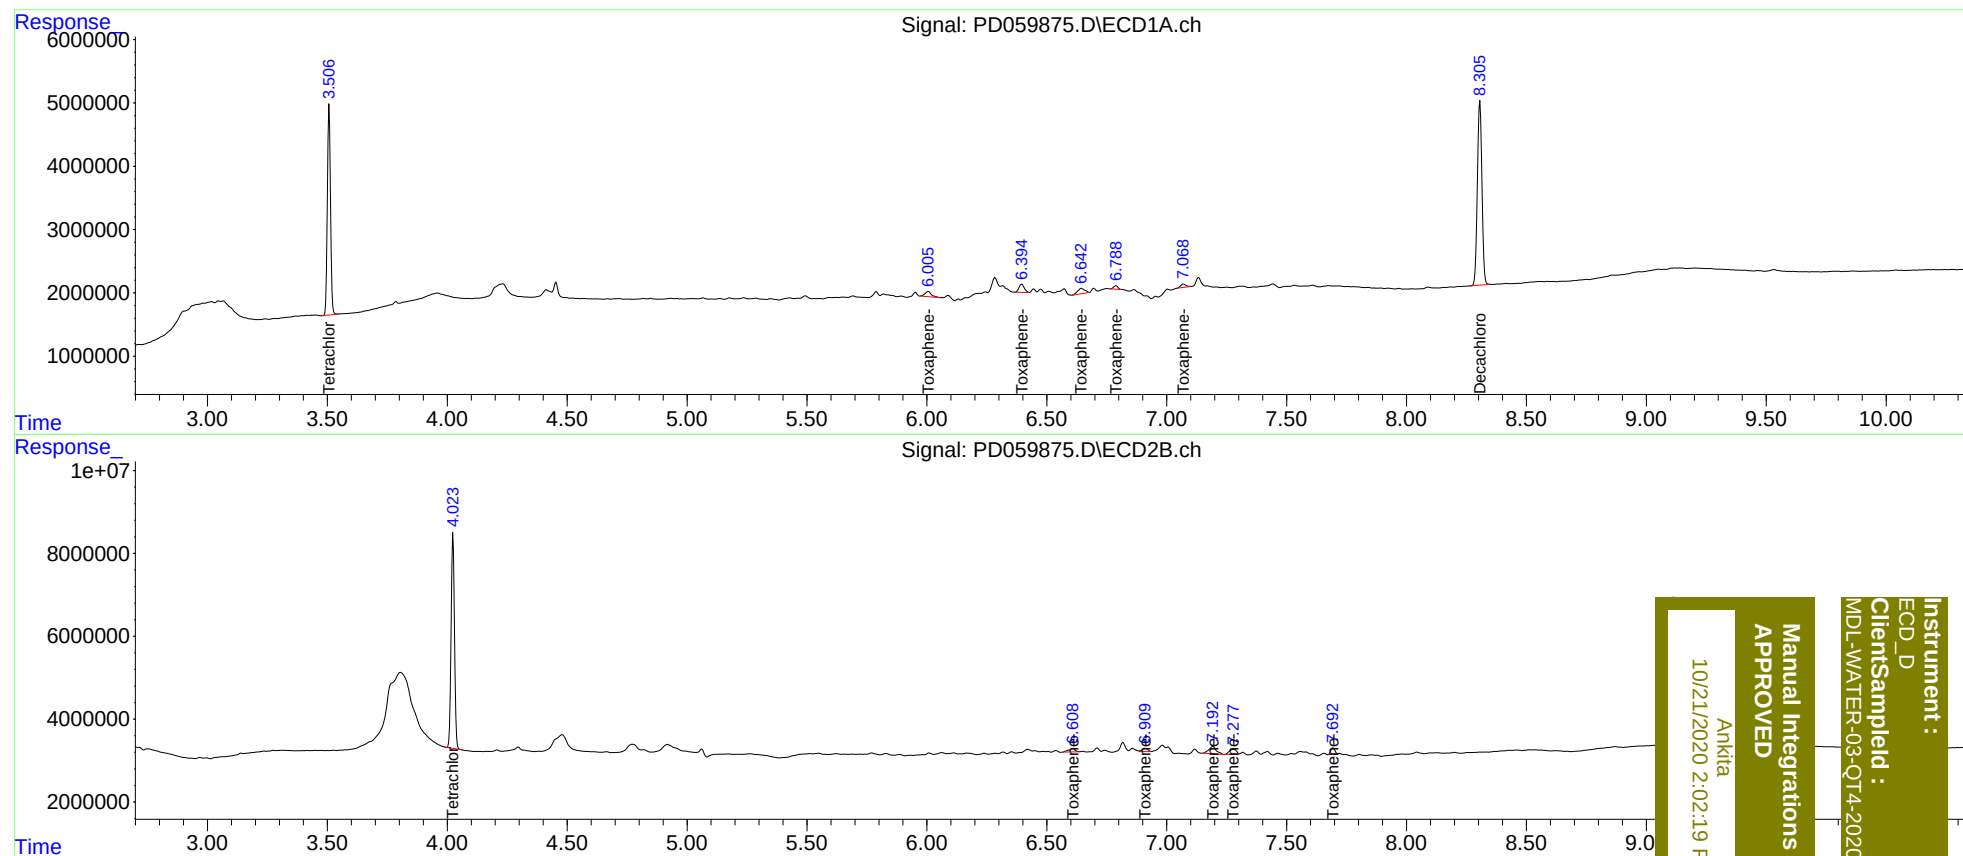

Manual Integrations
APPROVED

Ankita
10/21/2020 2:02:19 PM

Instrument :
ECD_D
Client Sample :
MDL-WATER-03-QT4-2020