

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102120\
 Data File : PD059877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 05:05
 Operator : DD\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 08:26:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX101920.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 20 07:47:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.508	4.024	75144151	127.3E6	50.927	52.204
7) SA Decachlor...	8.307	9.107	91863504	102.2E6	58.535	55.845
Target Compounds						
2) Toxaphene-1	6.007	6.609	9666996	13704643	501.786	524.086
3) Toxaphene-2	6.396	6.908	16532040	13547021	503.010	515.887
4) Toxaphene-3	6.645	7.194	16751670	31546588	550.090	510.922
5) Toxaphene-4	6.789	7.280	6177579	20197956	538.761	523.307
6) Toxaphene-5	7.070	7.694	6645476	15446114	507.736	559.453

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102120\
Data File : PD059877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 05:05
Operator : DD\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 08:26:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX101920.M
Quant Title : GC Extractables
QLast Update : Tue Oct 20 07:47:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

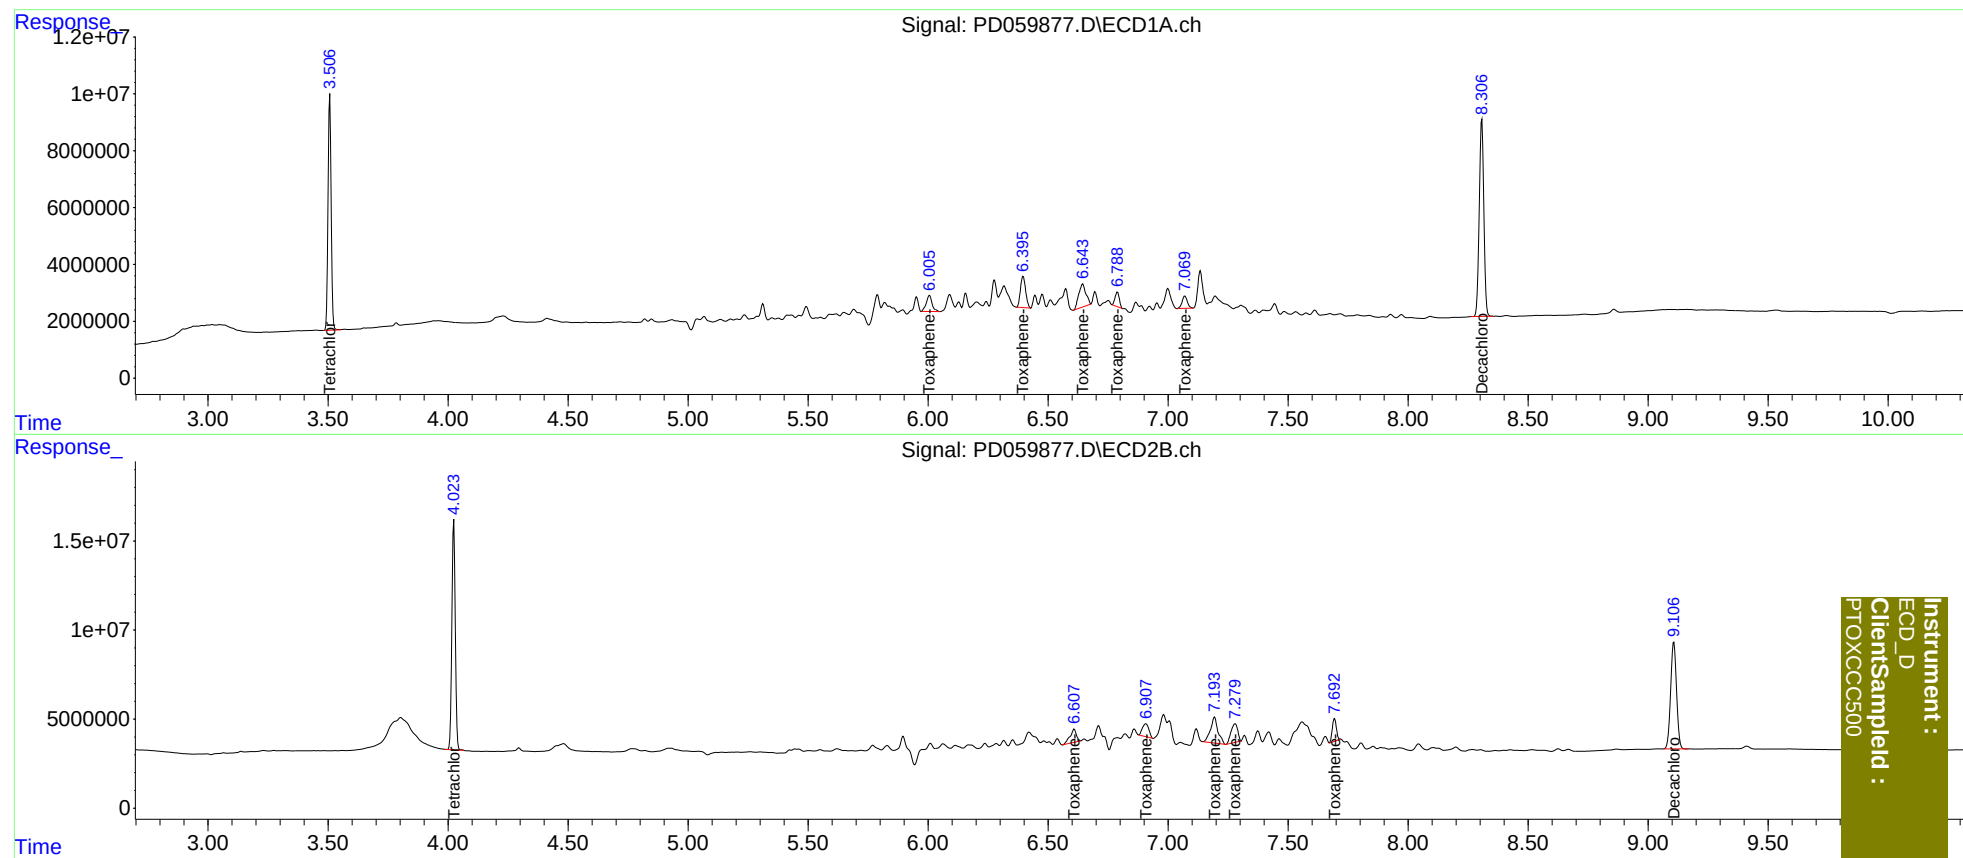

Instrument :
ECD_D
ClientSampled :
PTOXCCC500