

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102123\
 Data File : PD079026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2023 14:43
 Operator : AR\AJ
 Sample : PB156541BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 22:28:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.576	2.803	28986174	42052560	18.900	19.392
2) SA Decachlor...	9.129	7.958	39692030	49725447	20.927	21.321
Target Compounds						
3) MA gamma-BHC...	0.000	3.658	0	311999	N.D.	<MDL
7) B delta-BHC	4.807	0.000	2736610	0	1.043	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102123\
Data File : PD079026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2023 14:43
Operator : AR\AJ
Sample : PB156541BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 22:28:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

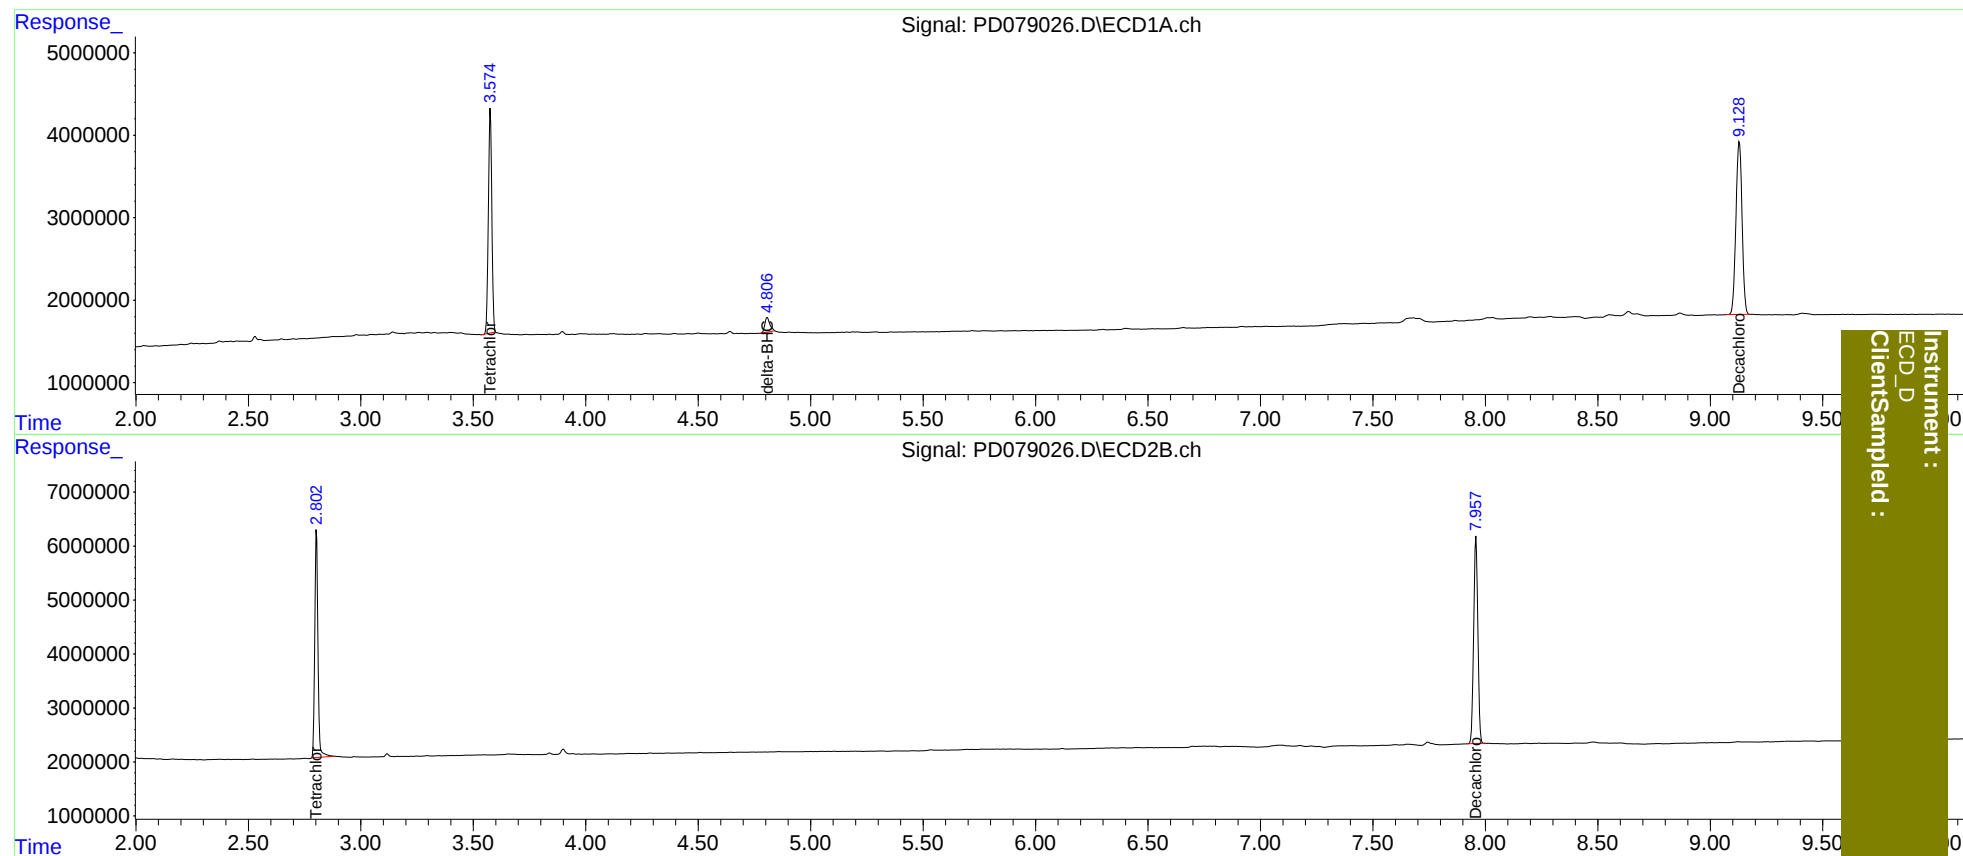


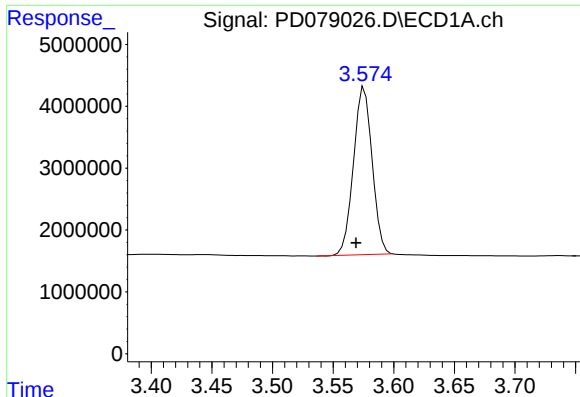

#1 Tetrachloro-m-xylene


R.T.: 3.576 min
Delta R.T.: 0.007 min
Response: 28986174
Conc: 18.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

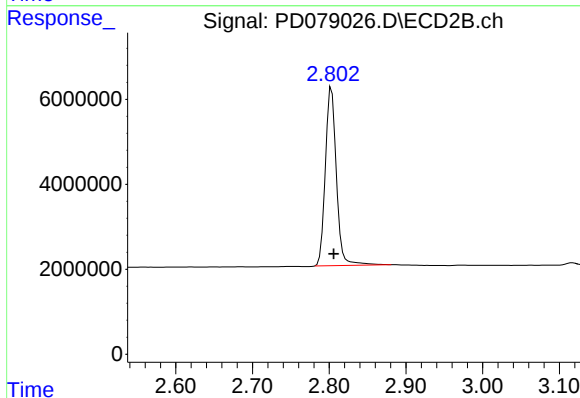


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: -0.003 min
Response: 42052560
Conc: 19.39 ng/ml

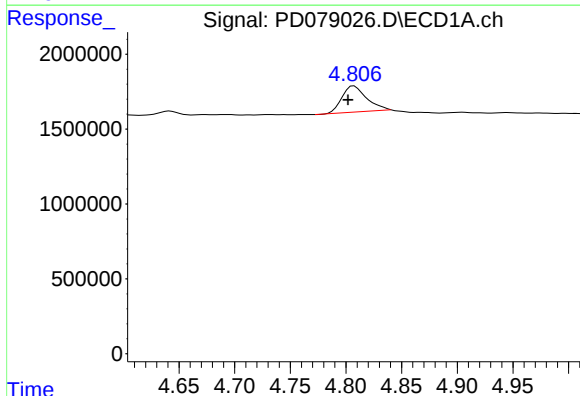


#7 delta-BHC

R.T.: 4.807 min
Delta R.T.: 0.005 min
Response: 2736610
Conc: 1.04 ng/ml

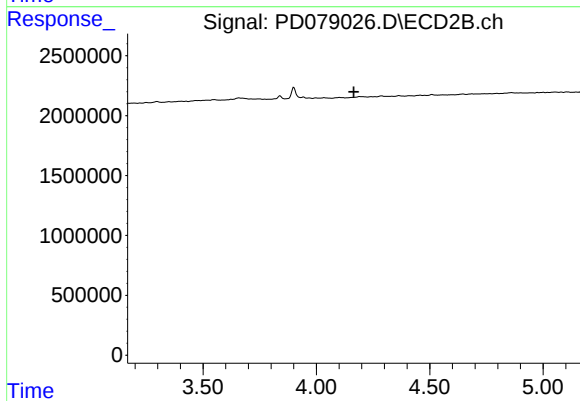

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.166 min
Response: 0
Conc: N.D.

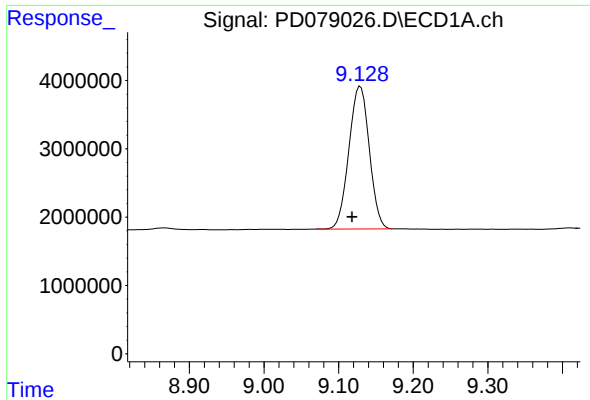

#27 Decachlorobiphenyl

R.T.: 9.129 min
Delta R.T.: 0.011 min
Response: 39692030
Conc: 20.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

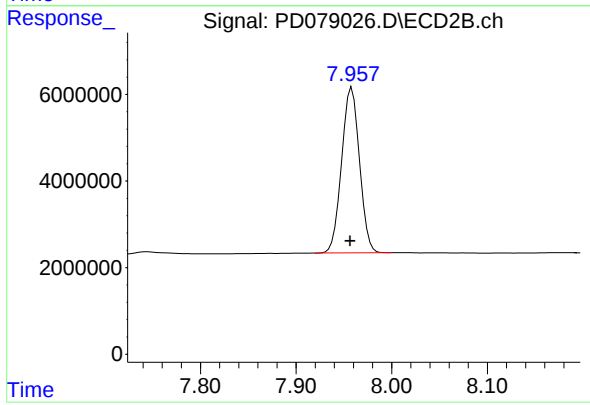

#27 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: 0.002 min
Response: 49725447
Conc: 21.32 ng/ml