

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102123\
 Data File : PD079052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2023 21:01
 Operator : AR\AJ
 Sample : PB156546BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 22:34:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.807	29110695	41070516	18.981	18.939
2)	SA Decachlor...	9.120	7.957	37861556	47395247	19.962	20.321
Target Compounds							
2)	A alpha-BHC	0.000	3.299	0	120812	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.661	0	265343	N.D.	<MDL
7)	B delta-BHC	4.798	0.000	3936295	0	1.500	N.D. #
15)	B Endosulfa...	0.000	5.935	0	77652	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102123\
Data File : PD079052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2023 21:01
Operator : AR\AJ
Sample : PB156546BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 22:34:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

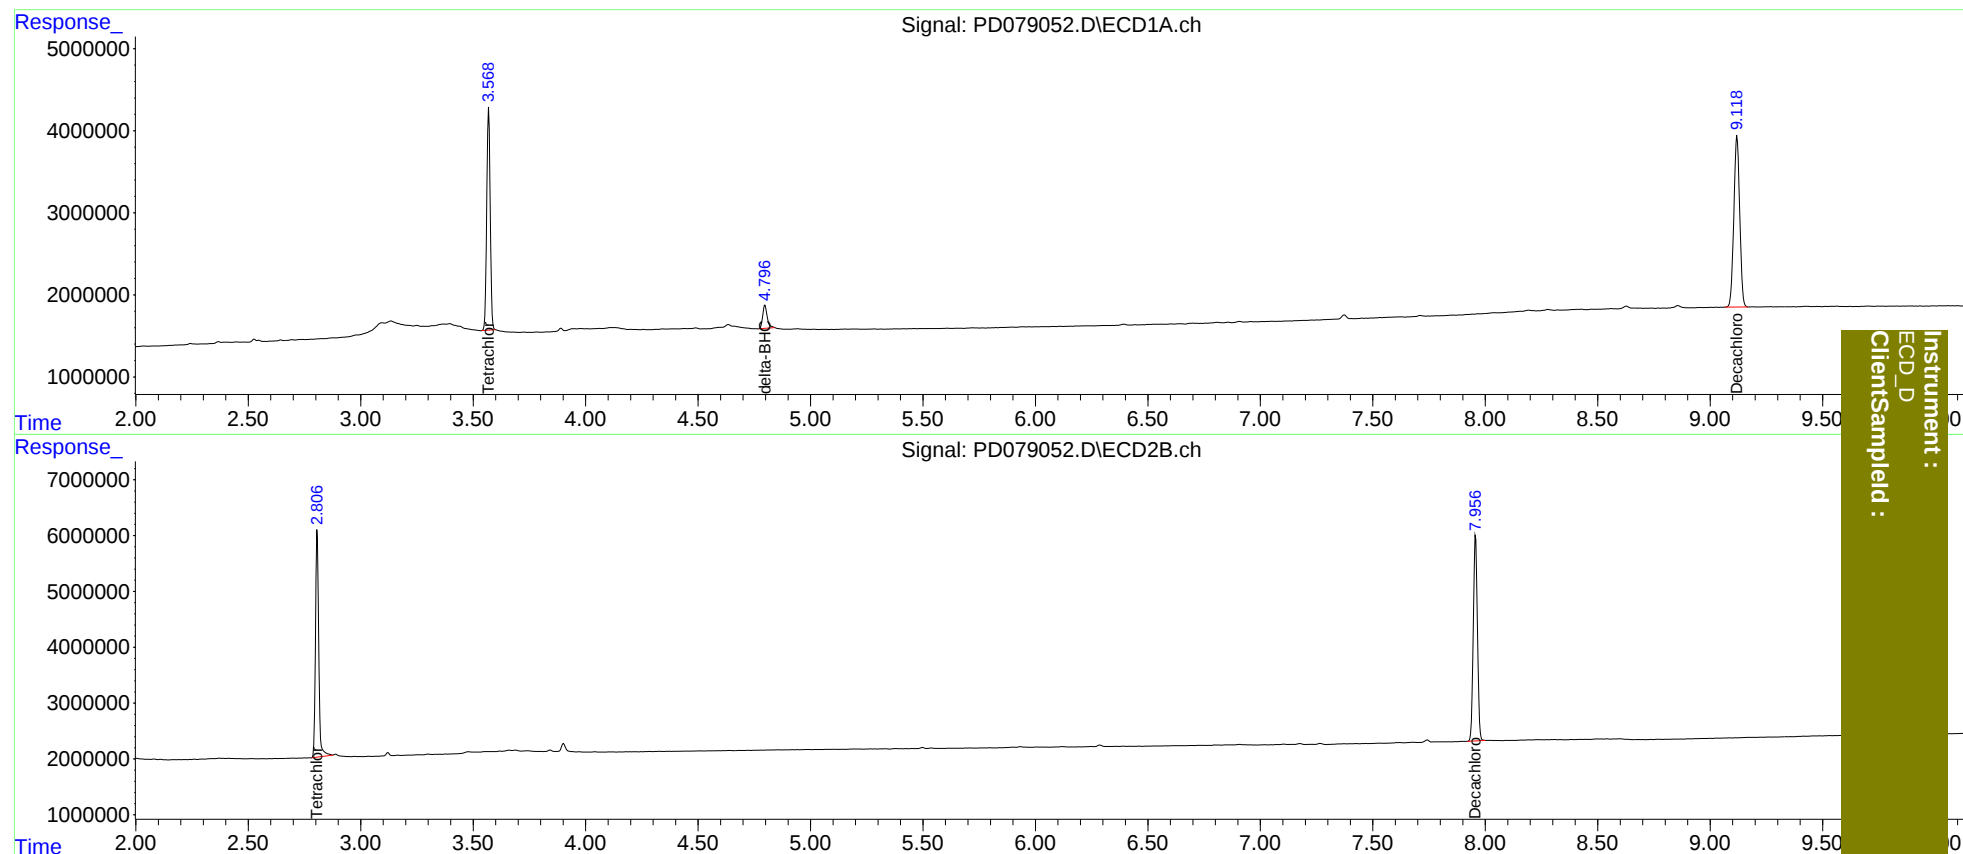


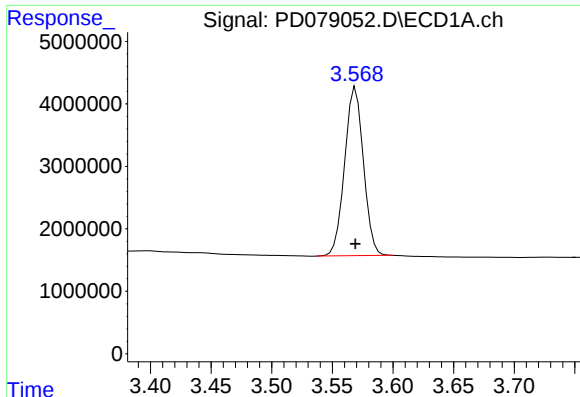

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 29110695
Conc: 18.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

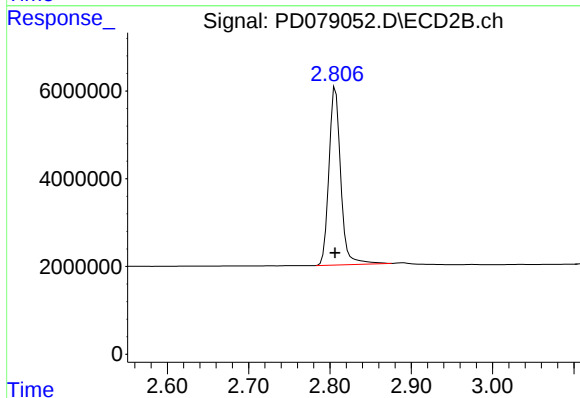


#1 Tetrachloro-m-xylene

R.T.: 2.807 min
Delta R.T.: 0.000 min
Response: 41070516
Conc: 18.94 ng/ml

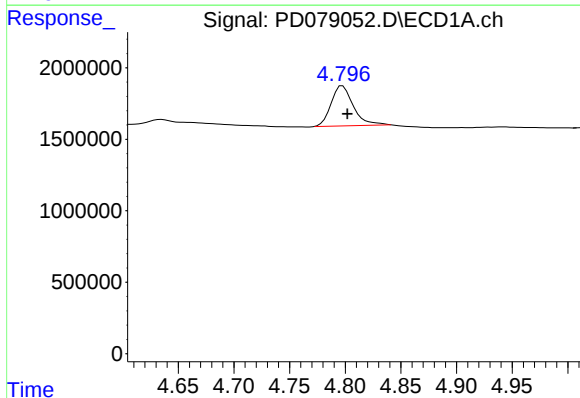


#7 delta-BHC

R.T.: 4.798 min
Delta R.T.: -0.004 min
Response: 3936295
Conc: 1.50 ng/ml

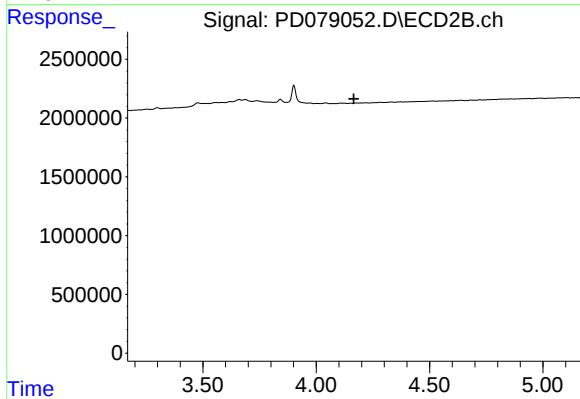

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.166 min
Response: 0
Conc: N.D.

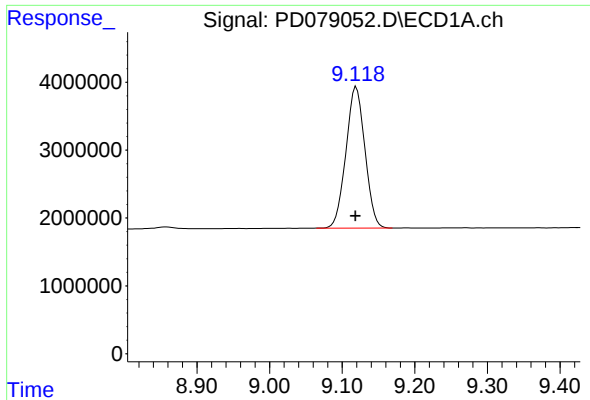

#27 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.001 min
Response: 37861556
Conc: 19.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

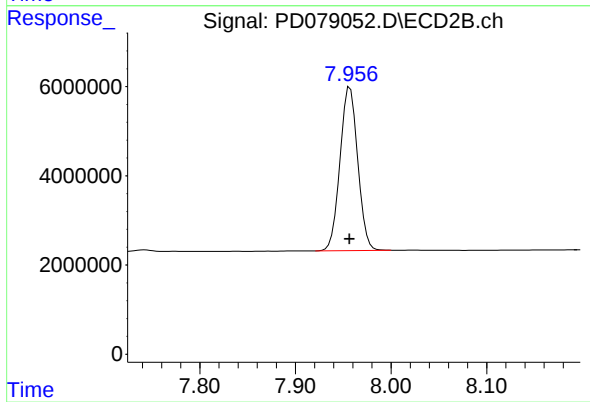

#27 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: 0.000 min
Response: 47395247
Conc: 20.32 ng/ml