

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102123\
 Data File : PD079061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2023 23:02
 Operator : AR\AJ
 Sample : 04950-21MS
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A49M0MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 03:04:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.807	28968264	38633062	18.888	17.815
2)	SA Decachlor...	9.119	7.958	31851139	40705995	16.793	17.453
Target Compounds							
2)	A alpha-BHC	4.027	3.311	122.0E6	163.1E6	46.806	47.831
3)	MA gamma-BHC...	4.360	3.640	111.8E6	148.0E6	44.915	45.788
4)	MA Heptachlor	4.954	3.983	116.0E6	139.0E6	43.554	45.725
5)	MB Aldrin	5.297	4.265	109.1E6	137.6E6	44.146	44.673
6)	B beta-BHC	4.553	3.935	48275101	63096181	42.335	43.625
7)	B delta-BHC	4.803	4.166	85077830	107.5E6	32.428	32.785
8)	B Heptachlo...	5.724	4.767	103.4E6	132.6E6	43.046	45.959
9)	A Endosulfan I	6.110	5.138	97344544	123.2E6	45.440	48.512
10)	B trans-Chl...	5.980	5.018	98777519	129.9E6	44.593	46.907
11)	B cis-Chlor...	6.060	5.081	100.3E6	130.6E6	44.117	46.109
12)	B 4,4'-DDE	6.230	5.271	192.1E6	252.1E6	93.241	96.417
13)	MA Dieldrin	6.386	5.403	210.3E6	279.1E6	92.575	94.758
14)	MA Endrin	6.617	5.678	180.5E6	249.3E6	95.319	98.788
15)	B Endosulfa...	6.834	5.970	180.0E6	232.4E6	90.768	97.677
16)	A 4,4'-DDD	6.747	5.825	156.6E6	208.5E6	93.167	94.385
17)	MA 4,4'-DDT	7.063	6.077	169.9E6	217.5E6	94.862	96.518
18)	B Endrin al...	6.964	6.149	129.9E6	168.0E6	85.615	90.647
19)	B Endosulfa...	7.198	6.372	163.3E6	205.3E6	84.993	89.059
20)	A Methoxychlor	7.537	6.652	431.3E6	539.8E6	449.554	442.714
21)	B Endrin ke...	7.686	6.878	183.6E6	251.0E6	87.888	95.099

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102123\
Data File : PD079061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2023 23:02
Operator : AR\AJ
Sample : 04950-21MS
Misc :
ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 03:04:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

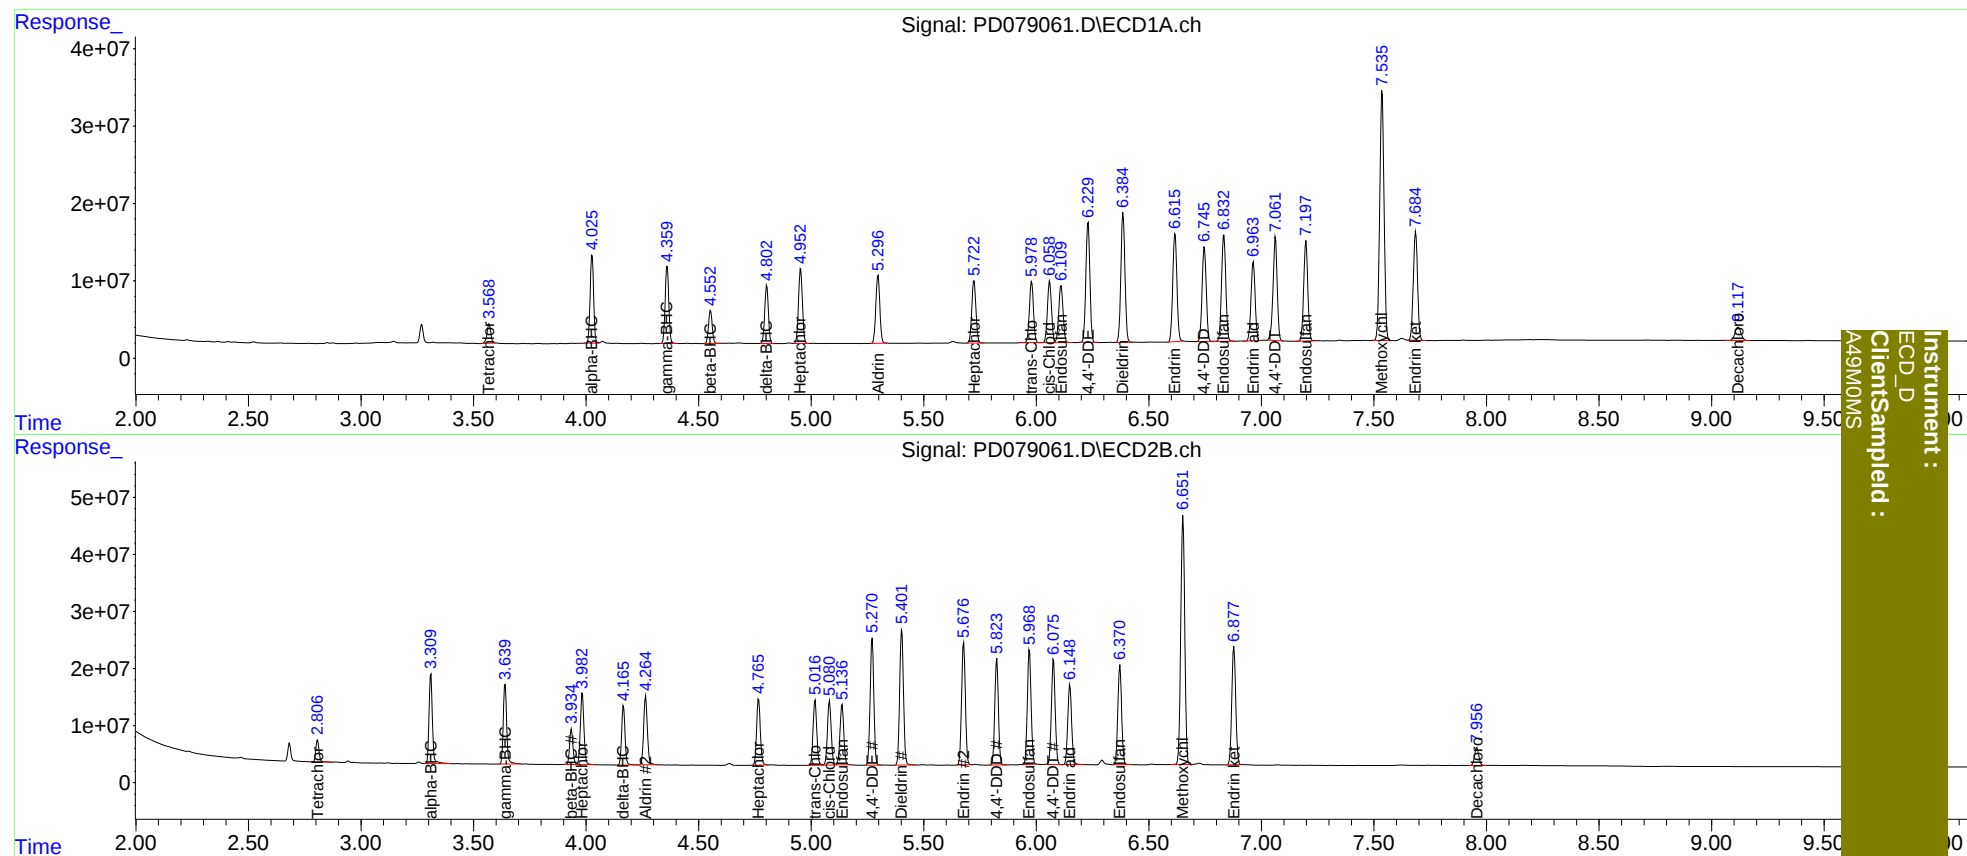

Instrument :
ECD_D
ClientSampled :
A49M0MS