

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102123\
 Data File : PD079062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2023 23:15
 Operator : AR\AJ
 Sample : 04950-22MSD
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A49M0MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 03:04:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.807	28952044	38826136	18.877	17.904
2)	SA Decachlor...	9.119	7.958	32349569	40514582	17.056	17.371
Target Compounds							
2)	A alpha-BHC	4.027	3.310	121.5E6	162.6E6	46.649	47.674
3)	MA gamma-BHC...	4.360	3.640	111.5E6	147.4E6	44.796	45.592
4)	MA Heptachlor	4.954	3.984	116.0E6	138.9E6	43.527	45.691
5)	MB Aldrin	5.297	4.265	109.0E6	137.3E6	44.096	44.567
6)	B beta-BHC	4.553	3.935	48087310	62717380	42.171	43.363
7)	B delta-BHC	4.803	4.167	84958695	107.1E6	32.382	32.673
8)	B Heptachlo...	5.724	4.767	102.9E6	132.1E6	42.860	45.761
9)	A Endosulfan I	6.110	5.138	96964670	122.6E6	45.263	48.278
10)	B trans-Chl...	5.979	5.017	98673116	129.4E6	44.546	46.728
11)	B cis-Chlor...	6.059	5.082	99943904	130.0E6	43.967	45.913
12)	B 4,4'-DDE	6.230	5.271	191.5E6	251.3E6	92.960	96.103
13)	MA Dieldrin	6.386	5.403	209.1E6	278.1E6	92.062	94.421
14)	MA Endrin	6.616	5.677	179.6E6	248.5E6	94.871	98.480
15)	B Endosulfa...	6.834	5.970	179.3E6	231.1E6	90.412	97.111
16)	A 4,4'-DDD	6.747	5.825	156.1E6	207.6E6	92.859	93.976
17)	MA 4,4'-DDT	7.062	6.077	168.9E6	216.3E6	94.342	96.010
18)	B Endrin al...	6.964	6.150	129.2E6	167.0E6	85.214	90.119
19)	B Endosulfa...	7.198	6.372	162.6E6	204.1E6	84.588	88.542
20)	A Methoxychlor	7.537	6.653	429.9E6	536.3E6	448.170	439.814
21)	B Endrin ke...	7.686	6.879	183.2E6	249.1E6	87.678	94.376

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102123\
Data File : PD079062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2023 23:15
Operator : AR\AJ
Sample : 04950-22MSD
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 03:04:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

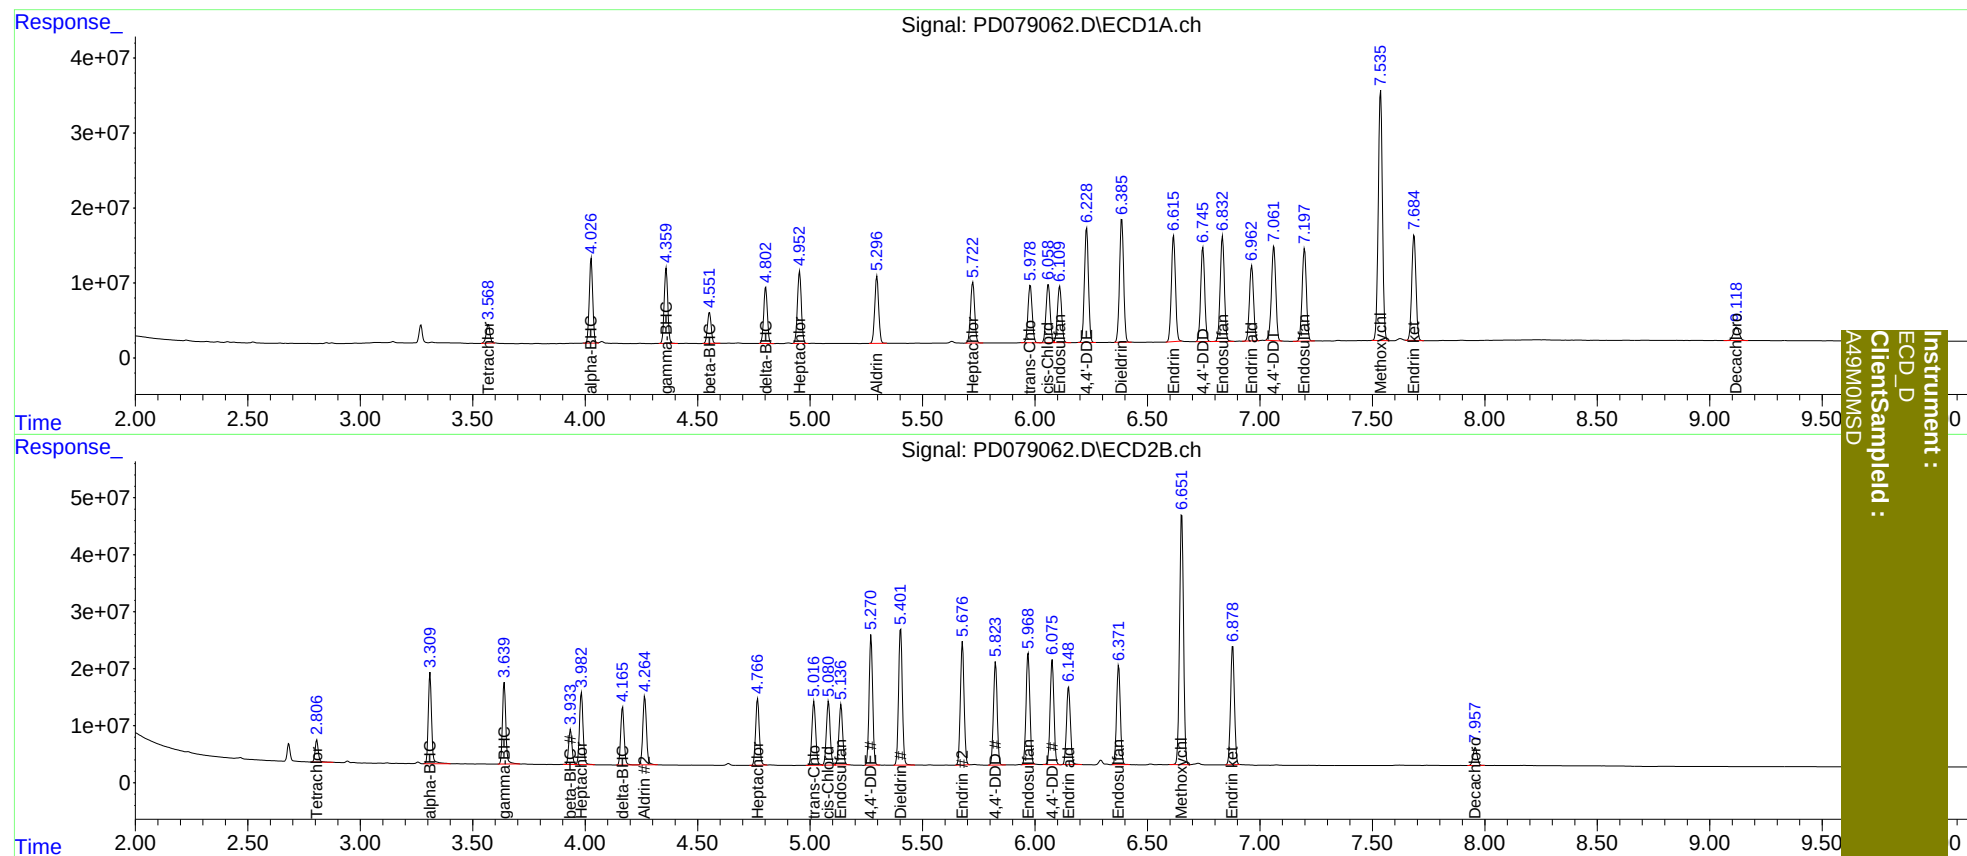

Instrument :
ECD_D
ClientSampled :
A49M0MSD