

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102123\
 Data File : PD079020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2023 11:32
 Operator : AR\AJ
 Sample : 04952-08MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAR8MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 22:24:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.807	29858876	39257053	19.469	18.103
2)	SA Decachlor...	9.120	7.959	33396422	40518214	17.608	17.373
Target Compounds							
2)	A alpha-BHC	4.027	3.311	118.7E6	156.8E6	45.575	45.983
3)	MA gamma-BHC...	4.360	3.641	108.4E6	141.5E6	43.542	43.789
4)	MA Heptachlor	4.954	3.984	111.7E6	135.1E6	41.930	44.415
5)	MB Aldrin	5.298	4.265	107.0E6	128.1E6	43.271	41.572
6)	B beta-BHC	4.553	3.935	46356284	58347126	40.653	40.341
7)	B delta-BHC	4.803	4.167	81645595	102.9E6	31.119	31.388
8)	B Heptachlo...	5.724	4.768	100.3E6	129.0E6	41.786	44.693
9)	A Endosulfan I	6.111	5.138	94660368	119.8E6	44.187	47.190
10)	B trans-Chl...	5.980	5.018	97086734	125.4E6	43.829	45.264
11)	B cis-Chlor...	6.060	5.083	97526304	126.6E6	42.904	44.720
12)	B 4,4'-DDE	6.231	5.272	188.9E6	246.5E6	91.701	94.256
13)	MA Dieldrin	6.387	5.403	205.3E6	273.7E6	90.349	92.917
14)	MA Endrin	6.617	5.678	176.1E6	243.9E6	93.002	96.662
15)	B Endosulfa...	6.835	5.971	175.1E6	227.1E6	88.317	95.449
16)	A 4,4'-DDD	6.748	5.825	152.9E6	203.7E6	90.964	92.213
17)	MA 4,4'-DDT	7.064	6.078	168.2E6	210.3E6	93.961	93.351
18)	B Endrin al...	6.965	6.150	127.8E6	166.2E6	84.287	89.667
19)	B Endosulfa...	7.200	6.373	159.9E6	201.8E6	83.203	87.554
20)	A Methoxychlor	7.537	6.653	425.1E6	533.5E6	443.122	437.556
21)	B Endrin ke...	7.687	6.880	183.8E6	244.5E6	87.967	92.630

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102123\
Data File : PD079020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2023 11:32
Operator : AR\AJ
Sample : 04952-08MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 22:24:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

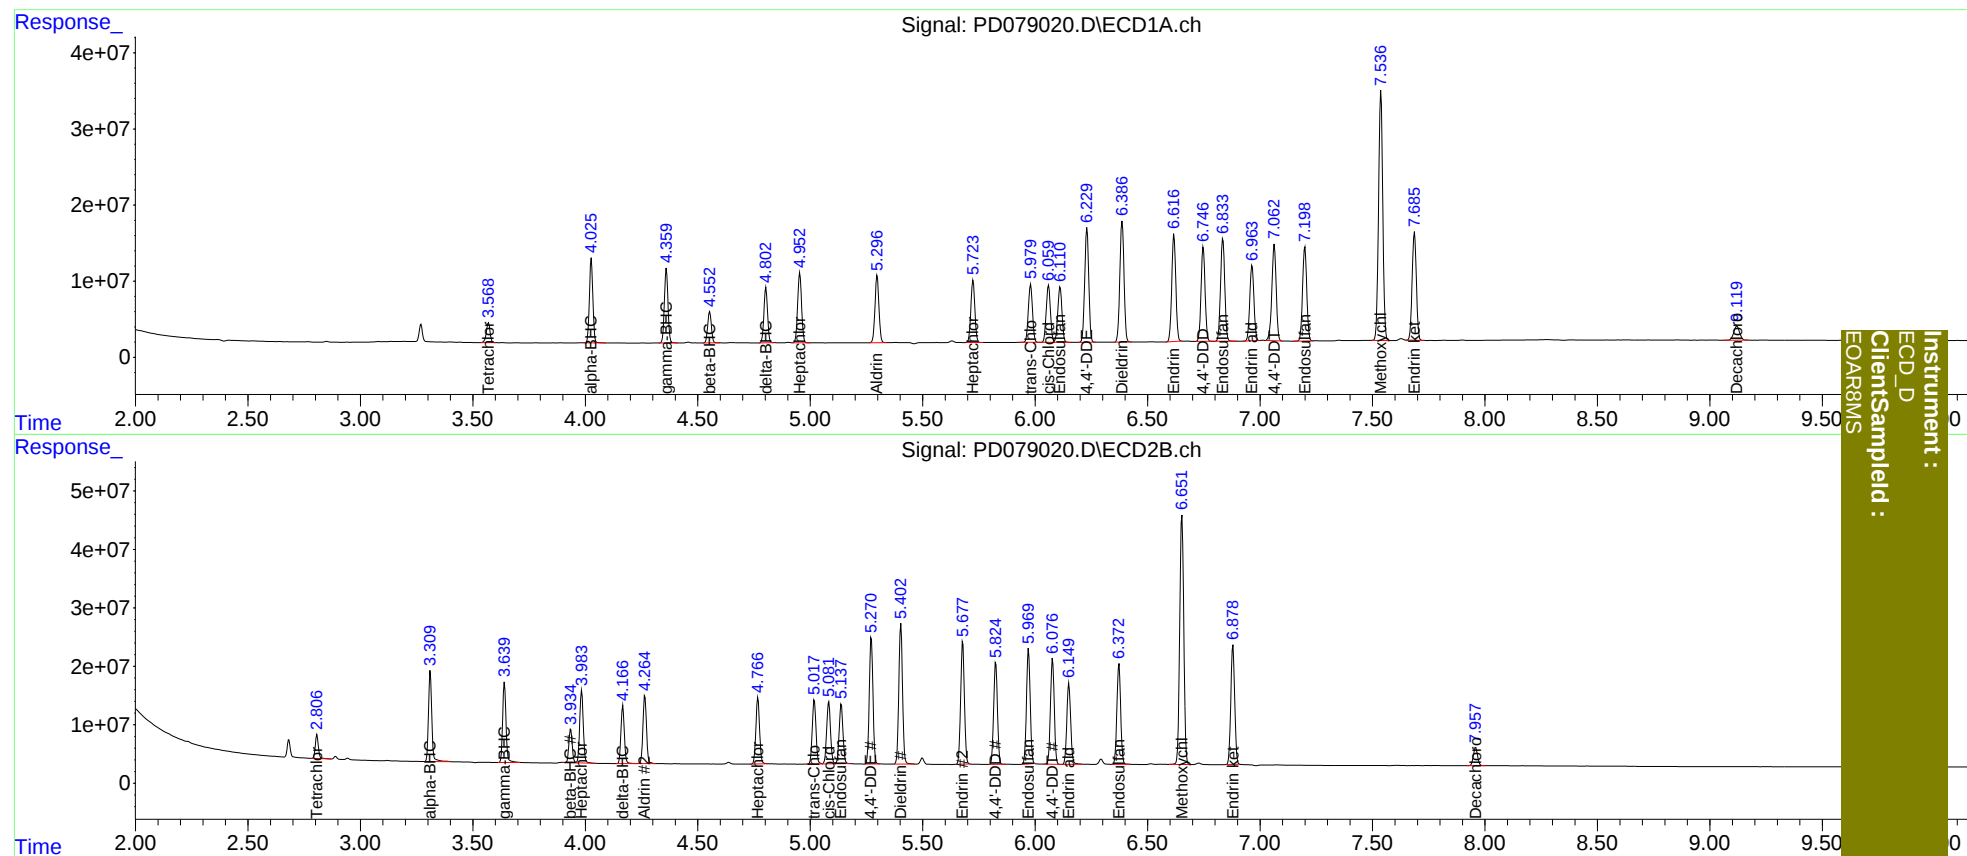

Instrument :
ECD_D
ClientSampled :
EOAR8MS