

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102124\
 Data File : PD086143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2024 20:18
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 06:12:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102124.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 22 06:07:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.381	2.822	160.7E6	1201.0E6	100.277	98.361
28)	SA Decachlor...	8.816	7.976	181.4E6	989.0E6	95.283	97.080
Target Compounds							
23)	Chlordane-1	4.530	3.831	102.4E6	436.5E6	999.792	989.950
24)	Chlordane-2	5.055	4.407	97781073	420.0E6	1019.490	966.905
25)	Chlordane-3	5.755	5.043	438.6E6	1457.1E6	1017.512	972.110
26)	Chlordane-4	5.839	5.106	524.7E6	1228.8E6	1008.345	972.390
27)	Chlordane-5	6.670	6.002	78693502	538.0E6	1032.069	979.712



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102124\
Data File : PD086143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2024 20:18
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 06:12:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102124.M
Quant Title : GC Extractables
QLast Update : Tue Oct 22 06:07:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

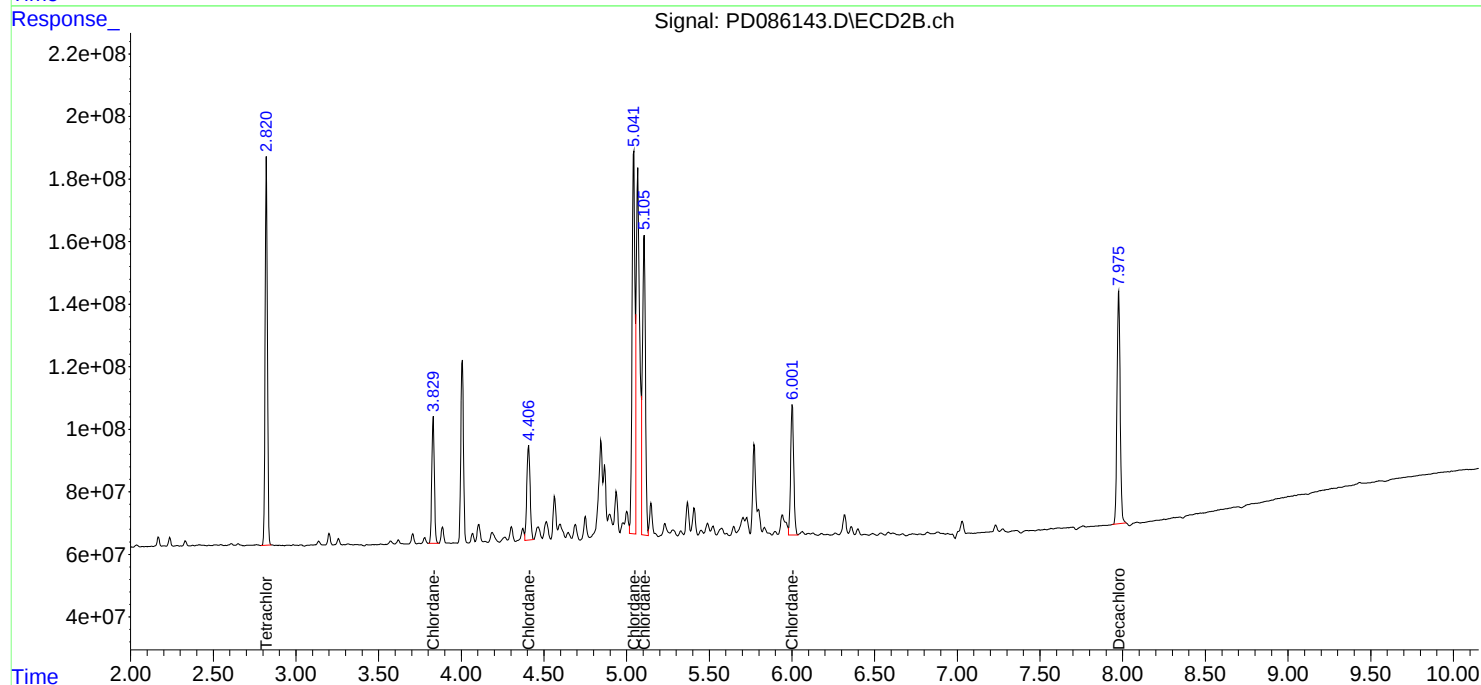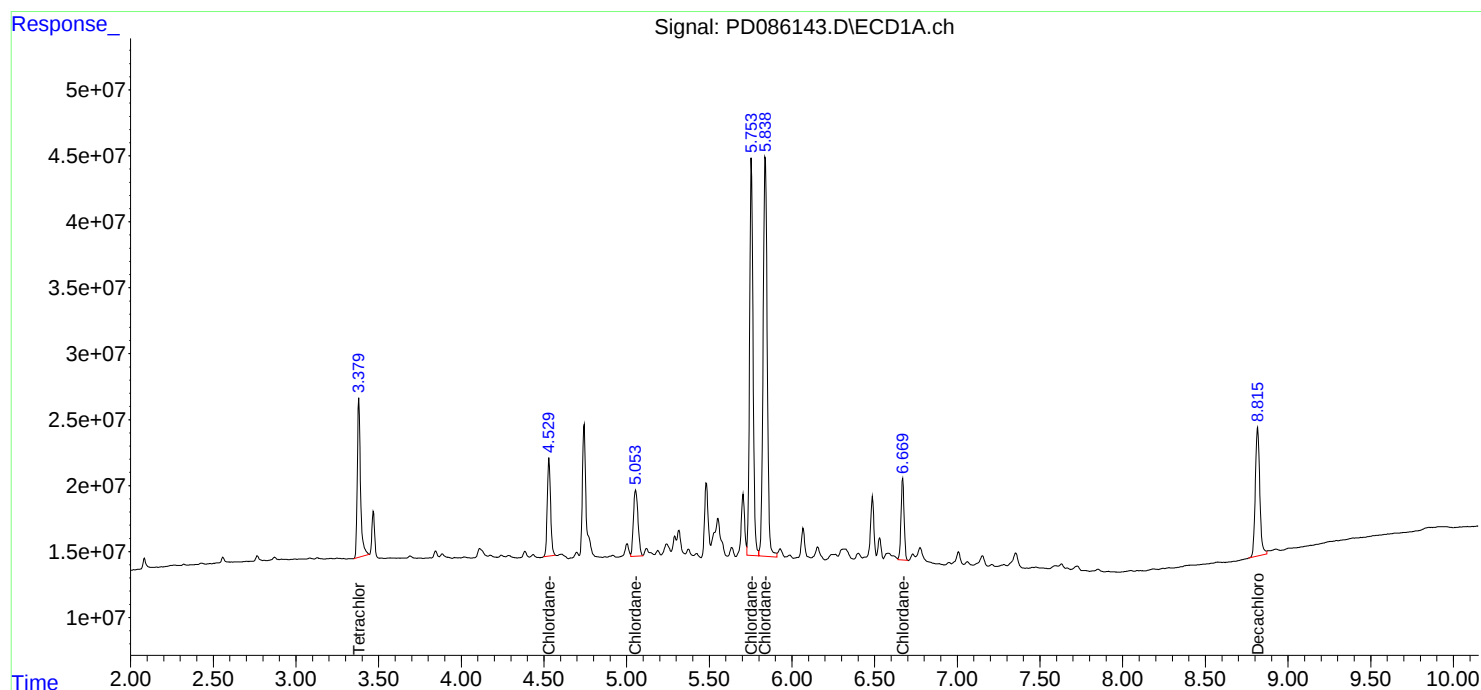


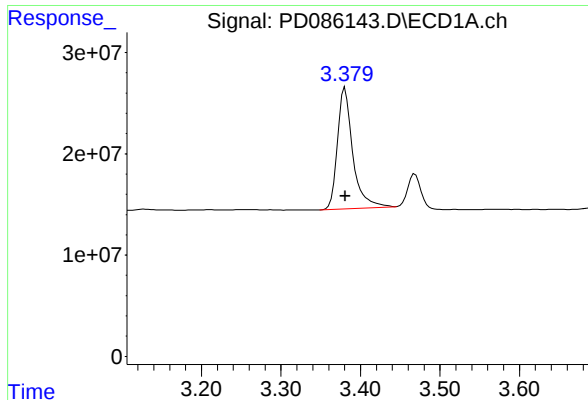

#1 Tetrachloro-m-xylene


R.T.: 3.381 min
Delta R.T.: 0.000 min
Response: 160738248
Conc: 100.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

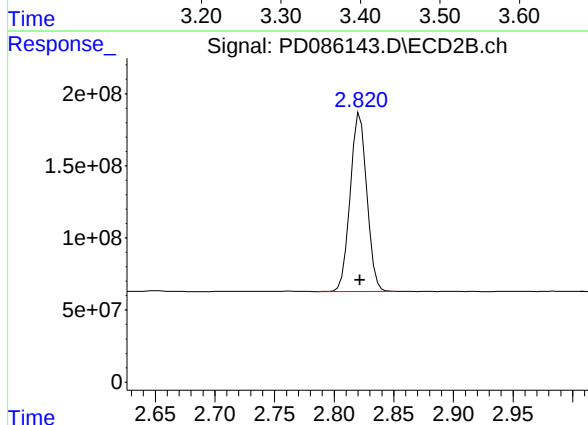


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: 0.000 min
Response: 1201019103
Conc: 98.36 ng/ml

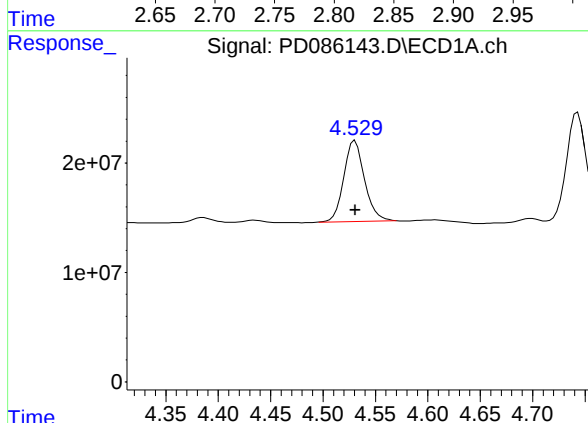


#23 Chlordane-1

R.T.: 4.530 min
Delta R.T.: 0.000 min
Response: 102383887
Conc: 999.79 ng/ml

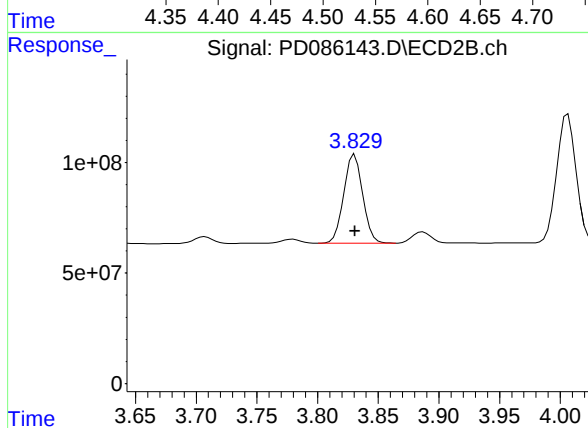

#23 Chlordane-1


R.T.: 3.831 min
Delta R.T.: 0.000 min
Response: 436466470
Conc: 989.95 ng/ml

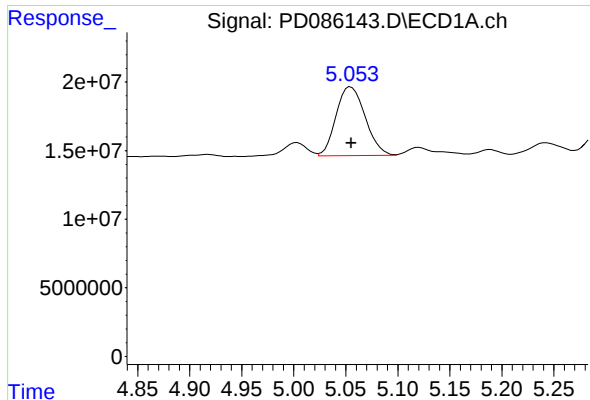

#24 Chlordane-2


R.T.: 5.055 min
Delta R.T.: 0.000 min
Response: 97781073
Conc: 1019.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

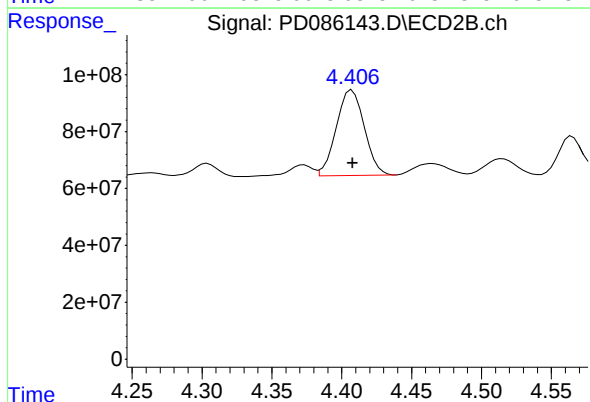


#24 Chlordane-2

R.T.: 4.407 min
Delta R.T.: 0.000 min
Response: 420047932
Conc: 966.90 ng/ml

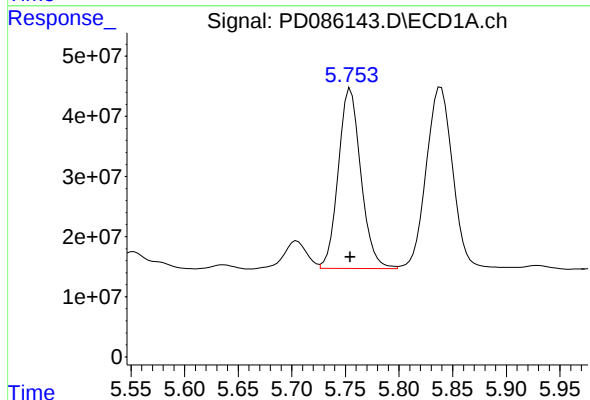


#25 Chlordane-3

R.T.: 5.755 min
Delta R.T.: 0.000 min
Response: 438573716
Conc: 1017.51 ng/ml

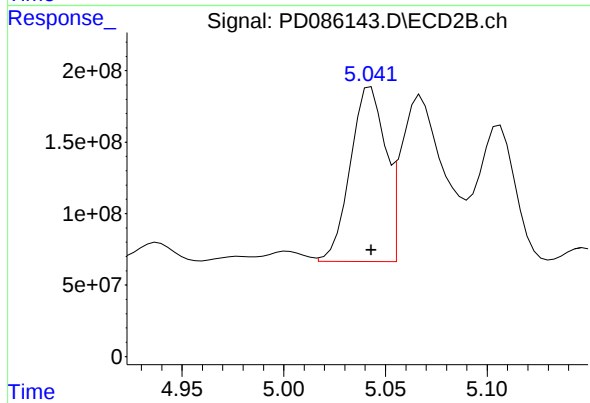

#25 Chlordane-3


R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 1457128635
Conc: 972.11 ng/ml

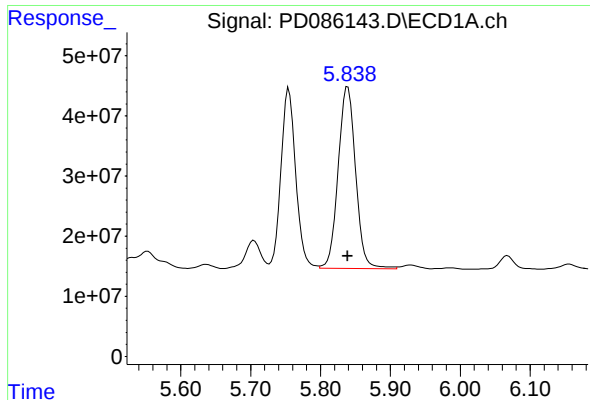

#26 Chlordane-4


R.T.: 5.839 min
Delta R.T.: 0.000 min
Response: 524744926
Conc: 1008.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

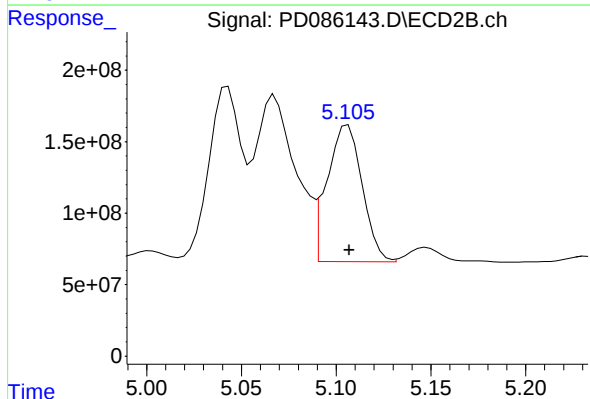


#26 Chlordane-4

R.T.: 5.106 min
Delta R.T.: 0.000 min
Response: 1228773064
Conc: 972.39 ng/ml

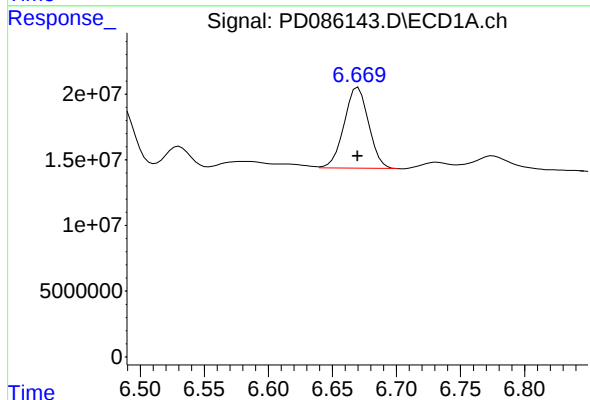


#27 Chlordane-5

R.T.: 6.670 min
Delta R.T.: 0.000 min
Response: 78693502
Conc: 1032.07 ng/ml

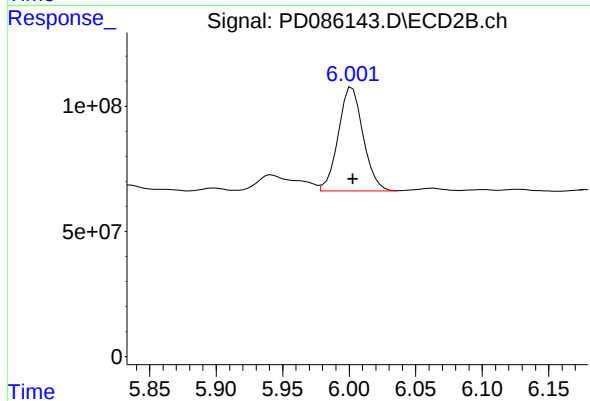

#27 Chlordane-5


R.T.: 6.002 min
Delta R.T.: 0.000 min
Response: 538047149
Conc: 979.71 ng/ml

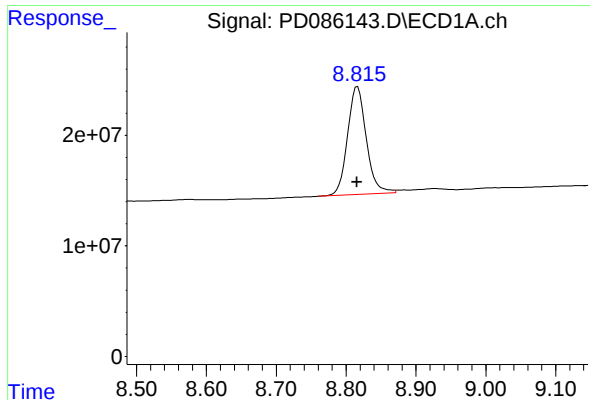

#28 Decachlorobiphenyl

R.T.: 8.816 min
Delta R.T.: 0.001 min
Response: 181400064
Conc: 95.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

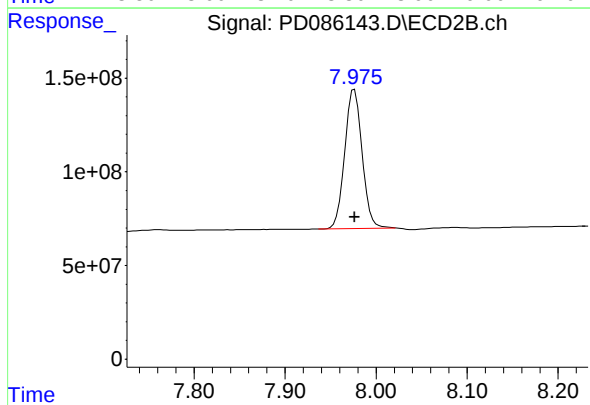

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: 0.000 min
Response: 989036705
Conc: 97.08 ng/ml