

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102124\
 Data File : PD086144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2024 20:31
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 06:12:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102124.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 22 06:07:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.381	2.822	119.5E6	897.1E6	74.552	73.468
28) SA Decachlor...	8.816	7.977	139.3E6	739.2E6	73.158	72.557
Target Compounds						
23) Chlordane-1	4.531	3.831	76821045	325.2E6	750.168	737.577
24) Chlordane-2	5.056	4.408	73240523	314.9E6	763.624	724.776
25) Chlordane-3	5.755	5.043	324.4E6	1087.7E6	752.667	725.669
26) Chlordane-4	5.839	5.107	389.1E6	917.4E6	747.654	725.973
27) Chlordane-5	6.670	6.003	57899373	401.5E6	759.353	731.070



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102124\
Data File : PD086144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2024 20:31
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 06:12:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102124.M
Quant Title : GC Extractables
QLast Update : Tue Oct 22 06:07:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

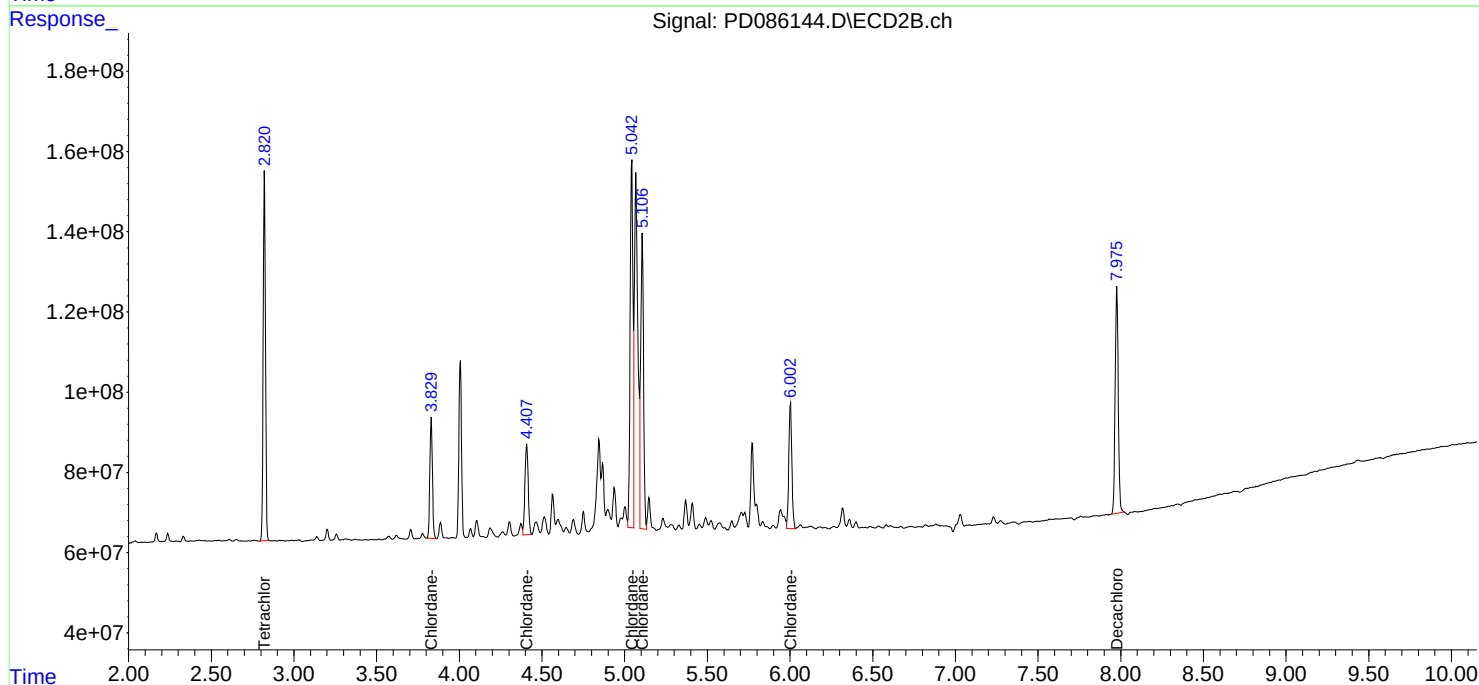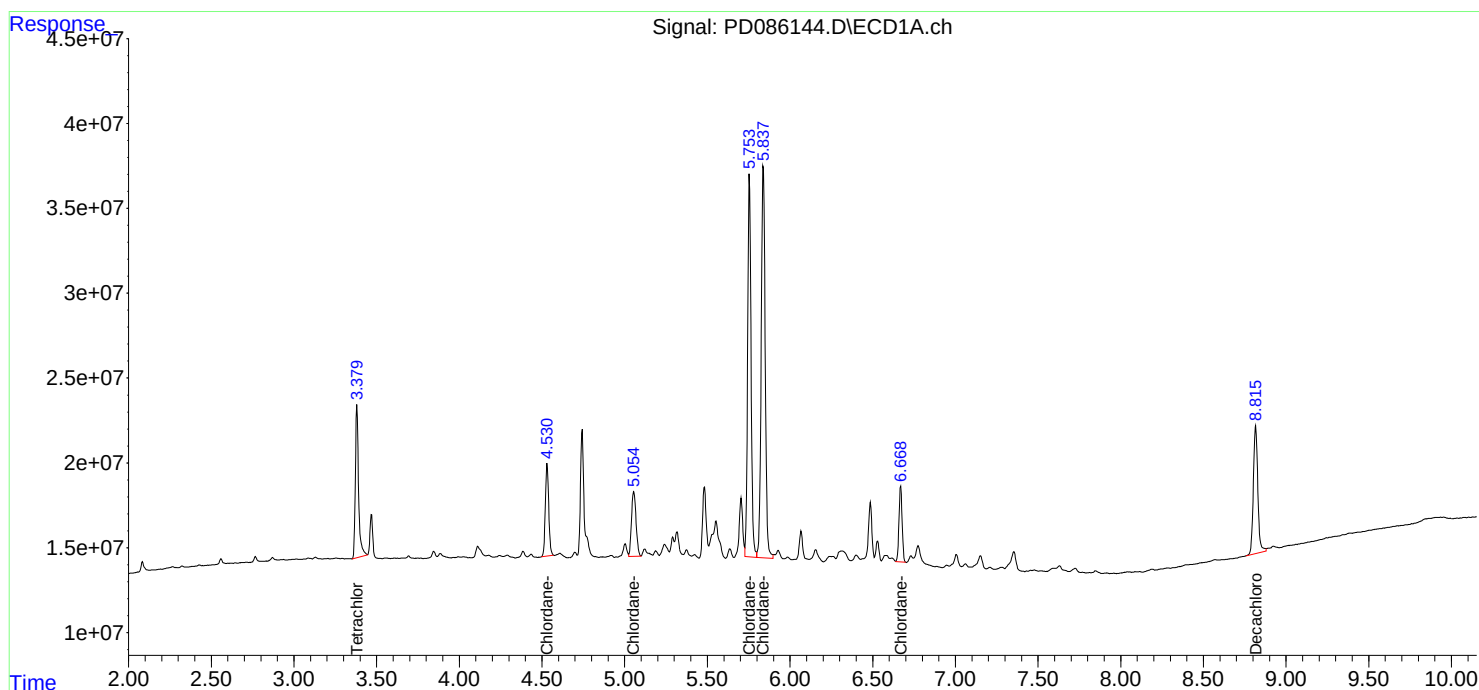


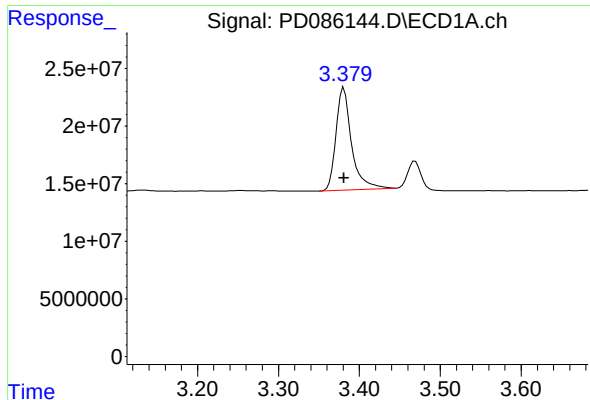

#1 Tetrachloro-m-xylene


R.T.: 3.381 min
Delta R.T.: 0.000 min
Response: 119502101
Conc: 74.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

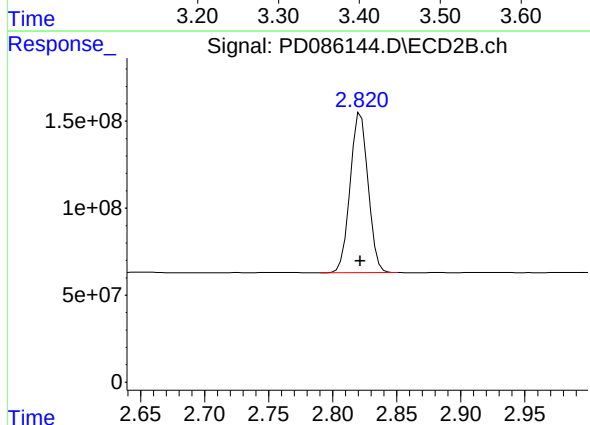


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: 0.000 min
Response: 897061361
Conc: 73.47 ng/ml

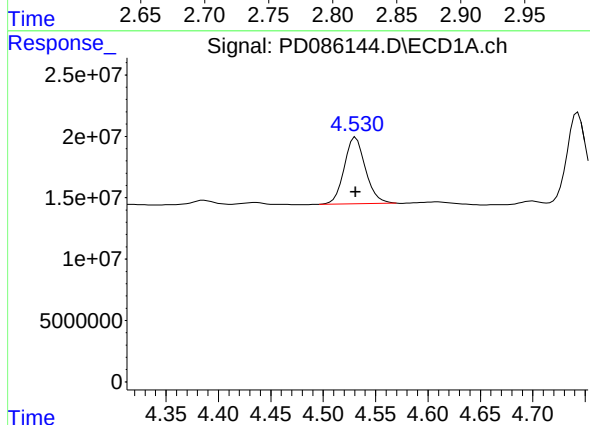


#23 Chlordane-1

R.T.: 4.531 min
Delta R.T.: 0.000 min
Response: 76821045
Conc: 750.17 ng/ml

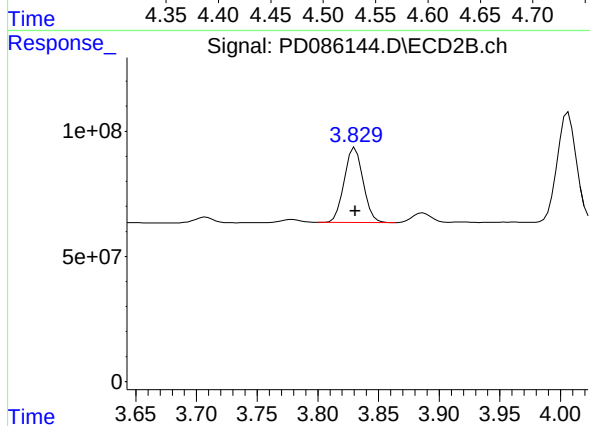

#23 Chlordane-1


R.T.: 3.831 min
Delta R.T.: 0.000 min
Response: 325195612
Conc: 737.58 ng/ml

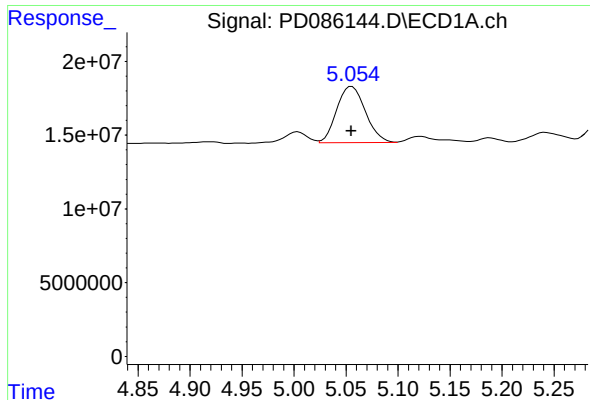

#24 Chlordane-2


R.T.: 5.056 min
Delta R.T.: 0.000 min
Response: 73240523
Conc: 763.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

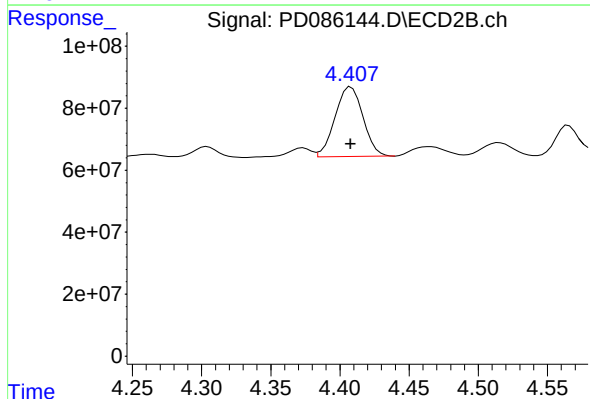


#24 Chlordane-2

R.T.: 4.408 min
Delta R.T.: 0.000 min
Response: 314861204
Conc: 724.78 ng/ml

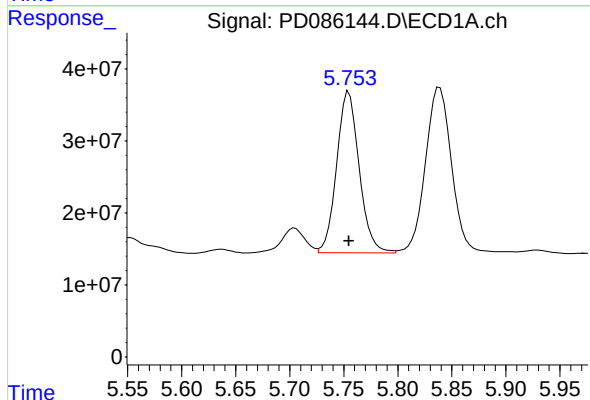


#25 Chlordane-3

R.T.: 5.755 min
Delta R.T.: 0.000 min
Response: 324418761
Conc: 752.67 ng/ml

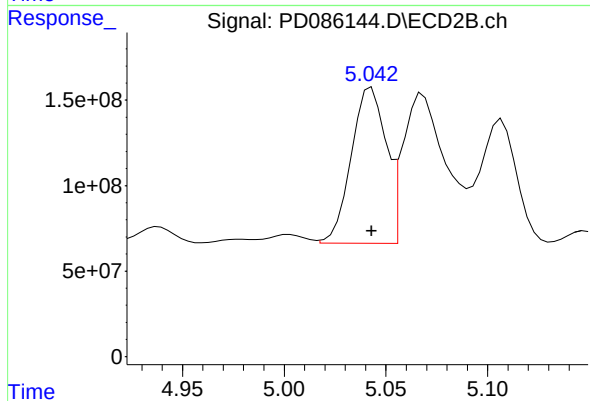

#25 Chlordane-3


R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 1087730664
Conc: 725.67 ng/ml

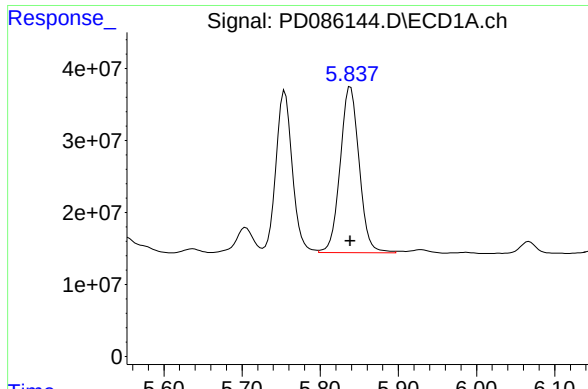

#26 Chlordane-4


R.T.: 5.839 min
Delta R.T.: 0.000 min
Response: 389080750
Conc: 747.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

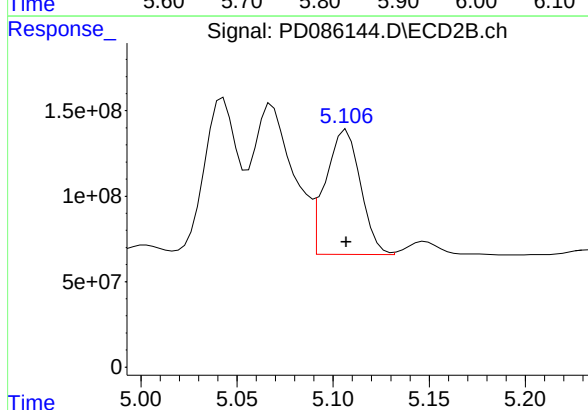


#26 Chlordane-4

R.T.: 5.107 min
Delta R.T.: 0.000 min
Response: 917384674
Conc: 725.97 ng/ml

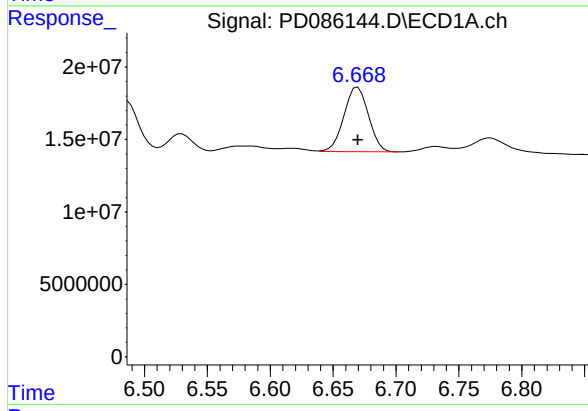


#27 Chlordane-5

R.T.: 6.670 min
Delta R.T.: 0.000 min
Response: 57899373
Conc: 759.35 ng/ml

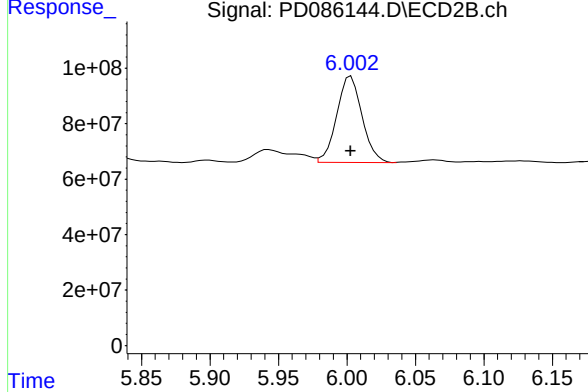

#27 Chlordane-5


R.T.: 6.003 min
Delta R.T.: 0.000 min
Response: 401495715
Conc: 731.07 ng/ml

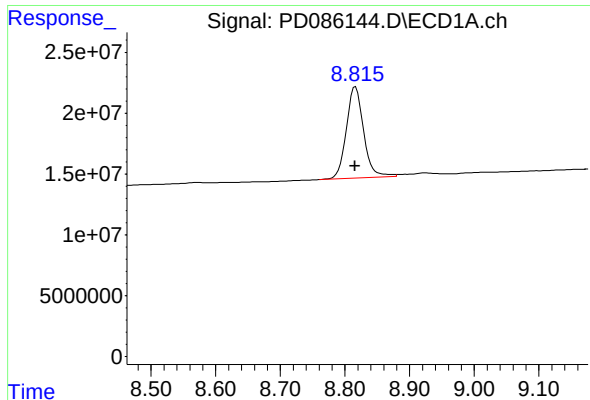

#28 Decachlorobiphenyl

R.T.: 8.816 min
Delta R.T.: 0.001 min
Response: 139279116
Conc: 73.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

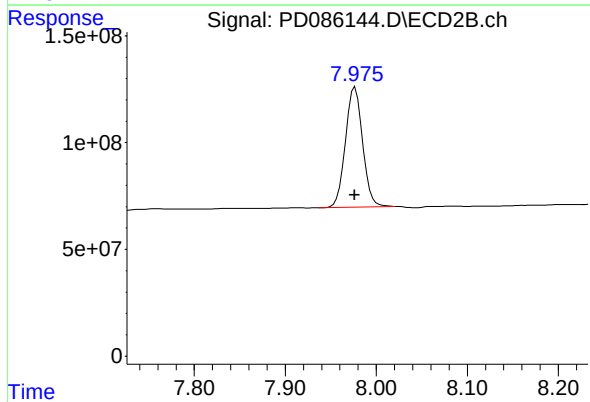

#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: 0.000 min
Response: 739199836
Conc: 72.56 ng/ml