

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102124\
 Data File : PD086145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2024 20:45
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 06:12:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102124.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 22 06:07:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.381	2.822	80146770	610.5E6	50.000	50.000
28) SA Decachlor...	8.815	7.976	95190149	509.4E6	50.000	50.000
Target Compounds						
23) Chlordane-1	4.531	3.831	51202568	220.4E6	500.000	500.000
24) Chlordane-2	5.055	4.408	47955866	217.2E6	500.000	500.000
25) Chlordane-3	5.755	5.043	215.5E6	749.5E6	500.000	500.000
26) Chlordane-4	5.839	5.107	260.2E6	631.8E6	500.000	500.000
27) Chlordane-5	6.670	6.003	38124142	274.6E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102124\
Data File : PD086145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2024 20:45
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 06:12:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102124.M
Quant Title : GC Extractables
QLast Update : Tue Oct 22 06:07:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

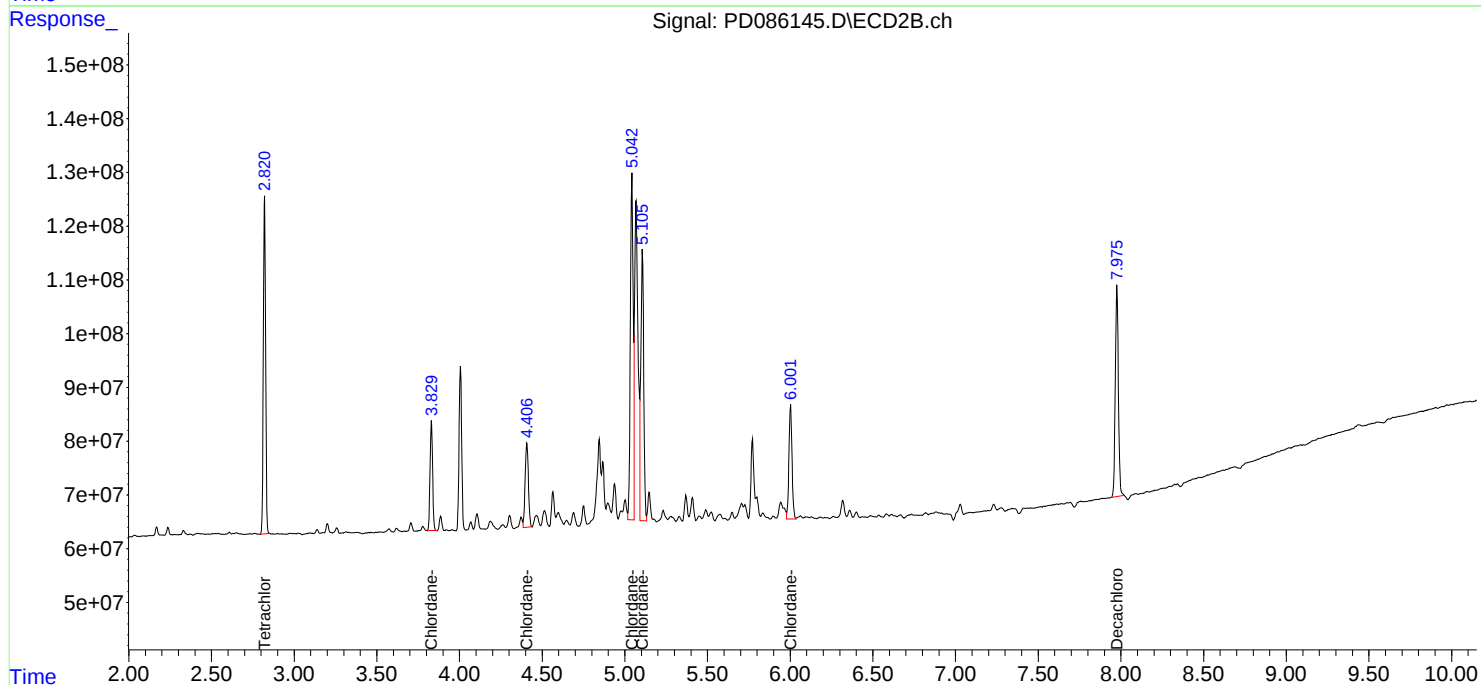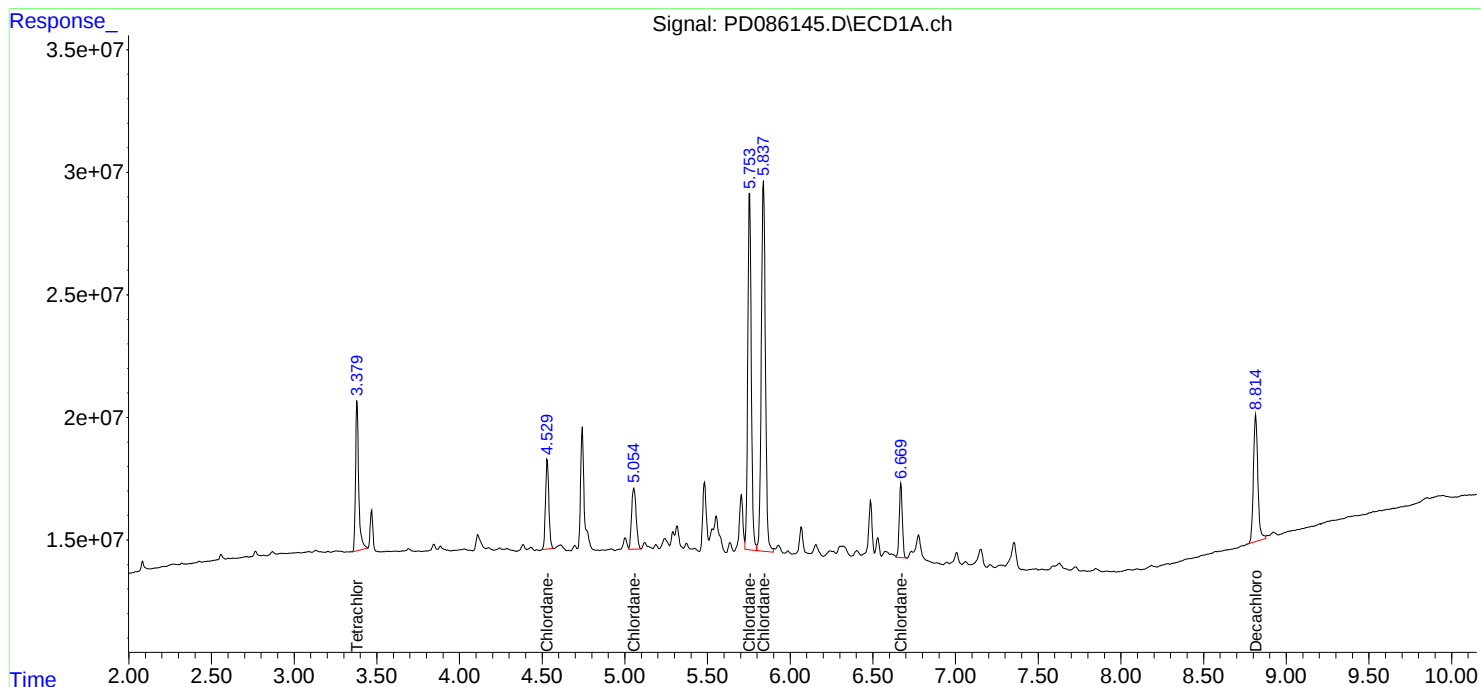


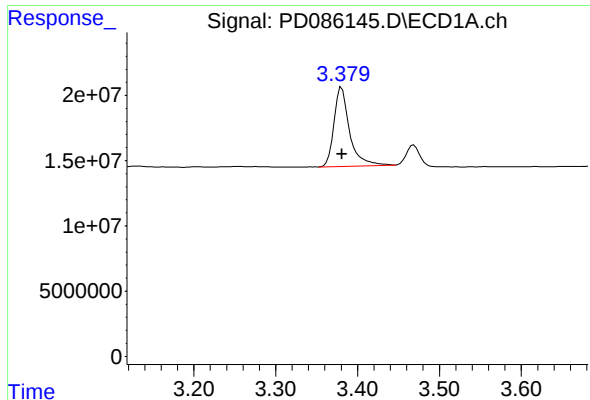

#1 Tetrachloro-m-xylene


R.T.: 3.381 min
Delta R.T.: 0.000 min
Response: 80146770
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

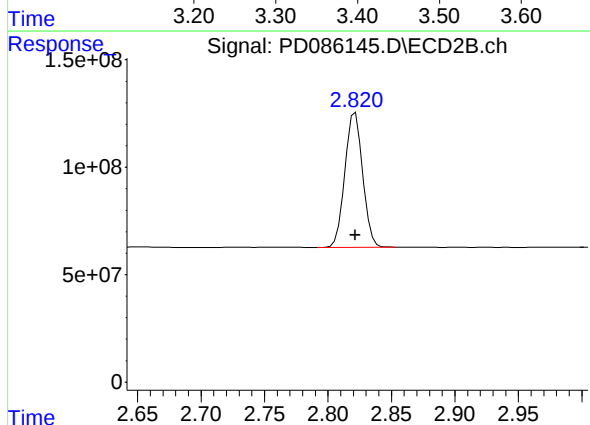


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: 0.000 min
Response: 610515678
Conc: 50.00 ng/ml

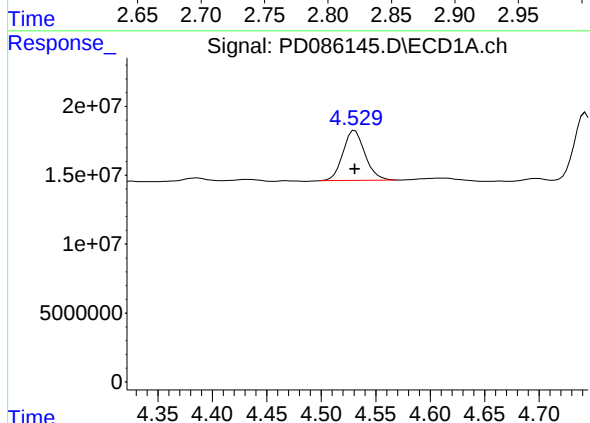


#23 Chlordane-1

R.T.: 4.531 min
Delta R.T.: 0.000 min
Response: 51202568
Conc: 500.00 ng/ml

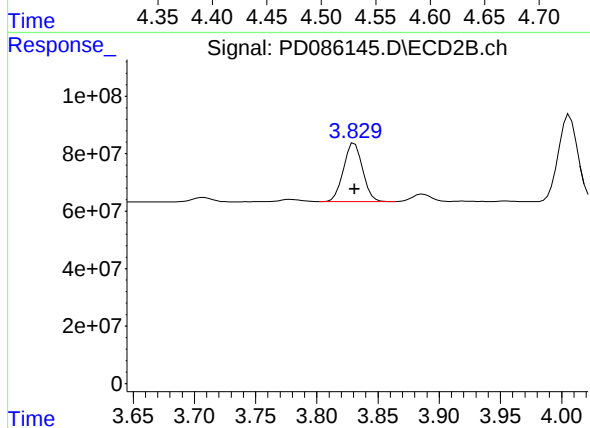

#23 Chlordane-1


R.T.: 3.831 min
Delta R.T.: 0.000 min
Response: 220448705
Conc: 500.00 ng/ml

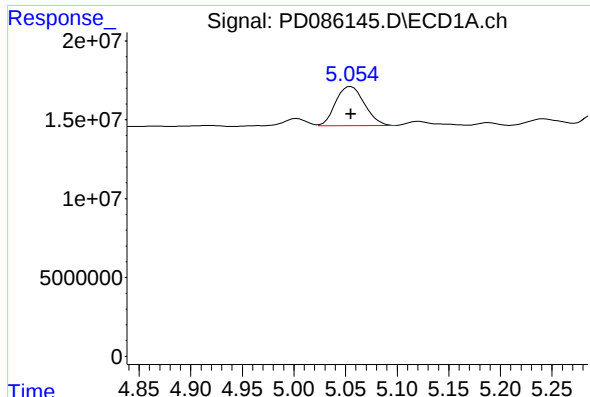

#24 Chlordane-2


R.T.: 5.055 min
Delta R.T.: 0.000 min
Response: 47955866
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

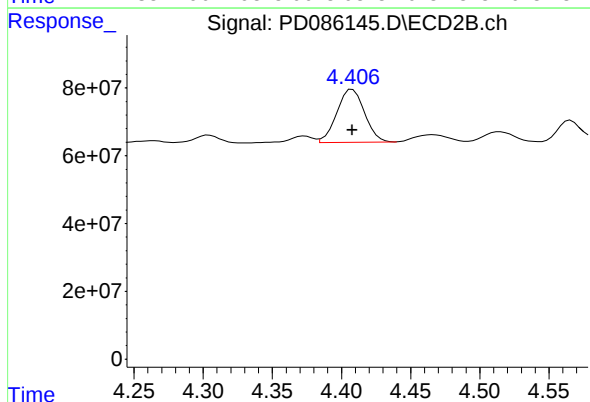


#24 Chlordane-2

R.T.: 4.408 min
Delta R.T.: 0.000 min
Response: 217212635
Conc: 500.00 ng/ml

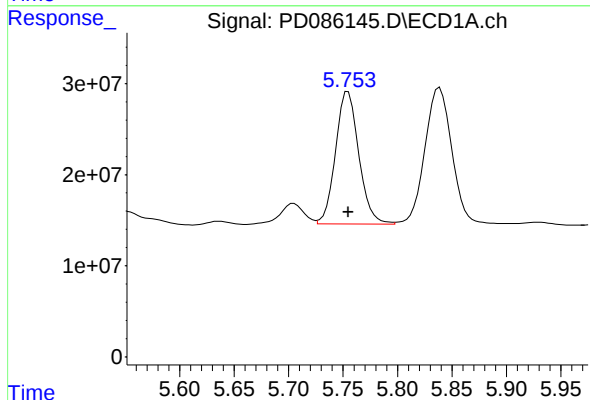


#25 Chlordane-3

R.T.: 5.755 min
Delta R.T.: 0.000 min
Response: 215512822
Conc: 500.00 ng/ml

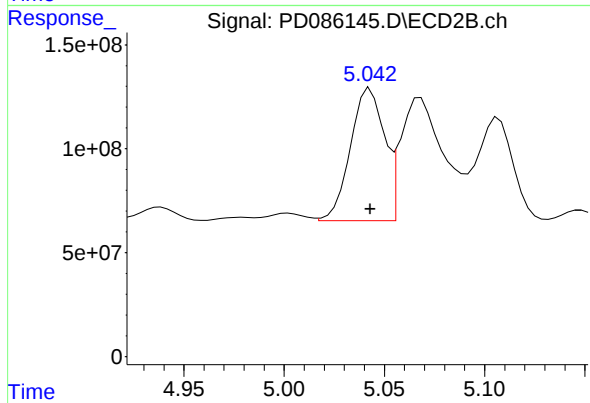

#25 Chlordane-3


R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 749467030
Conc: 500.00 ng/ml

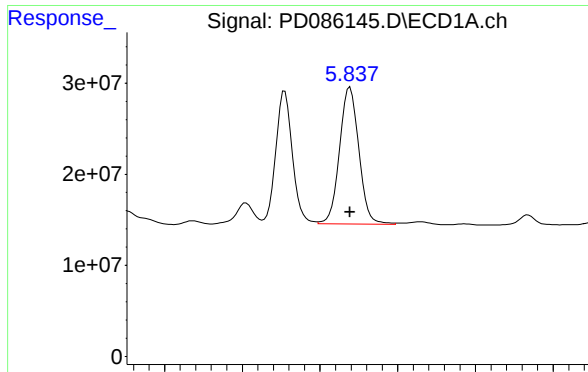

#26 Chlordane-4


R.T.: 5.839 min
Delta R.T.: 0.000 min
Response: 260200981
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

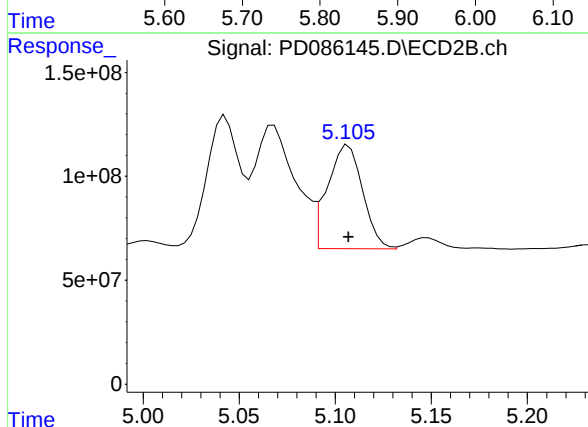


#26 Chlordane-4

R.T.: 5.107 min
Delta R.T.: 0.000 min
Response: 631831185
Conc: 500.00 ng/ml

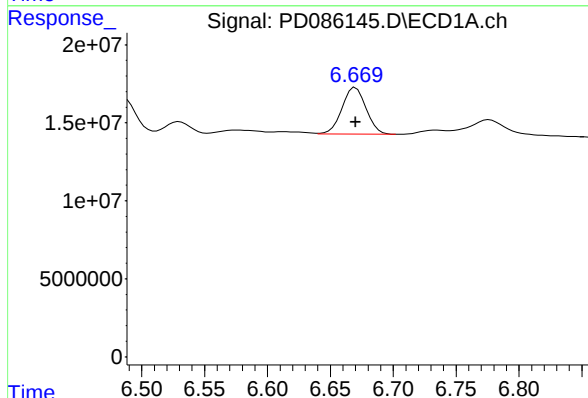


#27 Chlordane-5

R.T.: 6.670 min
Delta R.T.: 0.000 min
Response: 38124142
Conc: 500.00 ng/ml

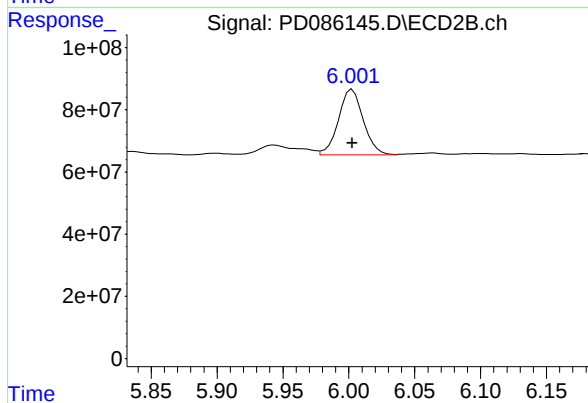

#27 Chlordane-5


R.T.: 6.003 min
Delta R.T.: 0.000 min
Response: 274594631
Conc: 500.00 ng/ml

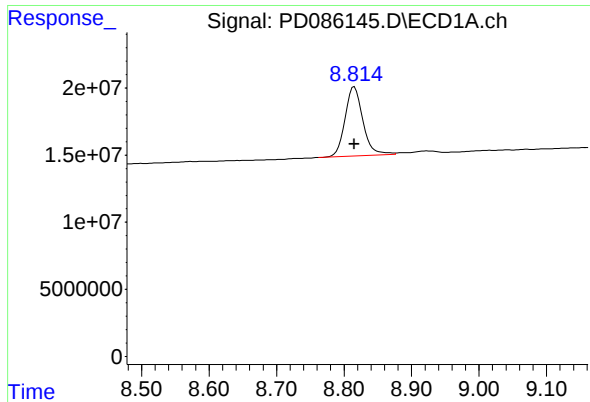

#28 Decachlorobiphenyl

R.T.: 8.815 min
Delta R.T.: 0.000 min
Response: 95190149
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

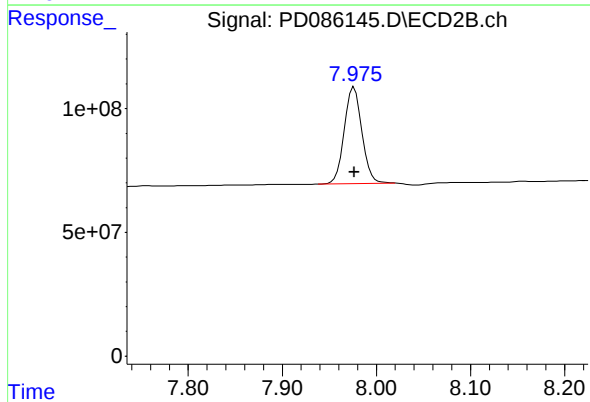

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: 0.000 min
Response: 509392681
Conc: 50.00 ng/ml