

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102124\
 Data File : PD086146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2024 20:58
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 06:13:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102124.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 22 06:07:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.381	2.822	39341795	304.4E6	24.544	24.927
28) SA Decachlor...	8.816	7.977	50027003	256.6E6	26.277	25.188
Target Compounds						
23) Chlordane-1	4.530	3.831	25179321	111.7E6	245.879	253.306
24) Chlordane-2	5.055	4.408	24626309	109.3E6	256.760	251.489
25) Chlordane-3	5.754	5.042	105.6E6	378.8E6	245.021	252.736
26) Chlordane-4	5.838	5.106	129.9E6	319.1E6	249.562	252.523
27) Chlordane-5	6.670	6.002	18023411	139.3E6	236.378	253.645



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102124\
Data File : PD086146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2024 20:58
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 06:13:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102124.M
Quant Title : GC Extractables
QLast Update : Tue Oct 22 06:07:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

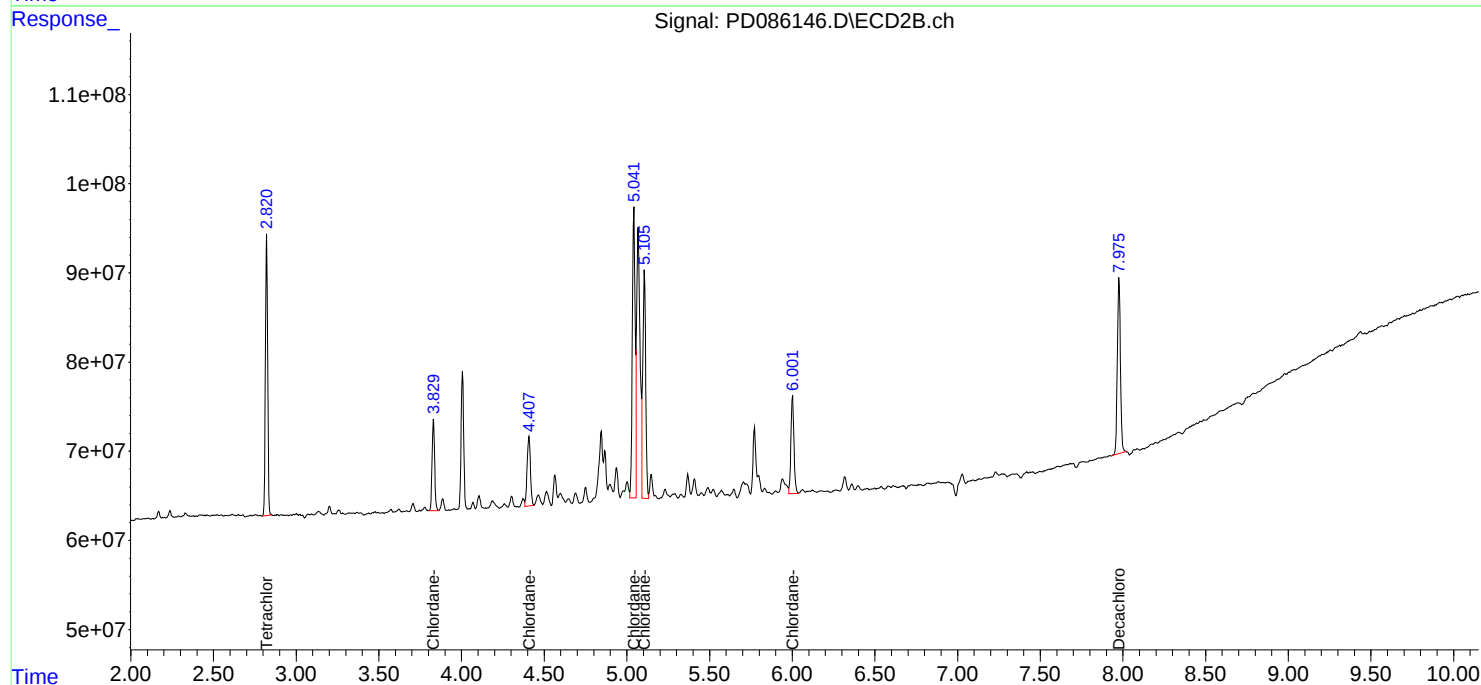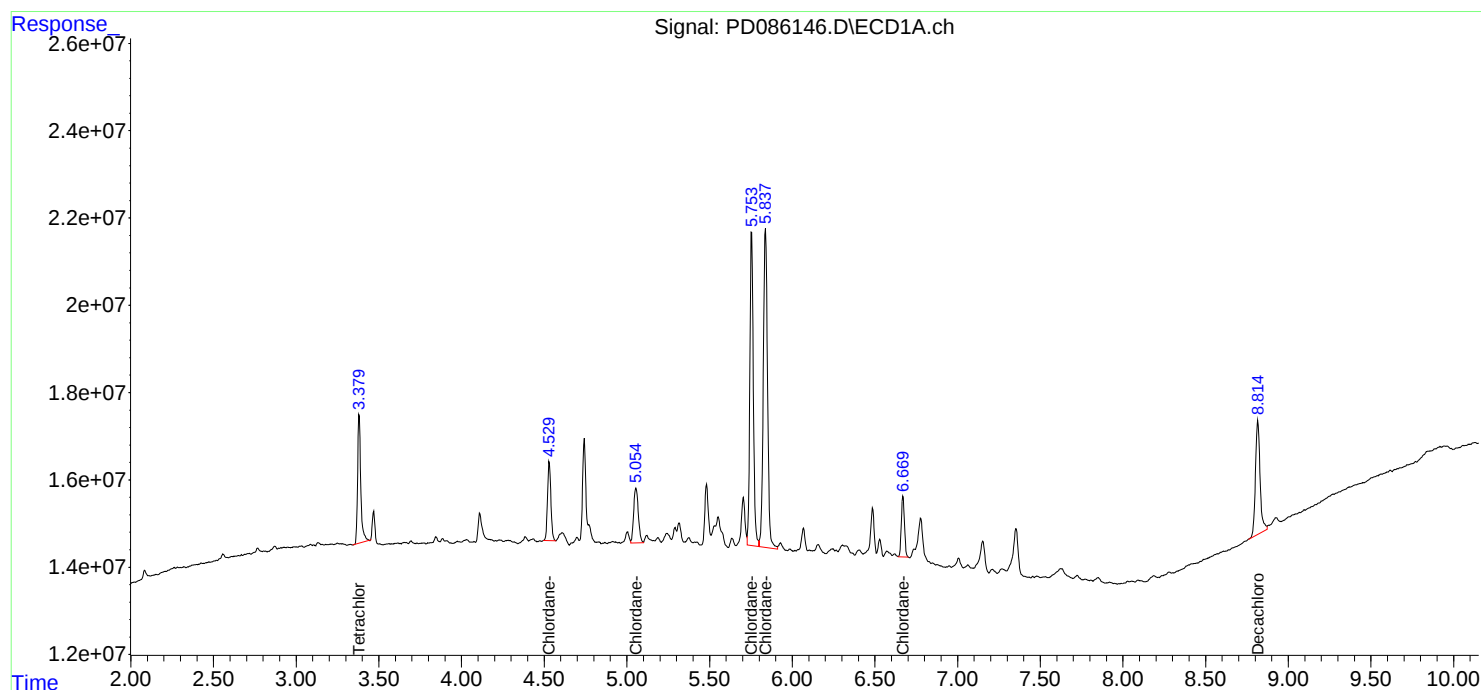


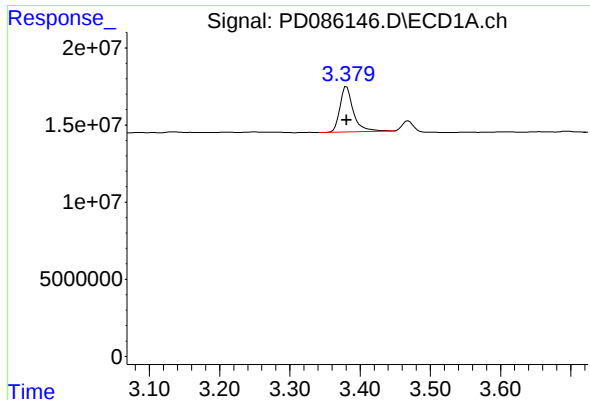

#1 Tetrachloro-m-xylene


R.T.: 3.381 min
Delta R.T.: 0.000 min
Response: 39341795
Conc: 24.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

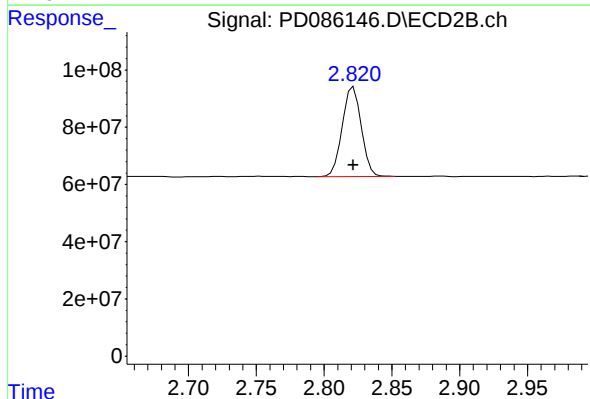


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: 0.000 min
Response: 304363240
Conc: 24.93 ng/ml

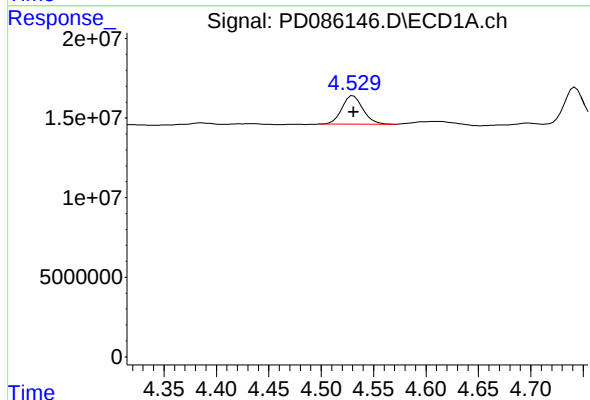


#23 Chlordane-1

R.T.: 4.530 min
Delta R.T.: 0.000 min
Response: 25179321
Conc: 245.88 ng/ml

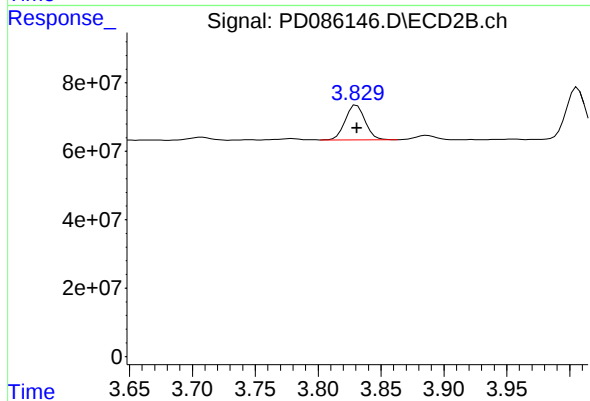

#23 Chlordane-1


R.T.: 3.831 min
Delta R.T.: 0.000 min
Response: 111682049
Conc: 253.31 ng/ml

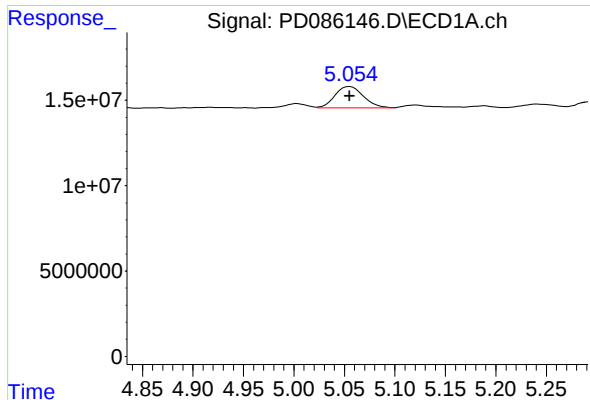

#24 Chlordane-2


R.T.: 5.055 min
Delta R.T.: 0.000 min
Response: 24626309
Conc: 256.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

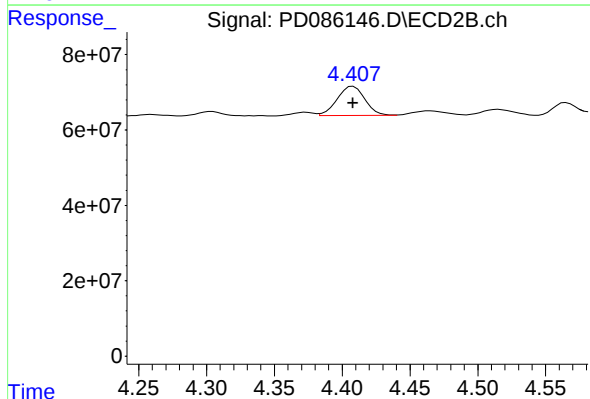


#24 Chlordane-2

R.T.: 4.408 min
Delta R.T.: 0.000 min
Response: 109253064
Conc: 251.49 ng/ml

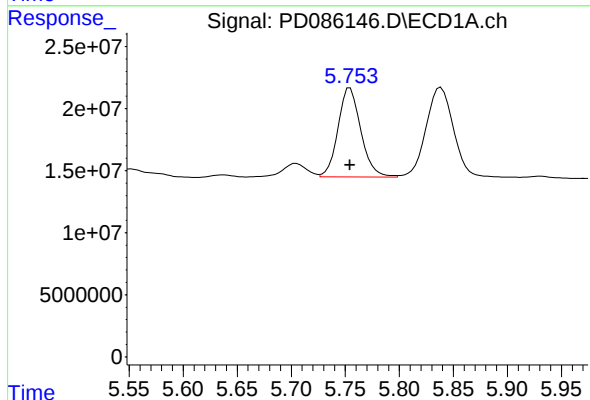


#25 Chlordane-3

R.T.: 5.754 min
Delta R.T.: 0.000 min
Response: 105610490
Conc: 245.02 ng/ml

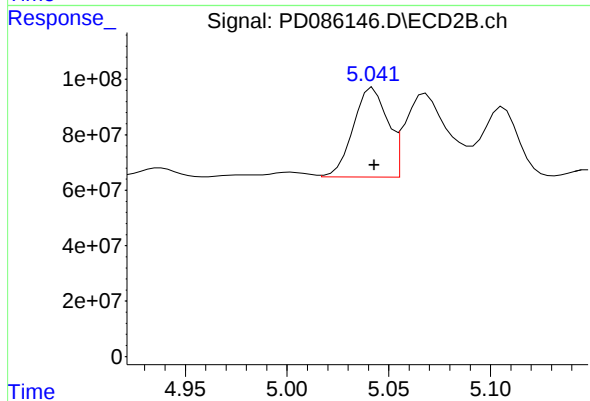

#25 Chlordane-3


R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 378834740
Conc: 252.74 ng/ml

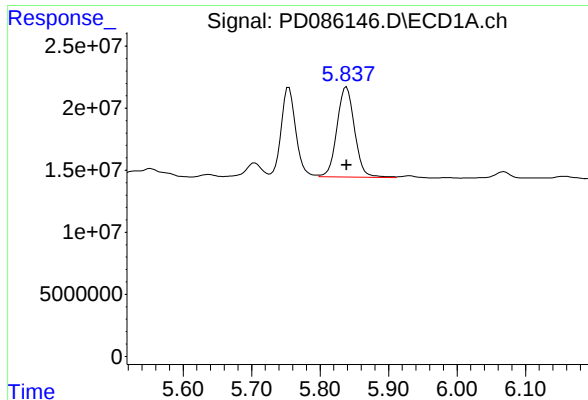

#26 Chlordane-4


R.T.: 5.838 min
Delta R.T.: 0.000 min
Response: 129872425
Conc: 249.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

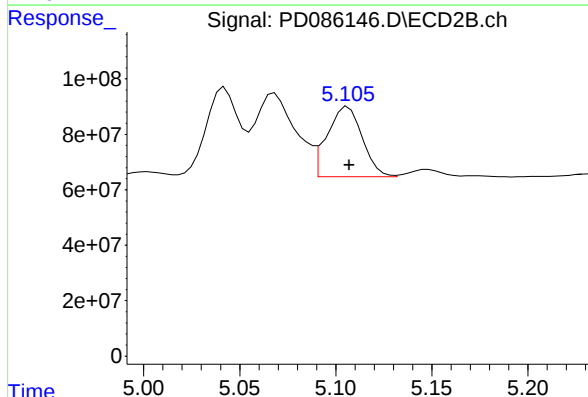


#26 Chlordane-4

R.T.: 5.106 min
Delta R.T.: 0.000 min
Response: 319104174
Conc: 252.52 ng/ml

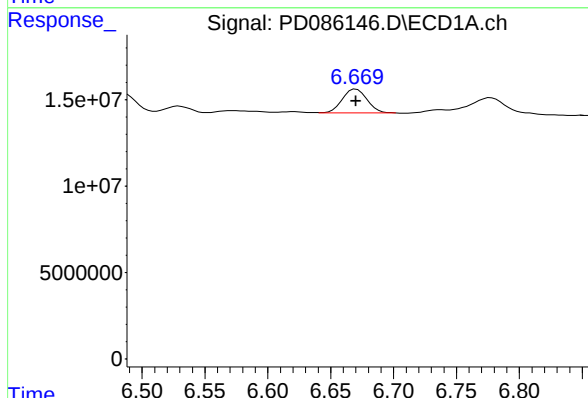


#27 Chlordane-5

R.T.: 6.670 min
Delta R.T.: 0.000 min
Response: 18023411
Conc: 236.38 ng/ml

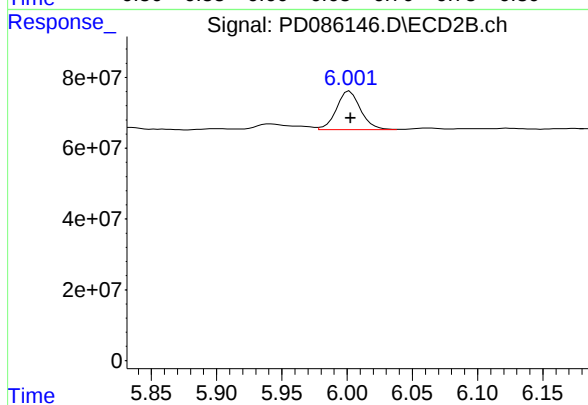

#27 Chlordane-5


R.T.: 6.002 min
Delta R.T.: 0.000 min
Response: 139298847
Conc: 253.64 ng/ml

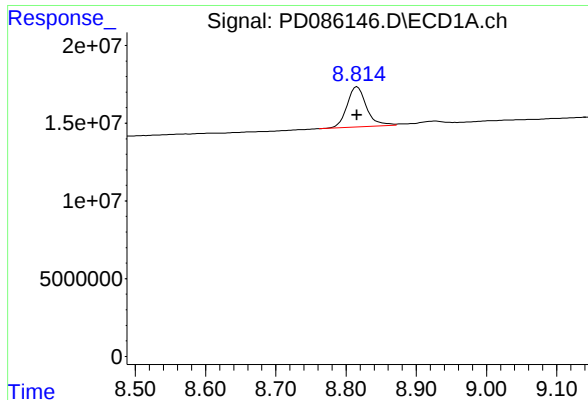

#28 Decachlorobiphenyl

R.T.: 8.816 min
Delta R.T.: 0.000 min
Response: 50027003
Conc: 26.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

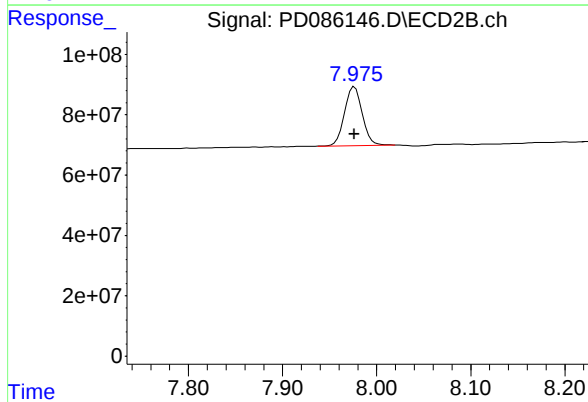

#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: 0.000 min
Response: 256614435
Conc: 25.19 ng/ml