

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102124\
 Data File : PD086154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2024 23:12
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD102124

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 06:48:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102124.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 22 06:44:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.381	2.822	80827313	616.6E6	51.193	49.929
28) SA Decachlor...	8.816	7.977	97004907	511.1E6	48.507	49.382
Target Compounds						
23) Chlordane-1	4.531	3.831	50844889	222.4E6	473.155	493.476
24) Chlordane-2	5.055	4.408	47962859	214.8E6	485.095	479.911
25) Chlordane-3	5.755	5.043	214.8E6	753.1E6	495.531	494.154
26) Chlordane-4	5.839	5.107	260.7E6	628.8E6	485.684	486.875
27) Chlordane-5	6.670	6.003	38308372	276.1E6	512.761	490.900



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102124\
Data File : PD086154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2024 23:12
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD102124

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 06:48:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102124.M
Quant Title : GC Extractables
QLast Update : Tue Oct 22 06:44:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

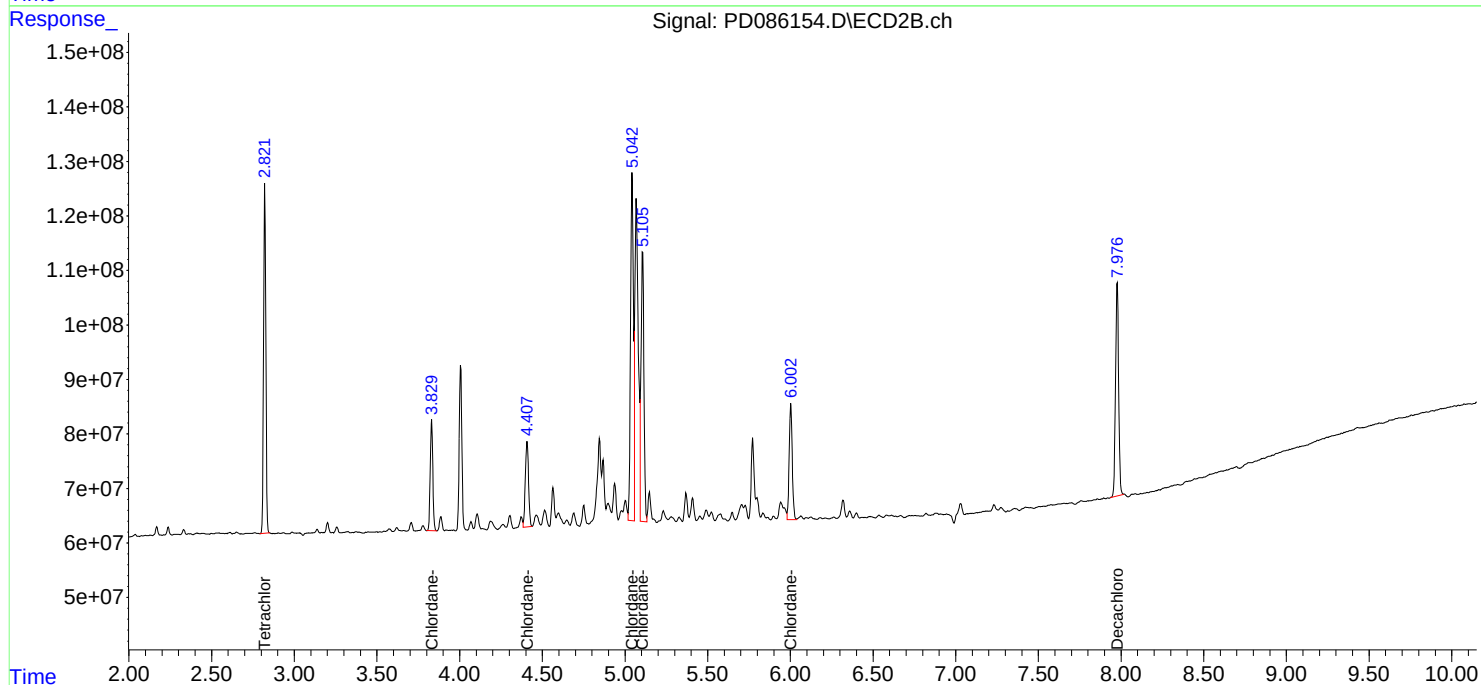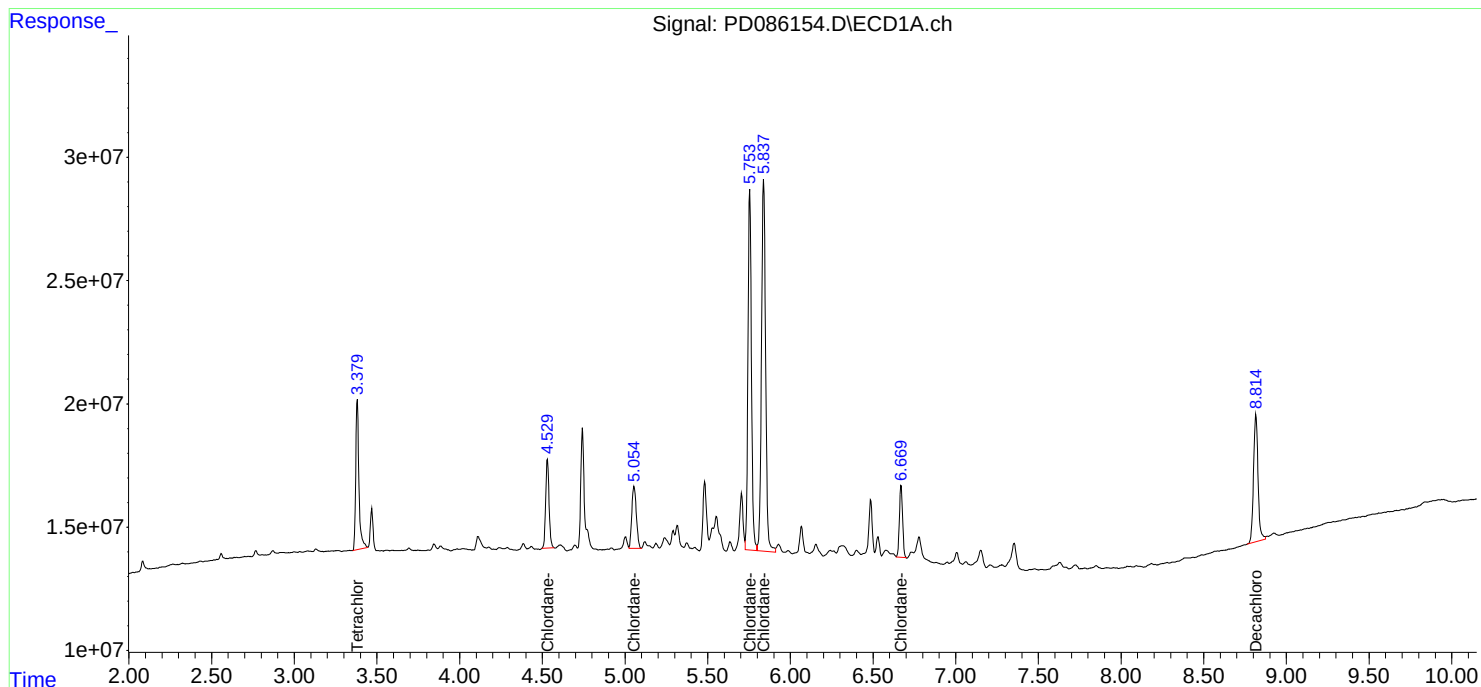


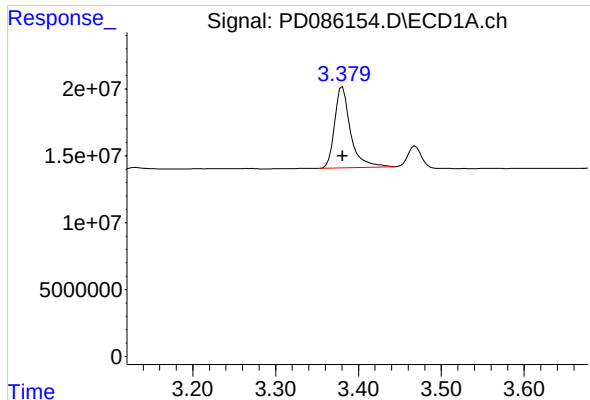

#1 Tetrachloro-m-xylene


R.T.: 3.381 min
Delta R.T.: 0.000 min
Response: 80827313
Conc: 51.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD102124

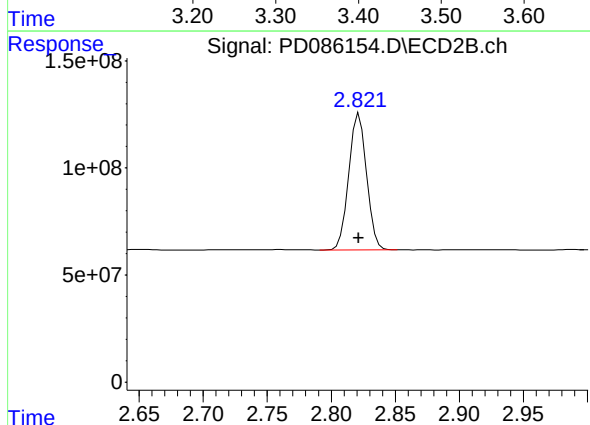


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: 0.000 min
Response: 616592152
Conc: 49.93 ng/ml

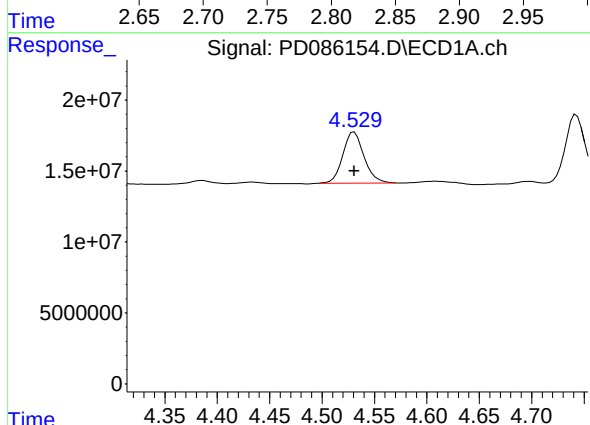


#23 Chlordane-1

R.T.: 4.531 min
Delta R.T.: 0.000 min
Response: 50844889
Conc: 473.16 ng/ml

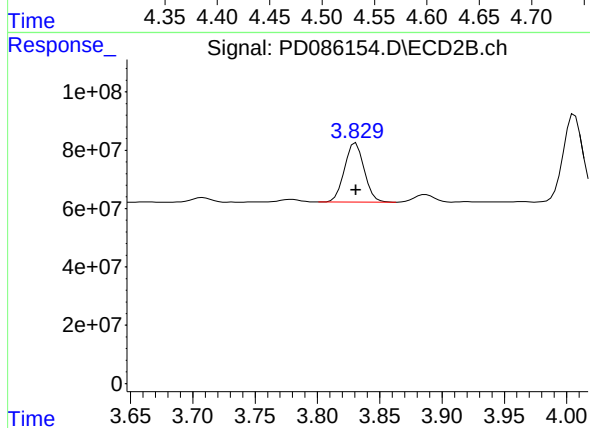

#23 Chlordane-1


R.T.: 3.831 min
Delta R.T.: 0.000 min
Response: 222415778
Conc: 493.48 ng/ml

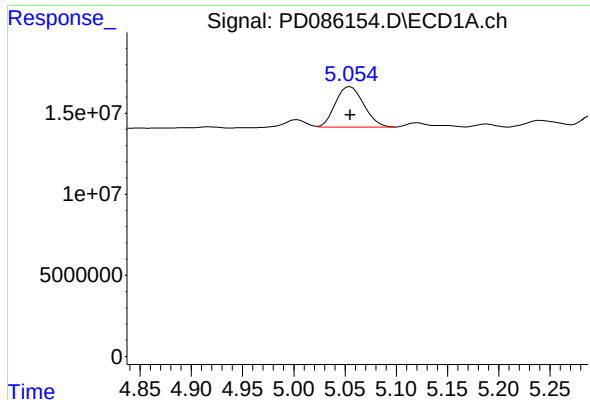

#24 Chlordane-2


R.T.: 5.055 min
Delta R.T.: 0.000 min
Response: 47962859
Conc: 485.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD102124

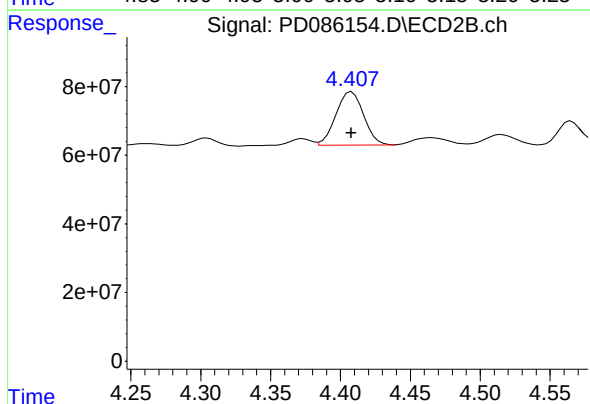


#24 Chlordane-2

R.T.: 4.408 min
Delta R.T.: 0.000 min
Response: 214799204
Conc: 479.91 ng/ml

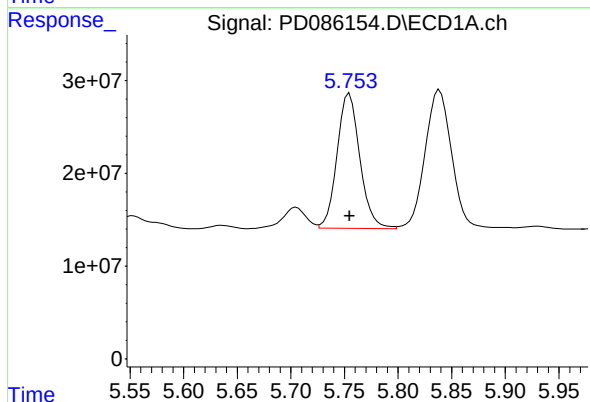


#25 Chlordane-3

R.T.: 5.755 min
Delta R.T.: 0.000 min
Response: 214781773
Conc: 495.53 ng/ml

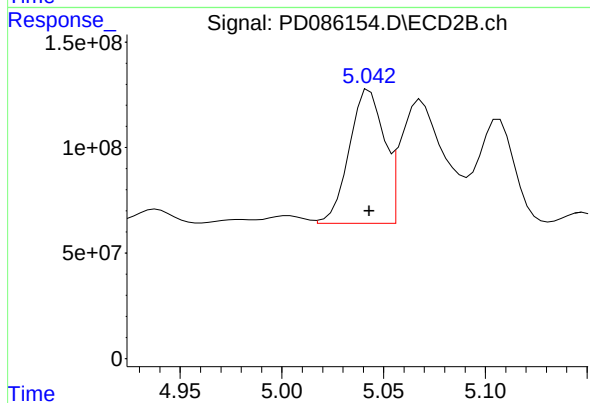

#25 Chlordane-3


R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 753055637
Conc: 494.15 ng/ml

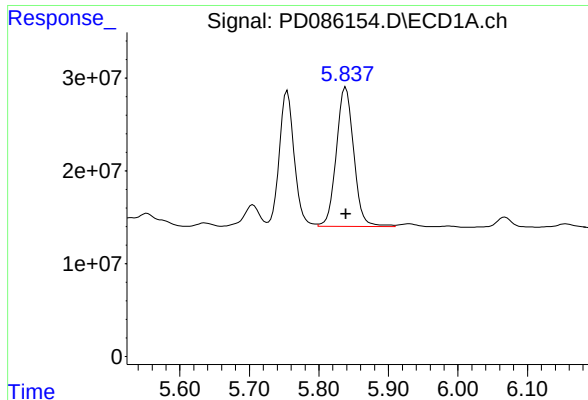

#26 Chlordane-4


R.T.: 5.839 min
Delta R.T.: 0.000 min
Response: 260663660
Conc: 485.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD102124

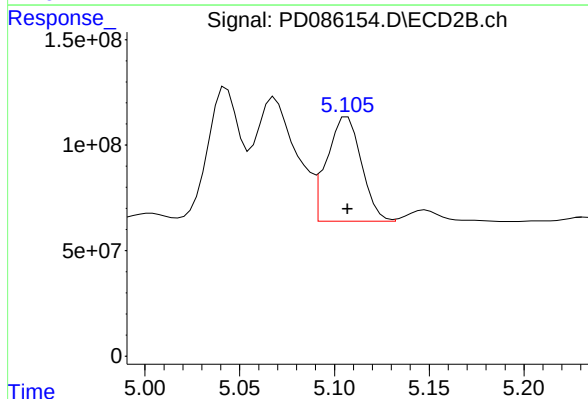


#26 Chlordane-4

R.T.: 5.107 min
Delta R.T.: 0.000 min
Response: 628812623
Conc: 486.87 ng/ml

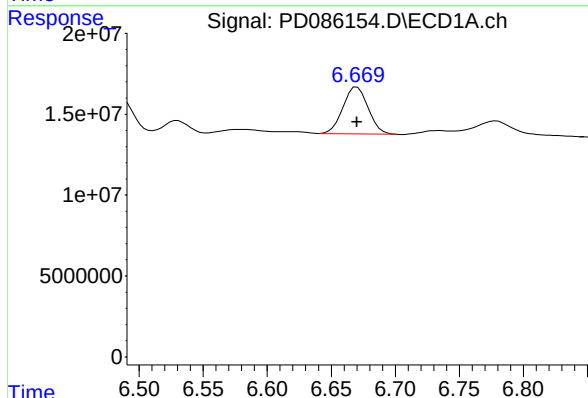


#27 Chlordane-5

R.T.: 6.670 min
Delta R.T.: 0.000 min
Response: 38308372
Conc: 512.76 ng/ml

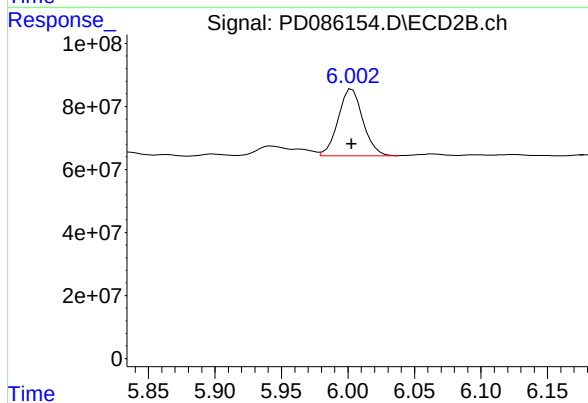

#27 Chlordane-5


R.T.: 6.003 min
Delta R.T.: 0.000 min
Response: 276147451
Conc: 490.90 ng/ml

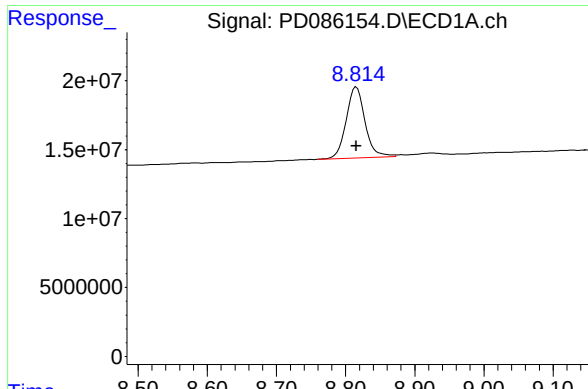

#28 Decachlorobiphenyl

R.T.: 8.816 min
Delta R.T.: 0.000 min
Response: 97004907
Conc: 48.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD102124

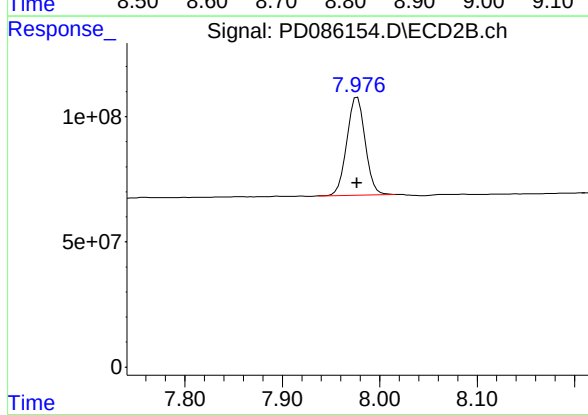

#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: 0.000 min
Response: 511107029
Conc: 49.38 ng/ml