

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102218\
 Data File : PD049950.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2018 10:11
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 04:20:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101918CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 19 05:13:06 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
27)	SA Decachlor...	0.000	9.138	0	3464921	N.D.	0.195
Target Compounds							
5)	MB Aldrin	5.525	0.000	171291	0	0.213	N.D. #
8)	B Heptachlo...	0.000	5.904f	0	4212893	N.D.	0.136
9)	A Endosulfan I	0.000	6.310	0	1847438	N.D.	<MDL
10)	B trans-Chl...	6.217	6.214	890057	-440832	1.061	N.D. #
11)	B cis-Chlor...	6.217f	6.282	890057	3824943	1.088	0.132 #
12)	B 4,4'-DDE	0.000	6.415	0	1571601	N.D.	<MDL
15)	B Endosulfa...	7.031f	0.000	860231	0	1.177	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102218\
Data File : PD049950.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2018 10:11
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 04:20:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101918CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 19 05:13:06 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

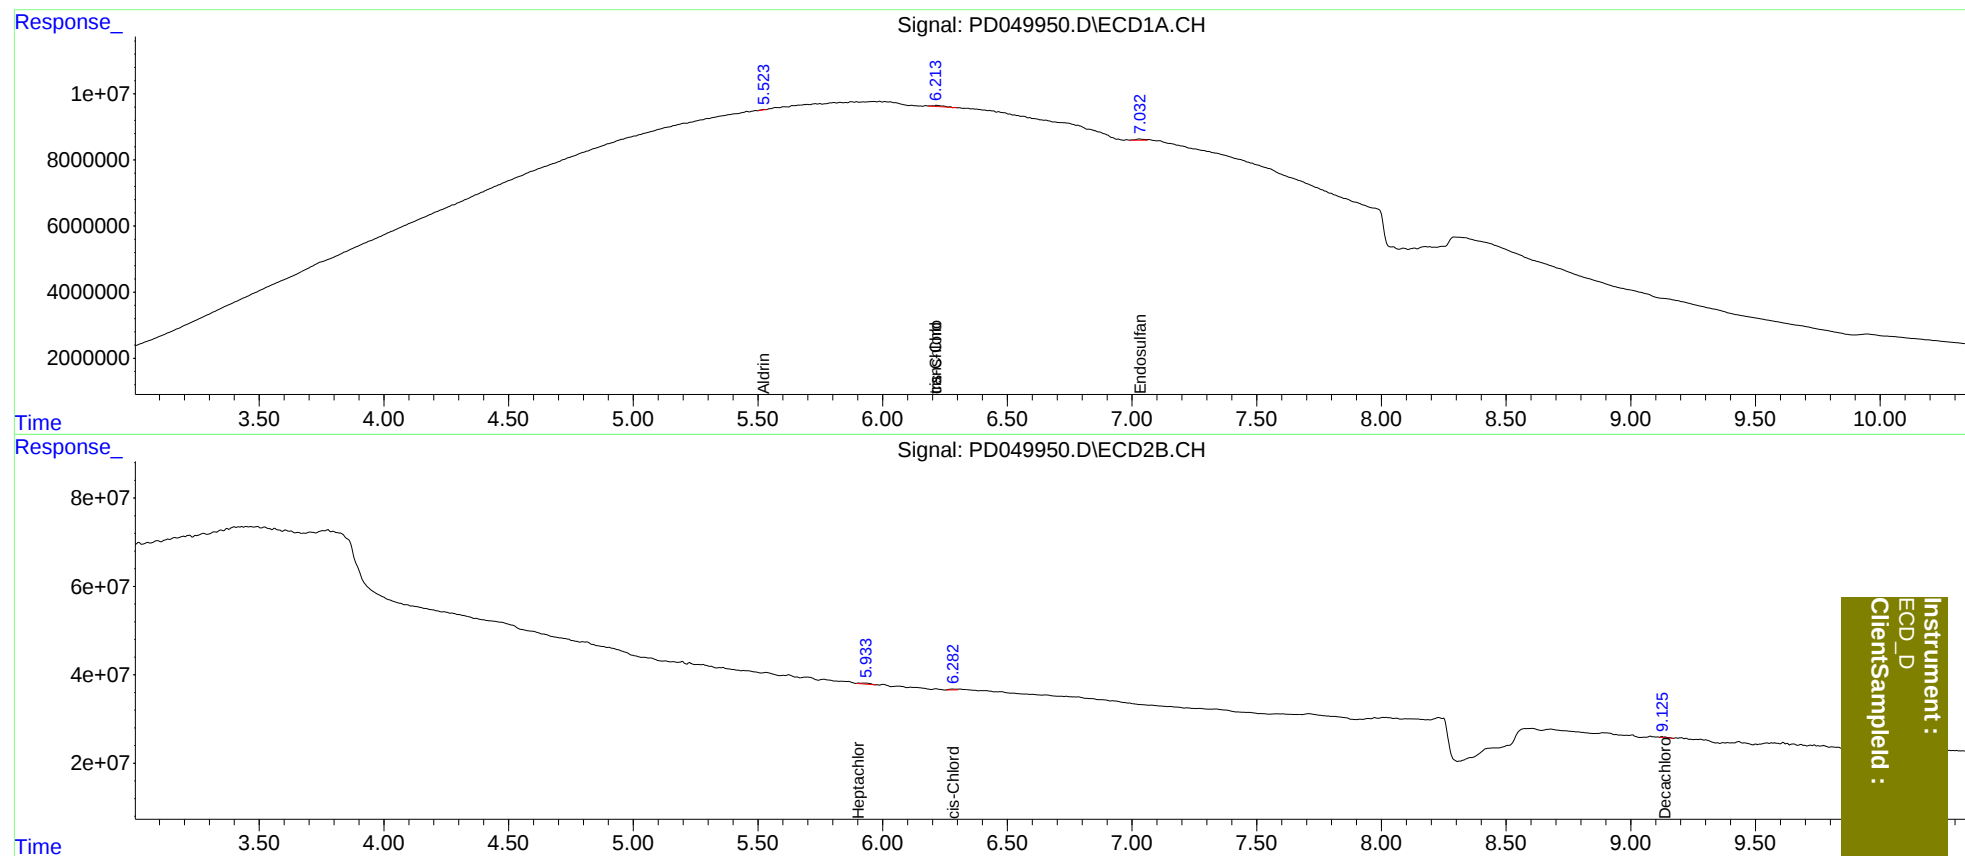


Instrument :
ECD_D
ClientSampled :

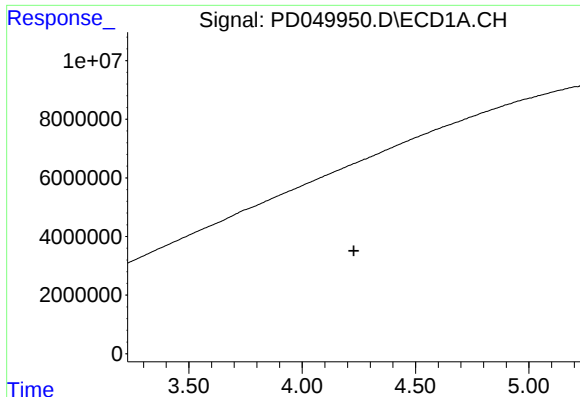

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 4.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

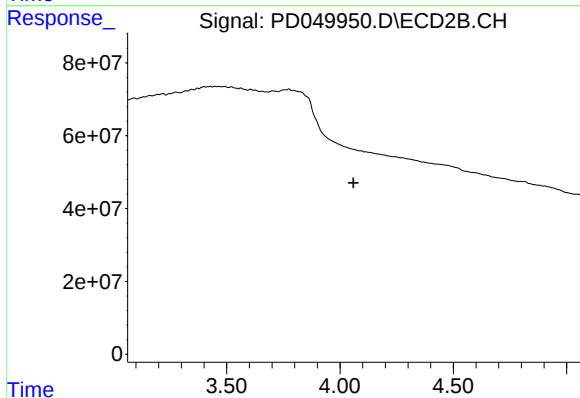


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.060 min
Response: 0
Conc: N.D.

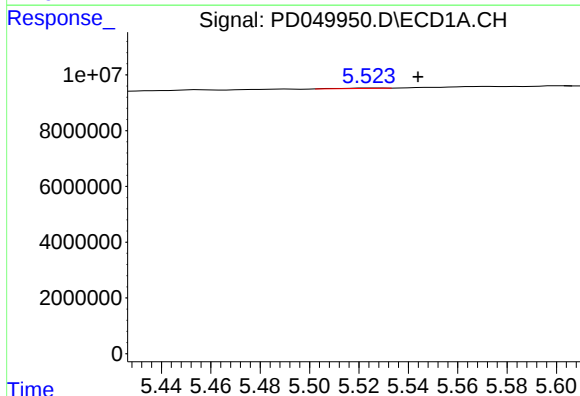


#5 Aldrin

R.T.: 5.525 min
Delta R.T.: -0.019 min
Response: 171291
Conc: 0.21 ng/ml

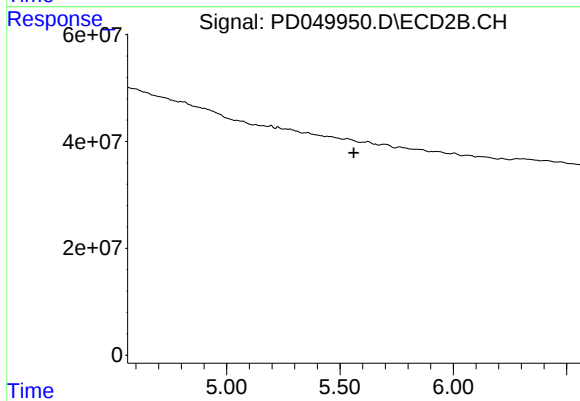

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.561 min
Response: 0
Conc: N.D.

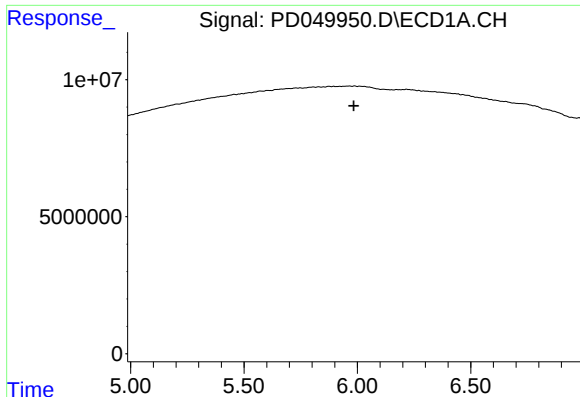

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.985 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

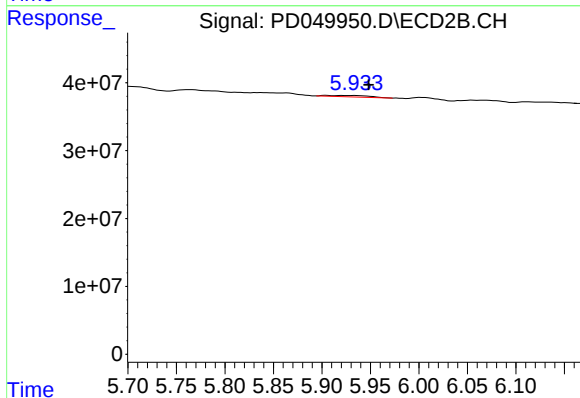


#8 Heptachlor epoxide

R.T.: 5.904 min
Delta R.T.: -0.044 min
Response: 4212893
Conc: 0.14 ng/ml

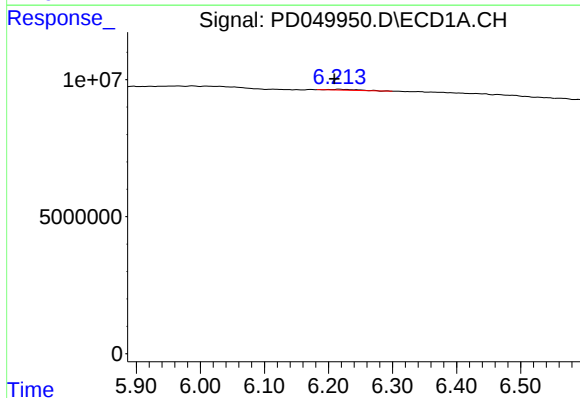


#10 trans-Chlordane

R.T.: 6.217 min
Delta R.T.: 0.008 min
Response: 890057
Conc: 1.06 ng/ml

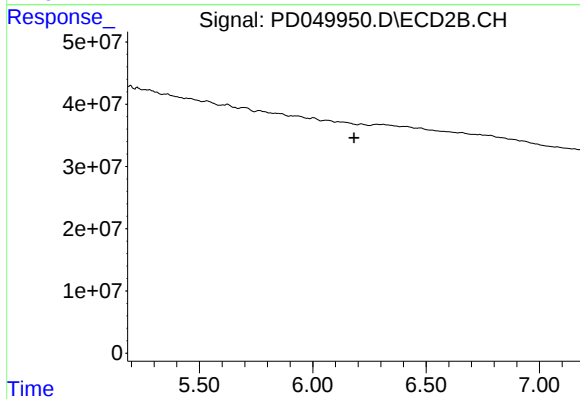

#10 trans-Chlordane


R.T.: 6.214 min
Delta R.T.: 0.032 min
Response: -440832
Conc: N.D.

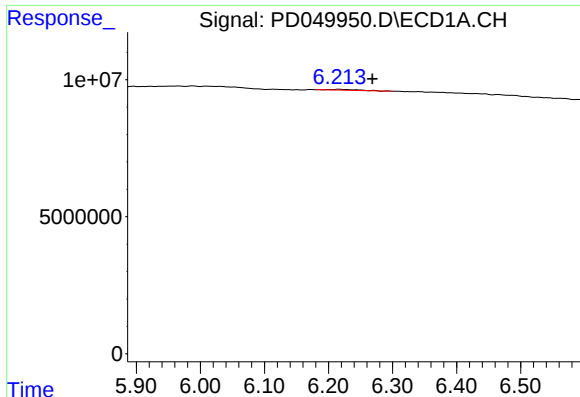

#11 cis-Chlordane


R.T.: 6.217 min
Delta R.T.: -0.052 min
Response: 890057
Conc: 1.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

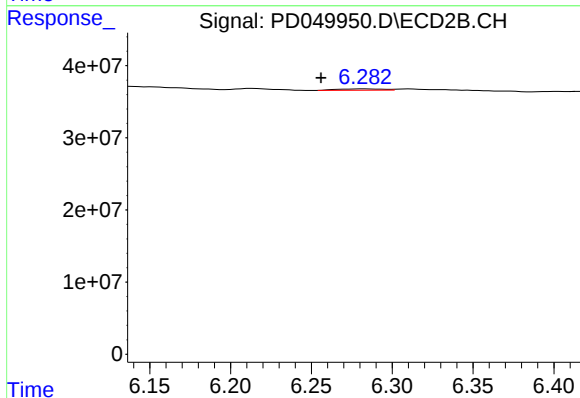


#11 cis-Chlordane

R.T.: 6.282 min
Delta R.T.: 0.026 min
Response: 3824943
Conc: 0.13 ng/ml

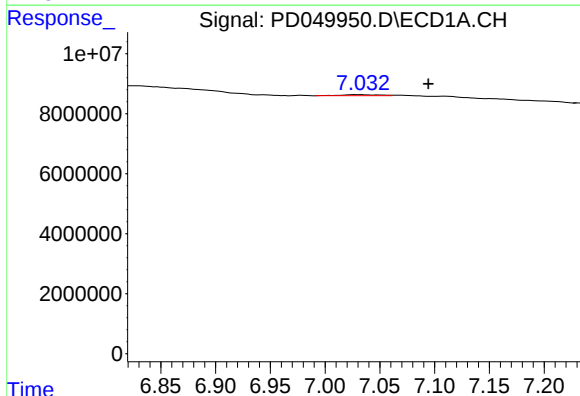


#15 Endosulfan II

R.T.: 7.031 min
Delta R.T.: -0.063 min
Response: 860231
Conc: 1.18 ng/ml

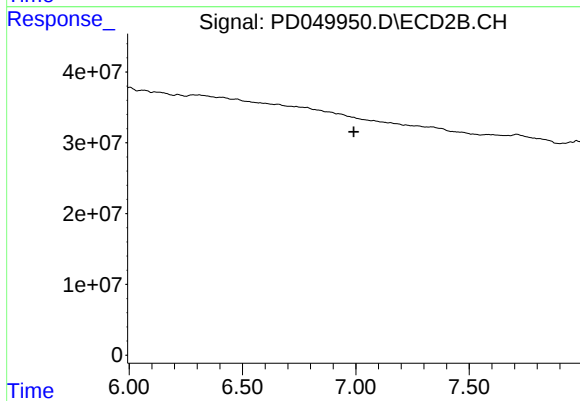

#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

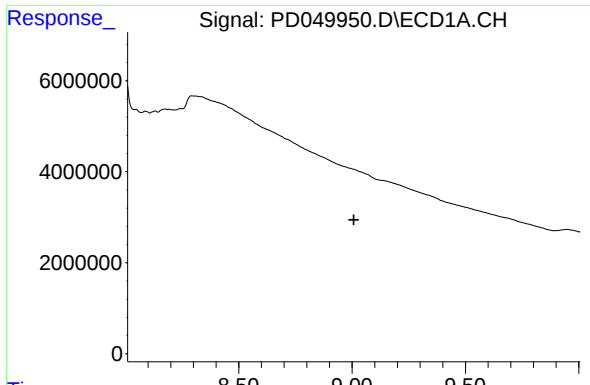

#27 Decachlorobiphenyl


R.T.: 0.000 min

Exp R.T.: 9.007 min

Response: 0

Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

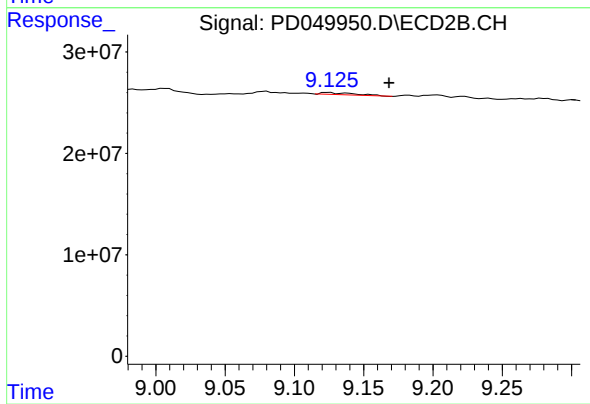

#27 Decachlorobiphenyl

R.T.: 9.138 min

Delta R.T.: -0.030 min

Response: 3464921

Conc: 0.19 ng/ml