

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102220\
 Data File : PD059889.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 18:26
 Operator : DD\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 02:20:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 02:19:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.024	7468816	12358655	5.082	4.808
27)	SA Decachlor...	8.305	9.109	19516621	21906419	10.591	10.399
Target Compounds							
2)	A alpha-BHC	3.949	4.415	11063359	18381734	4.931	4.846
3)	MA gamma-BHC...	4.235	4.701	11169148	16309498	5.138	4.709
4)	MA Heptachlor	4.543	5.212	10778058	16371647	4.880	4.827
9)	A Endosulfan I	5.583	6.263	9398134	13684799	4.975	4.929
13)	MA Dieldrin	5.829	6.520	20181290	29010848	9.516	9.542
14)	MA Endrin	6.088	6.738	16348380	22768172	9.498	9.474
16)	A 4,4'-DDD	6.213	6.857	16286901	23159487	9.669	9.637
17)	MA 4,4'-DDT	6.456	7.157	16920740	22126303	9.309	9.307
20)	A Methoxychlor	7.005	7.614	46655148	61568037	50.204	50.110

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102220\
Data File : PD059889.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 18:26
Operator : DD\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 02:20:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 02:19:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

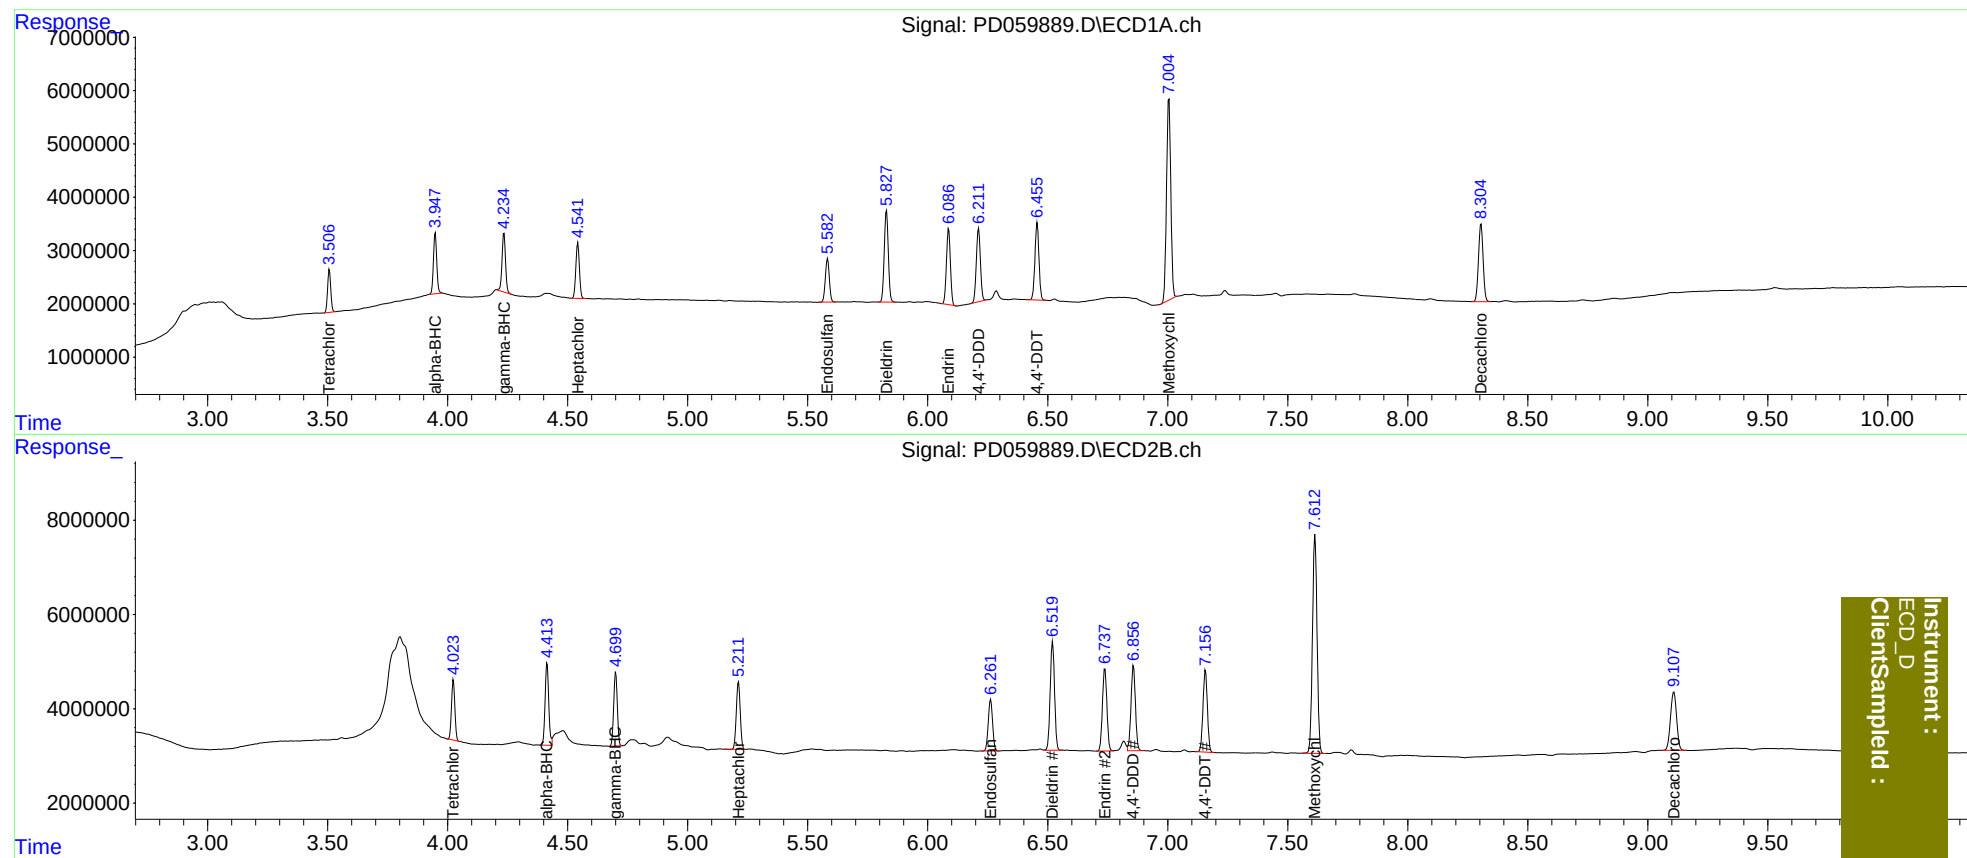


Instrument :
ECD_D
ClientSampled :

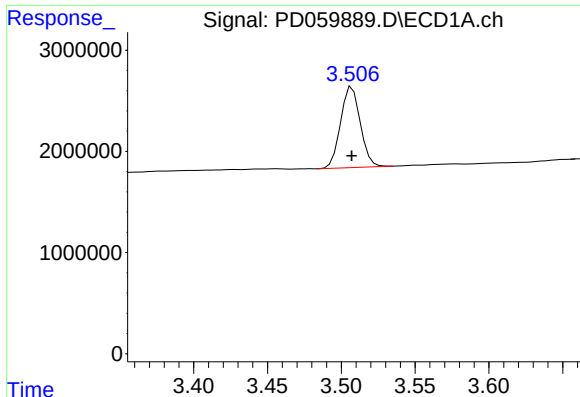

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 7468816
Conc: 5.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

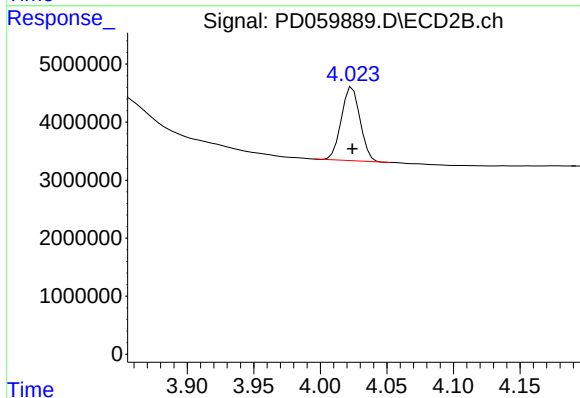


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 12358655
Conc: 4.81 ng/ml

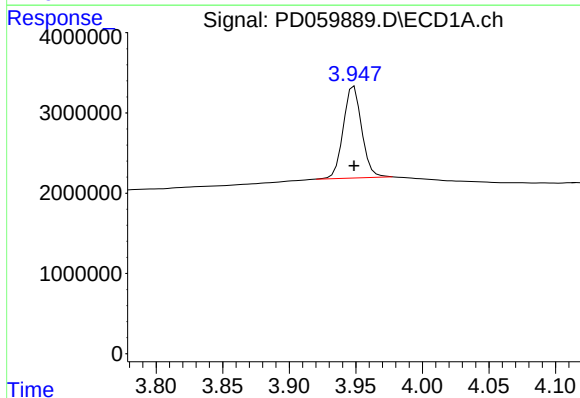


#2 alpha-BHC

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 11063359
Conc: 4.93 ng/ml

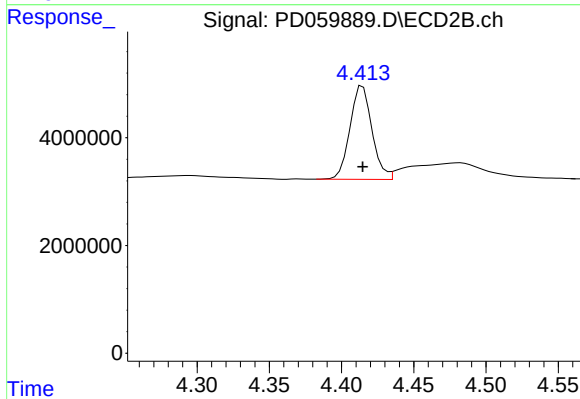

#2 alpha-BHC


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 18381734
Conc: 4.85 ng/ml

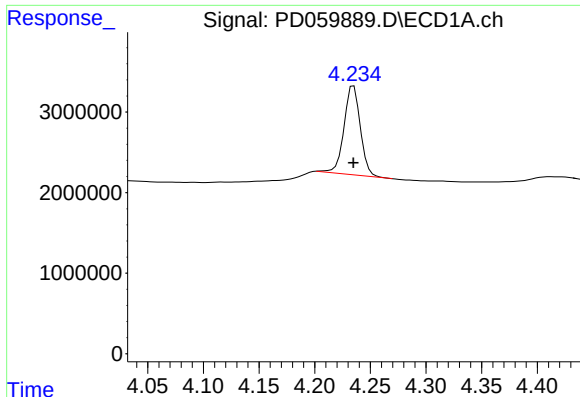

#3 gamma-BHC (Lindane)


R.T.: 4.235 min
Delta R.T.: 0.000 min
Response: 11169148
Conc: 5.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

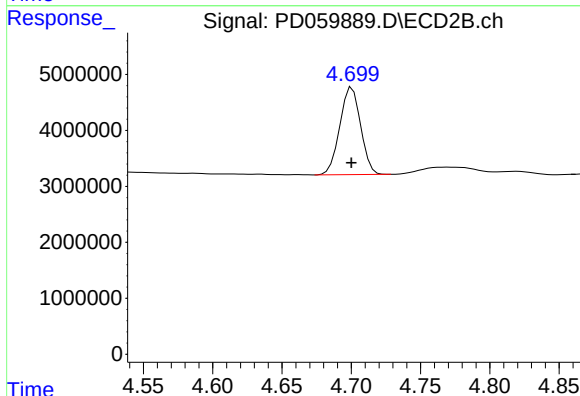


#3 gamma-BHC (Lindane)

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 16309498
Conc: 4.71 ng/ml

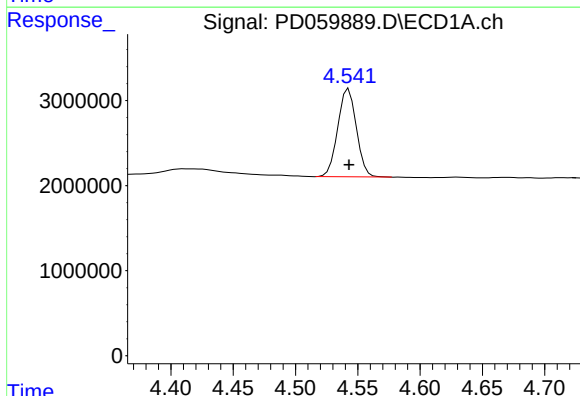


#4 Heptachlor

R.T.: 4.543 min
Delta R.T.: 0.000 min
Response: 10778058
Conc: 4.88 ng/ml

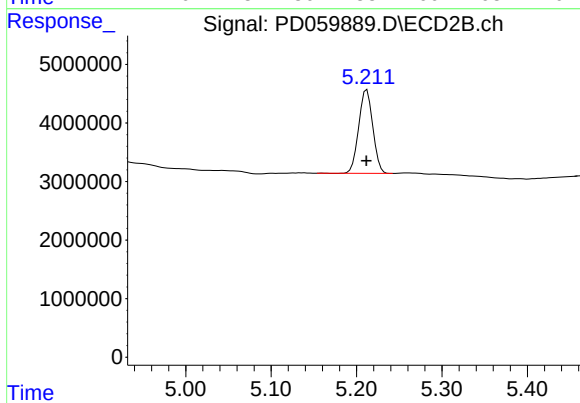

#4 Heptachlor


R.T.: 5.212 min
Delta R.T.: 0.000 min
Response: 16371647
Conc: 4.83 ng/ml

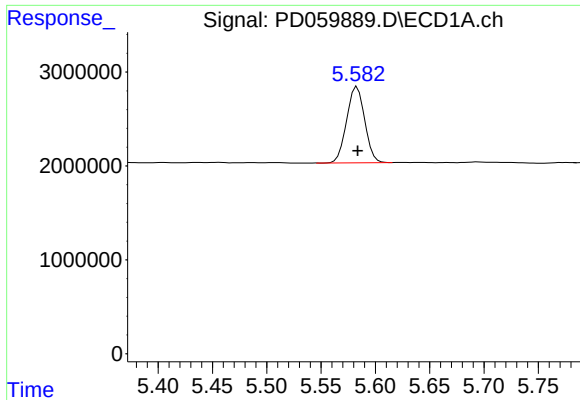

#9 Endosulfan I


R.T.: 5.583 min
Delta R.T.: 0.000 min
Response: 9398134
Conc: 4.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

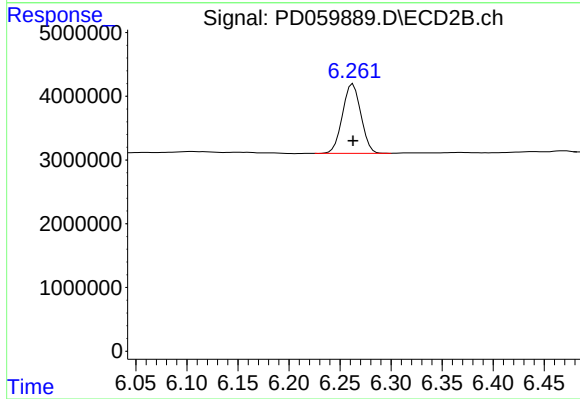


#9 Endosulfan I

R.T.: 6.263 min
Delta R.T.: 0.000 min
Response: 13684799
Conc: 4.93 ng/ml

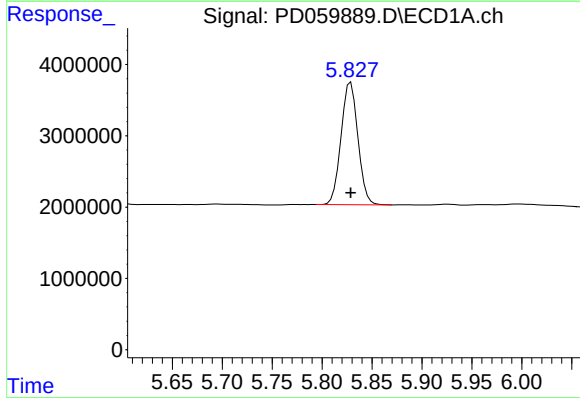


#13 Dieldrin

R.T.: 5.829 min
Delta R.T.: 0.000 min
Response: 20181290
Conc: 9.52 ng/ml

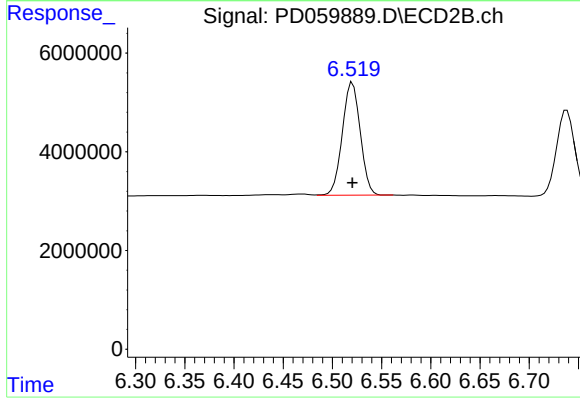

#13 Dieldrin


R.T.: 6.520 min
Delta R.T.: 0.000 min
Response: 29010848
Conc: 9.54 ng/ml

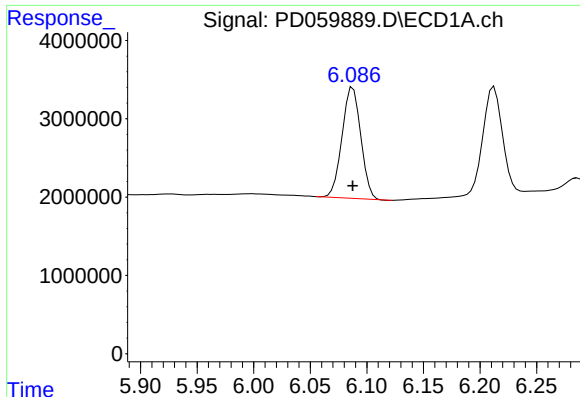

#14 Endrin


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 16348380
Conc: 9.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

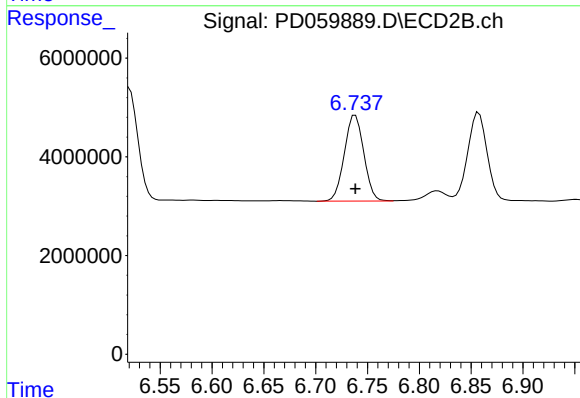


#14 Endrin

R.T.: 6.738 min
Delta R.T.: 0.000 min
Response: 22768172
Conc: 9.47 ng/ml

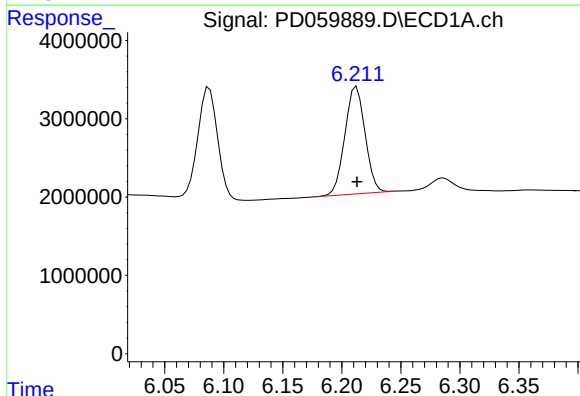


#16 4,4'-DDD

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 16286901
Conc: 9.67 ng/ml

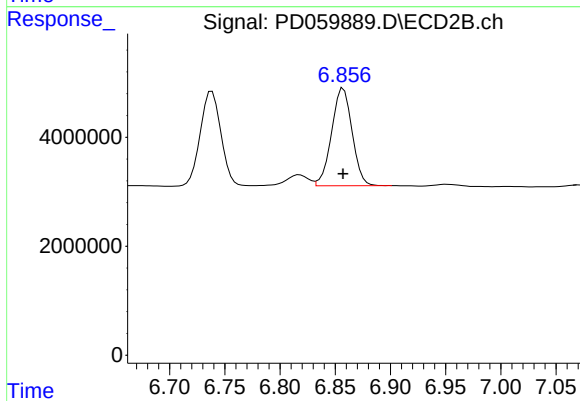

#16 4,4'-DDD


R.T.: 6.857 min
Delta R.T.: 0.000 min
Response: 23159487
Conc: 9.64 ng/ml

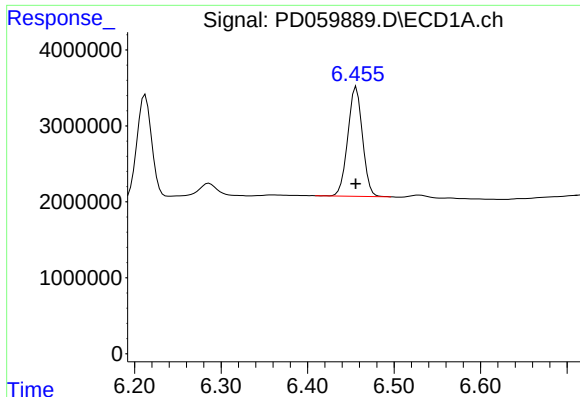

#17 4,4'-DDT


R.T.: 6.456 min
Delta R.T.: 0.000 min
Response: 16920740
Conc: 9.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

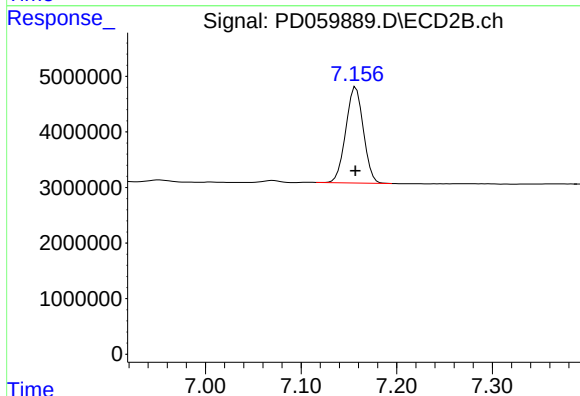


#17 4,4'-DDT

R.T.: 7.157 min
Delta R.T.: 0.000 min
Response: 22126303
Conc: 9.31 ng/ml

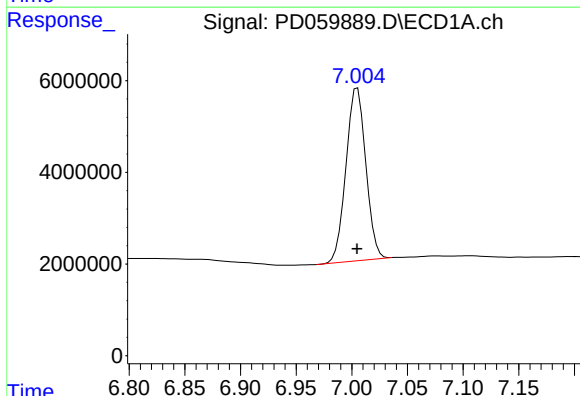


#20 Methoxychlor

R.T.: 7.005 min
Delta R.T.: 0.000 min
Response: 46655148
Conc: 50.20 ng/ml

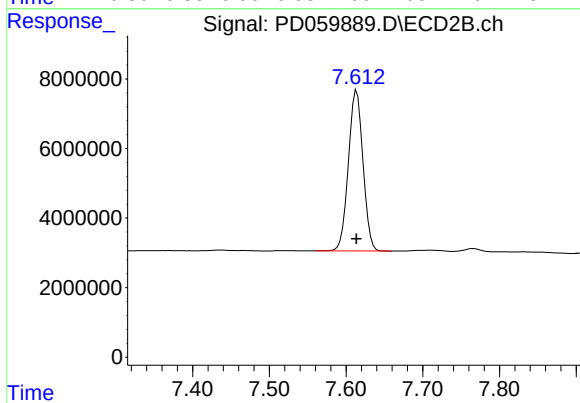

#20 Methoxychlor


R.T.: 7.614 min
Delta R.T.: 0.000 min
Response: 61568037
Conc: 50.11 ng/ml

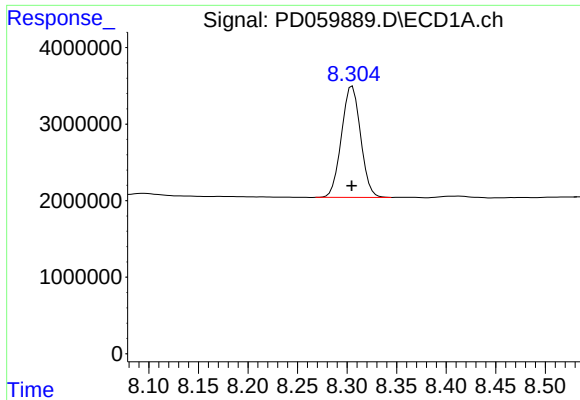

#27 Decachlorobiphenyl

R.T.: 8.305 min
Delta R.T.: 0.000 min
Response: 19516621
Conc: 10.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

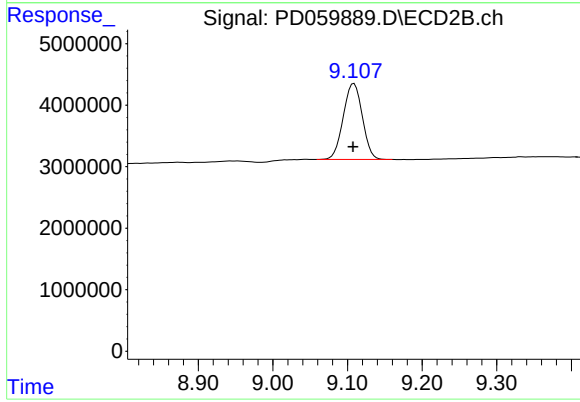

#27 Decachlorobiphenyl

R.T.: 9.109 min
Delta R.T.: 0.001 min
Response: 21906419
Conc: 10.40 ng/ml