

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102220\
 Data File : PD059893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 19:22
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 02:21:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 02:19:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.024	29393408	51412960	20.000	20.000
27)	SA Decachlor...	8.305	9.107	73707788	84264250	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.949	4.415	44871922	75866458	20.000	20.000
3)	MA gamma-BHC...	4.235	4.700	43473197	69271268	20.000	20.000
4)	MA Heptachlor	4.543	5.211	44176795	67834089	20.000	20.000
9)	A Endosulfan I	5.584	6.263	37782259	55532184	20.000	20.000
13)	MA Dieldrin	5.829	6.520	84830019	121.6E6	40.000	40.000
14)	MA Endrin	6.087	6.738	68848369	96126936	40.000	40.000
16)	A 4,4'-DDD	6.213	6.857	67377394	96124877	40.000	40.000
17)	MA 4,4'-DDT	6.456	7.157	72708718	95095514	40.000	40.000
20)	A Methoxychlor	7.005	7.614	185.9E6	245.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102220\
Data File : PD059893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 19:22
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 02:21:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 02:19:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

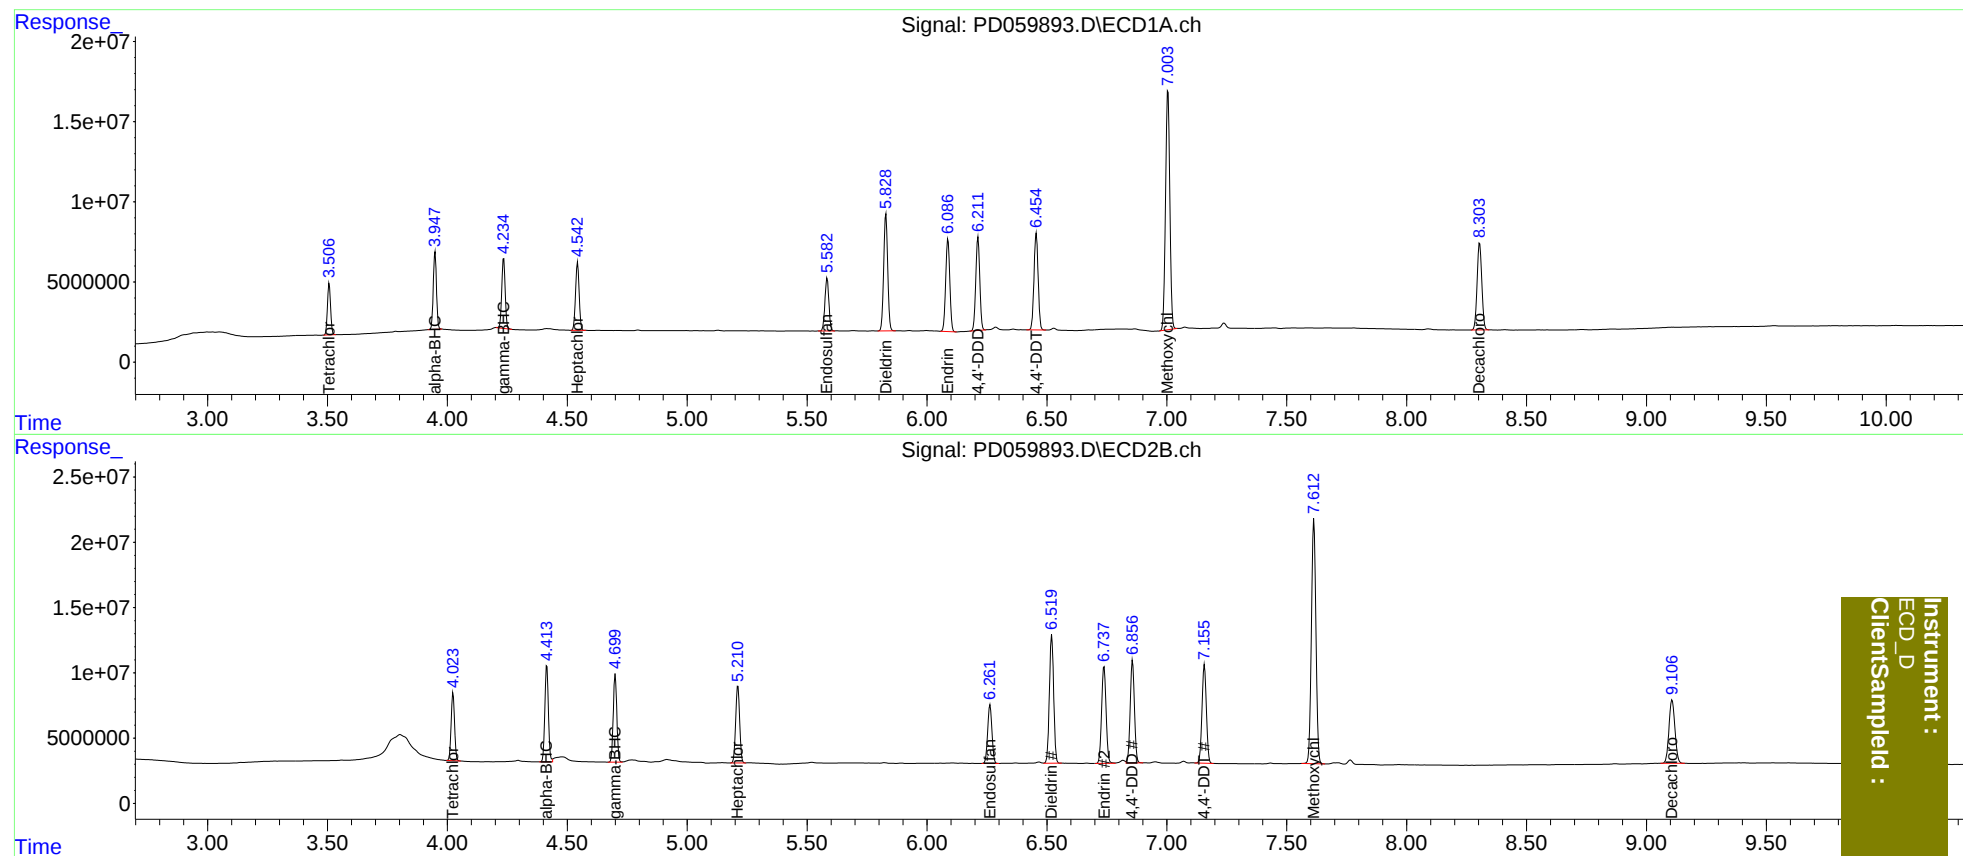


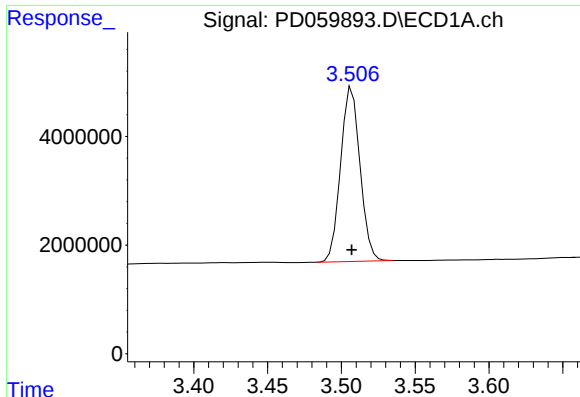

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 29393408
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

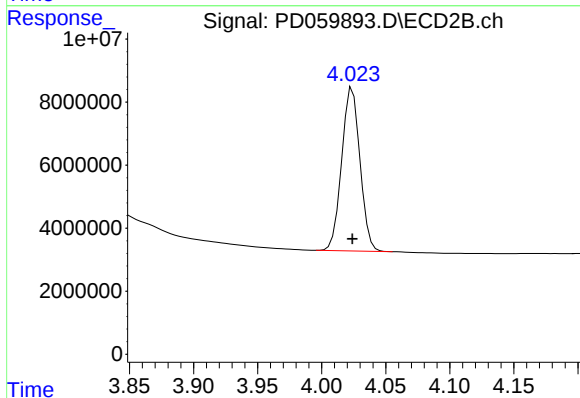


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 51412960
Conc: 20.00 ng/ml

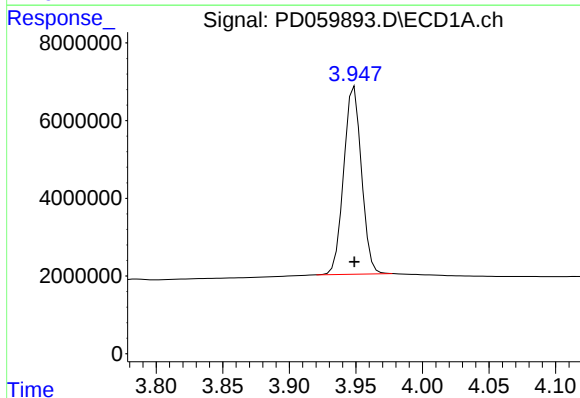


#2 alpha-BHC

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 44871922
Conc: 20.00 ng/ml

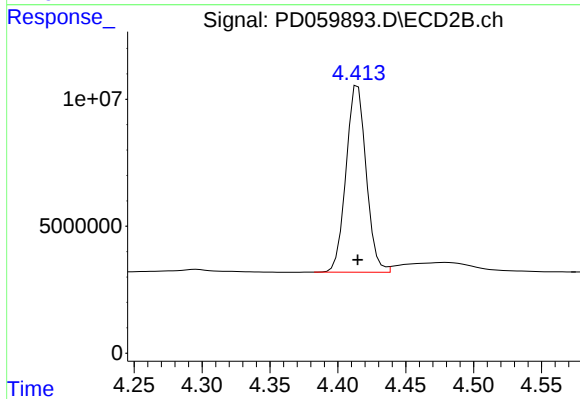

#2 alpha-BHC


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 75866458
Conc: 20.00 ng/ml

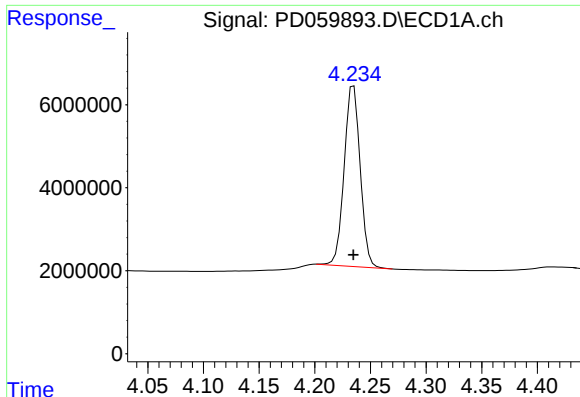

#3 gamma-BHC (Lindane)


R.T.: 4.235 min
Delta R.T.: 0.000 min
Response: 43473197
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

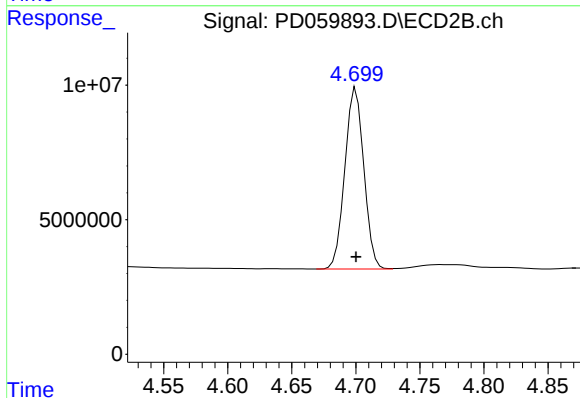


#3 gamma-BHC (Lindane)

R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 69271268
Conc: 20.00 ng/ml

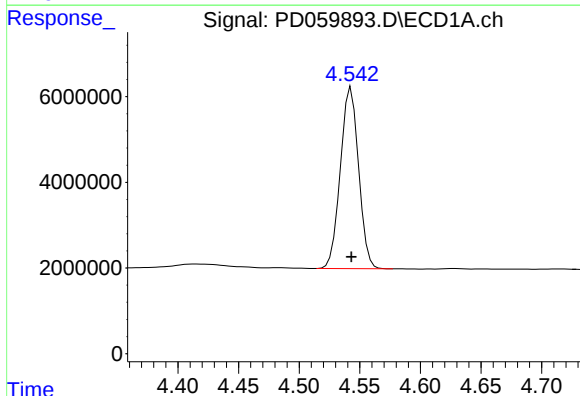


#4 Heptachlor

R.T.: 4.543 min
Delta R.T.: 0.000 min
Response: 44176795
Conc: 20.00 ng/ml

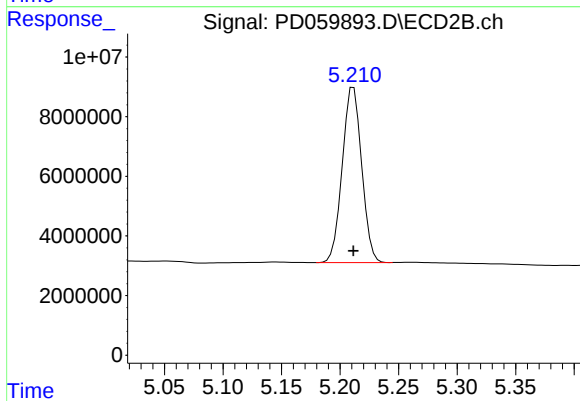

#4 Heptachlor


R.T.: 5.211 min
Delta R.T.: 0.000 min
Response: 67834089
Conc: 20.00 ng/ml

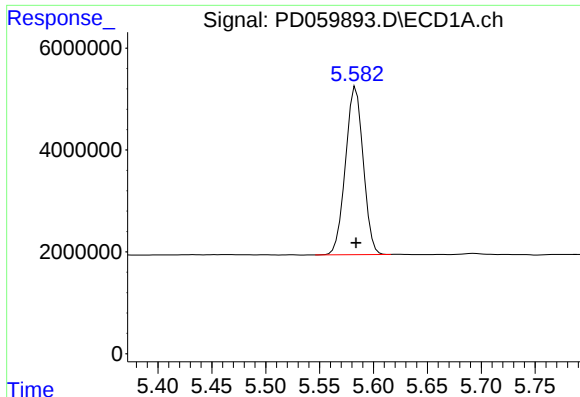

#9 Endosulfan I


R.T.: 5.584 min
Delta R.T.: 0.000 min
Response: 37782259
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

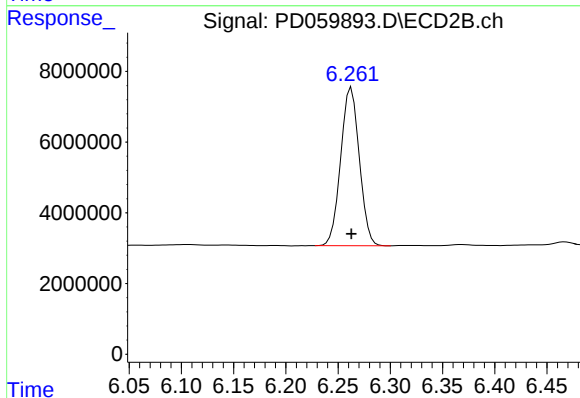


#9 Endosulfan I

R.T.: 6.263 min
Delta R.T.: 0.000 min
Response: 55532184
Conc: 20.00 ng/ml

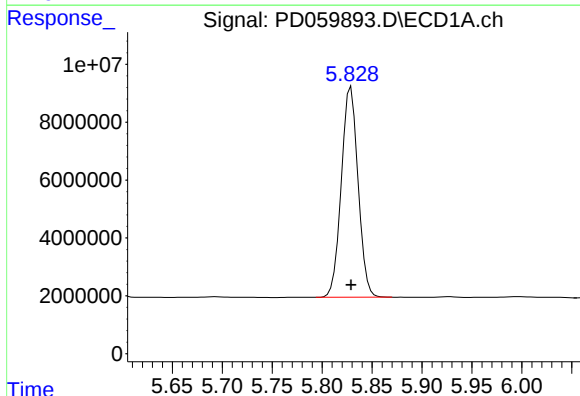


#13 Dieldrin

R.T.: 5.829 min
Delta R.T.: 0.000 min
Response: 84830019
Conc: 40.00 ng/ml

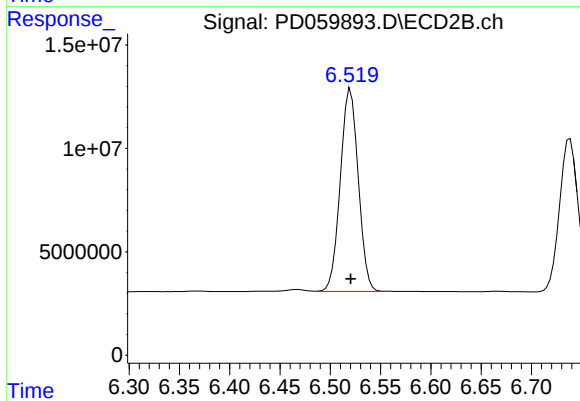

#13 Dieldrin


R.T.: 6.520 min
Delta R.T.: 0.000 min
Response: 121613712
Conc: 40.00 ng/ml

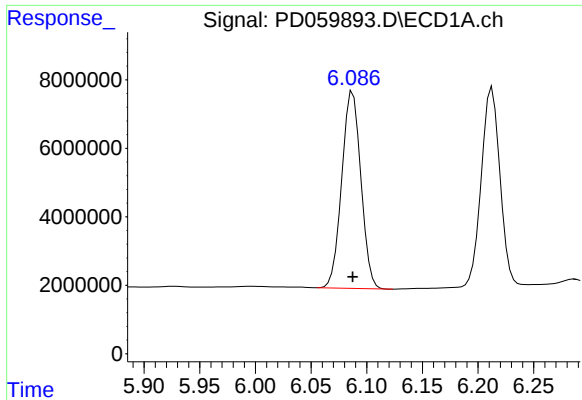

#14 Endrin


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 68848369
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

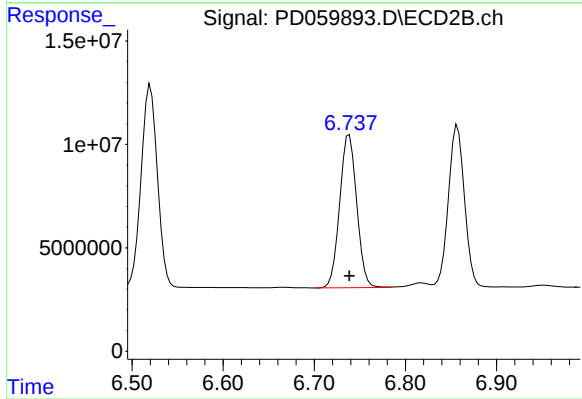


#14 Endrin

R.T.: 6.738 min
Delta R.T.: 0.000 min
Response: 96126936
Conc: 40.00 ng/ml

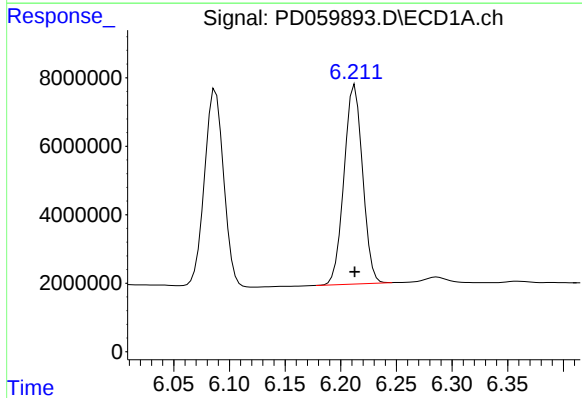


#16 4,4'-DDD

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 67377394
Conc: 40.00 ng/ml

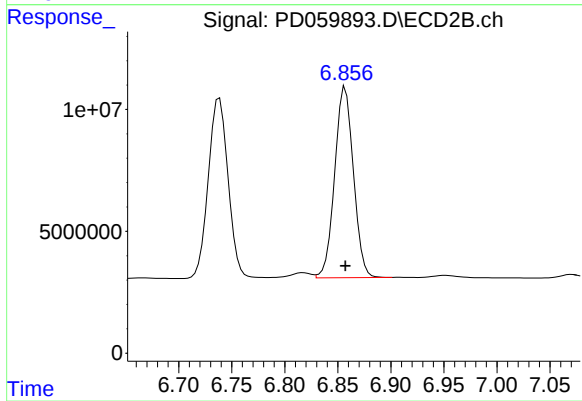

#16 4,4'-DDD


R.T.: 6.857 min
Delta R.T.: 0.000 min
Response: 96124877
Conc: 40.00 ng/ml

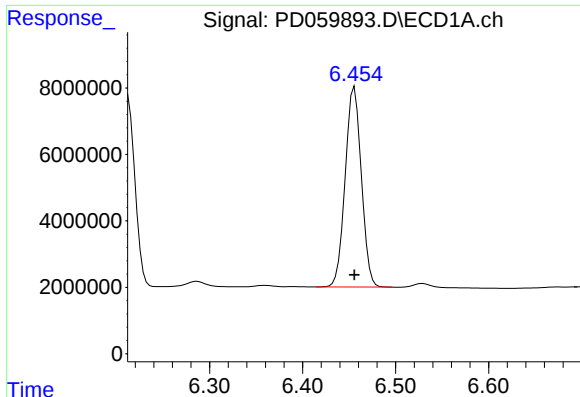

#17 4,4'-DDT


R.T.: 6.456 min
Delta R.T.: 0.000 min
Response: 72708718
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

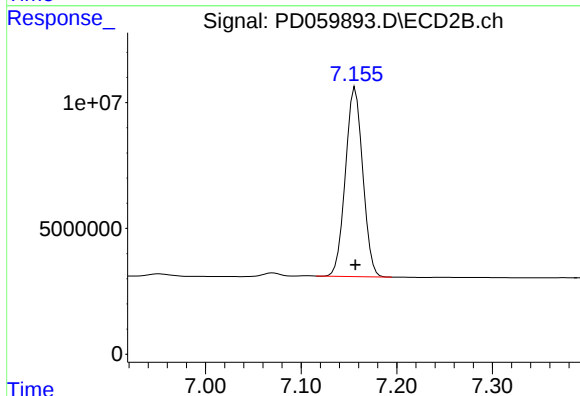


#17 4,4'-DDT

R.T.: 7.157 min
Delta R.T.: 0.000 min
Response: 95095514
Conc: 40.00 ng/ml

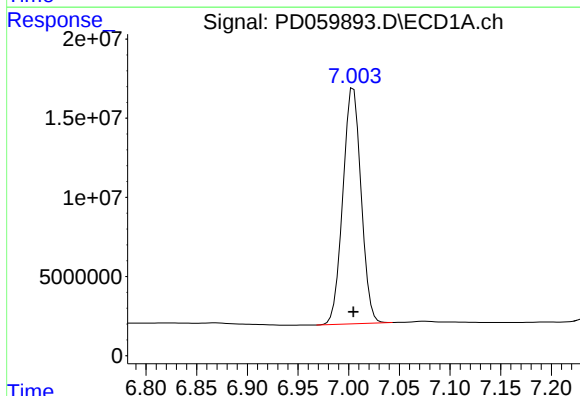


#20 Methoxychlor

R.T.: 7.005 min
Delta R.T.: 0.000 min
Response: 185863715
Conc: 200.00 ng/ml

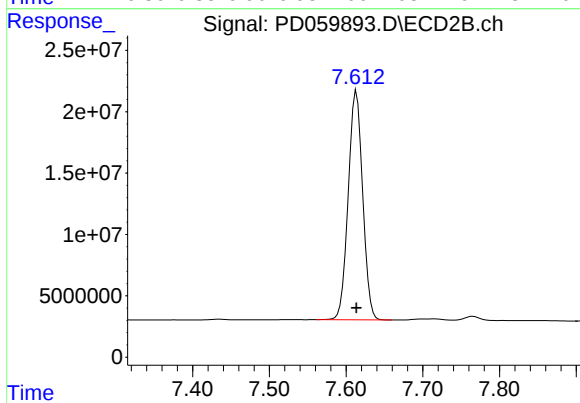

#20 Methoxychlor


R.T.: 7.614 min
Delta R.T.: 0.000 min
Response: 245731146
Conc: 200.00 ng/ml

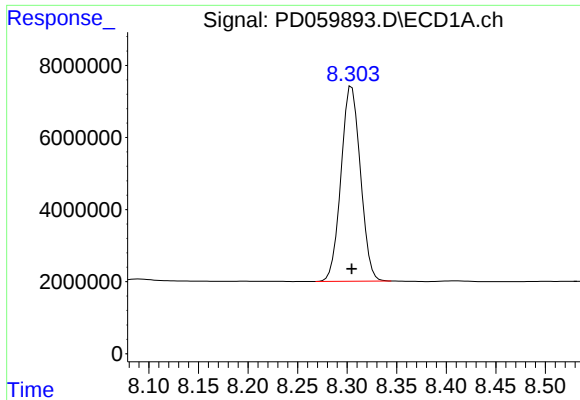

#27 Decachlorobiphenyl

R.T.: 8.305 min
Delta R.T.: 0.000 min
Response: 73707788
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

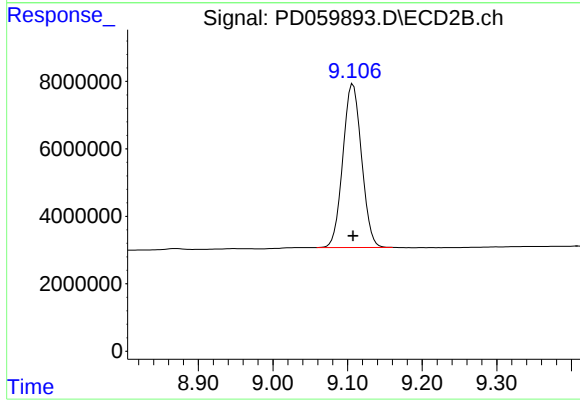

#27 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 84264250
Conc: 40.00 ng/ml