

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102220\
 Data File : PD059895.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 19:51
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 02:21:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 02:19:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.024	56859149	101.5E6	38.688	39.471
27)	SA Decachlor...	8.305	9.108	139.6E6	161.3E6	75.768	76.590
Target Compounds							
2)	A alpha-BHC	3.949	4.414	89689229	153.4E6	39.976	40.448
3)	MA gamma-BHC...	4.235	4.700	85035971	140.0E6	39.121	40.410
4)	MA Heptachlor	4.543	5.212	87269378	135.4E6	39.509	39.922
9)	A Endosulfan I	5.584	6.263	74370985	109.1E6	39.368	39.298
13)	MA Dieldrin	5.829	6.520	169.5E6	243.5E6	79.910	80.097
14)	MA Endrin	6.089	6.739	135.9E6	191.9E6	78.982	79.860
16)	A 4,4'-DDD	6.213	6.858	134.2E6	191.7E6	79.692	79.768
17)	MA 4,4'-DDT	6.456	7.157	146.0E6	192.5E6	80.297	80.962
20)	A Methoxychlor	7.005	7.613	355.8E6	472.5E6	382.809	384.553


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102220\
Data File : PD059895.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 19:51
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 02:21:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 02:19:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

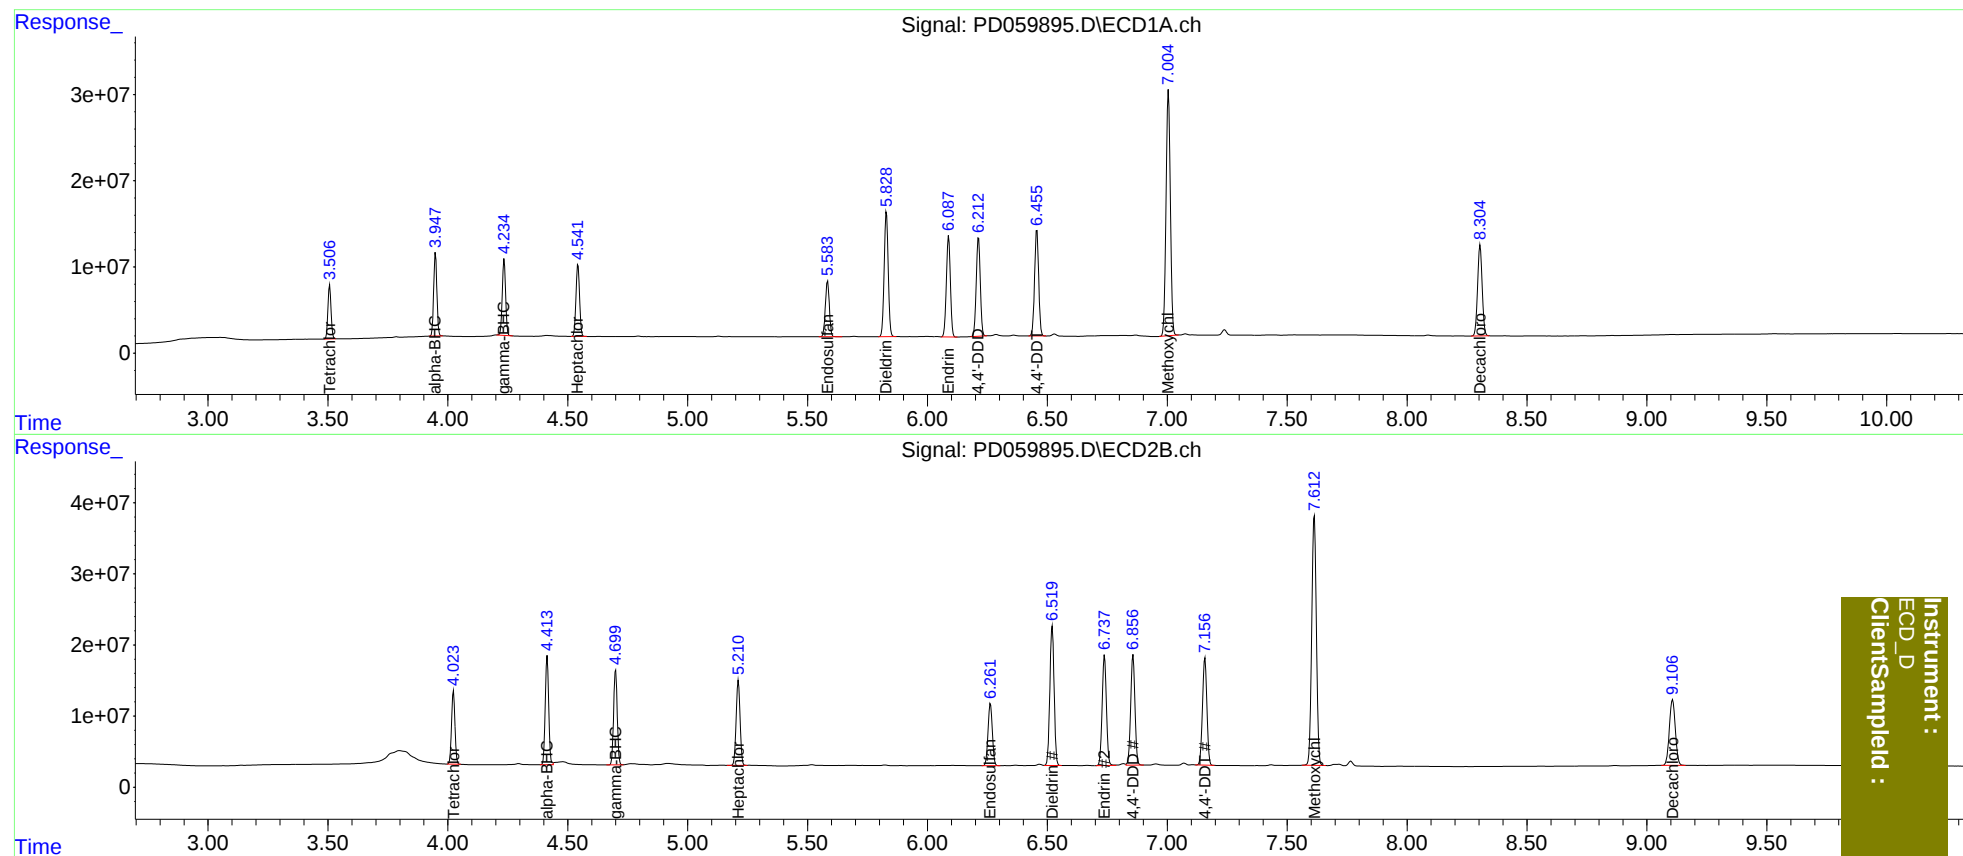


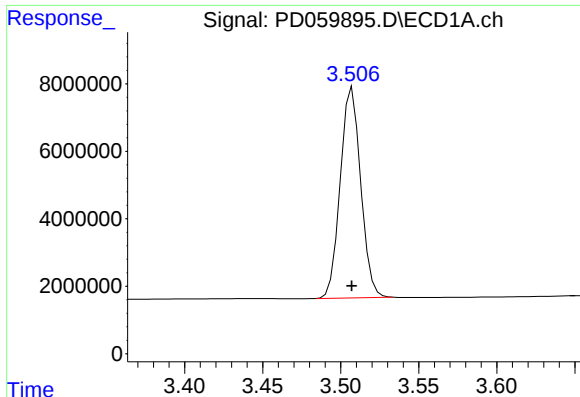

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 56859149
Conc: 38.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

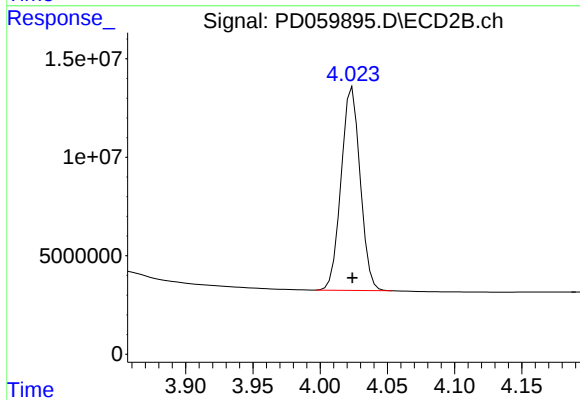


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 101467288
Conc: 39.47 ng/ml

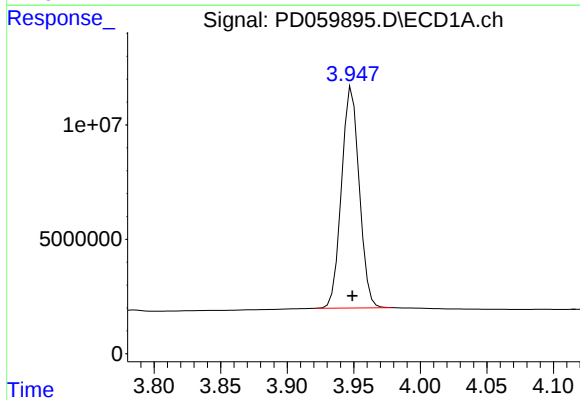


#2 alpha-BHC

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 89689229
Conc: 39.98 ng/ml

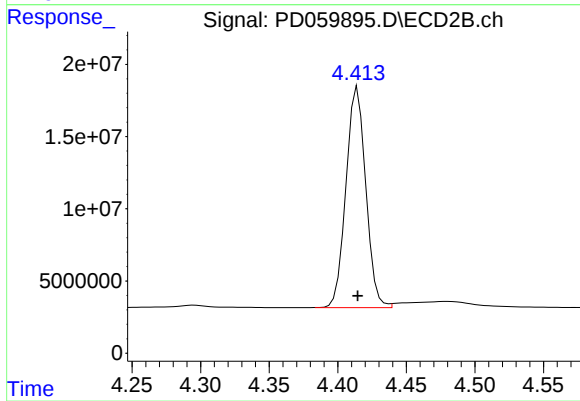

#2 alpha-BHC


R.T.: 4.414 min
Delta R.T.: 0.000 min
Response: 153433172
Conc: 40.45 ng/ml

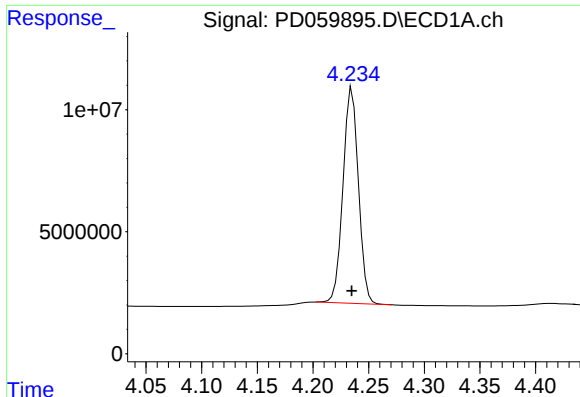

#3 gamma-BHC (Lindane)


R.T.: 4.235 min
Delta R.T.: 0.000 min
Response: 85035971
Conc: 39.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

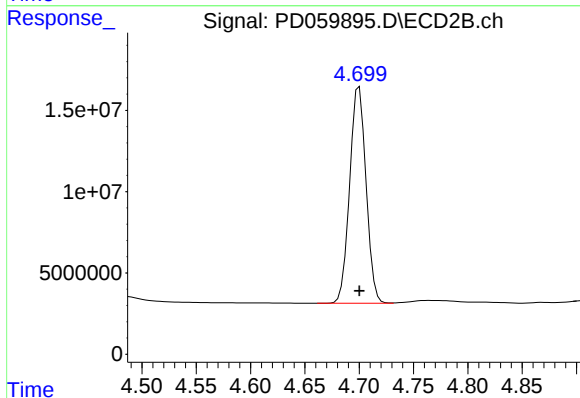


#3 gamma-BHC (Lindane)

R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 139963454
Conc: 40.41 ng/ml

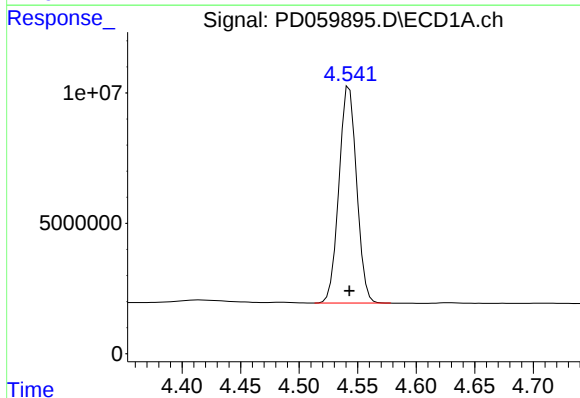


#4 Heptachlor

R.T.: 4.543 min
Delta R.T.: 0.000 min
Response: 87269378
Conc: 39.51 ng/ml

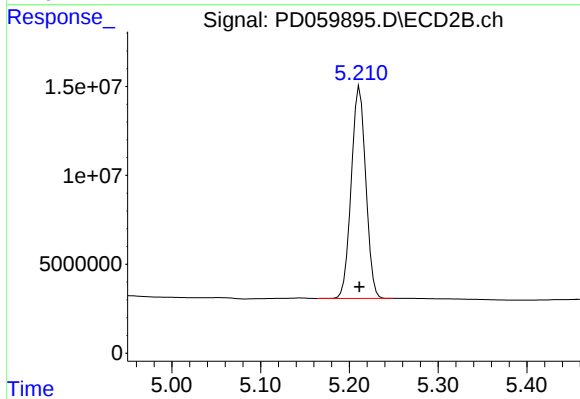

#4 Heptachlor


R.T.: 5.212 min
Delta R.T.: 0.000 min
Response: 135402639
Conc: 39.92 ng/ml

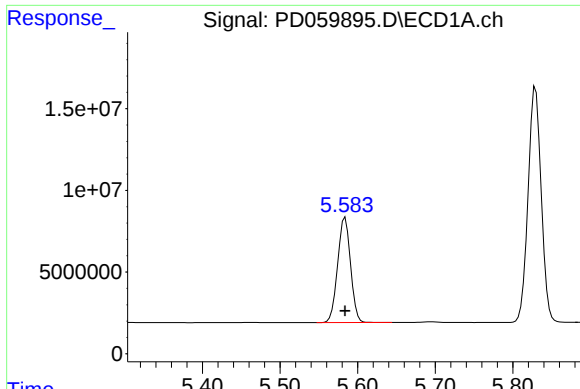

#9 Endosulfan I


R.T.: 5.584 min
Delta R.T.: 0.000 min
Response: 74370985
Conc: 39.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

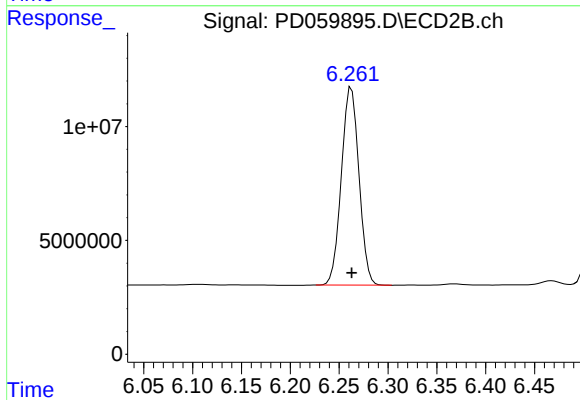


#9 Endosulfan I

R.T.: 6.263 min
Delta R.T.: 0.000 min
Response: 109116258
Conc: 39.30 ng/ml

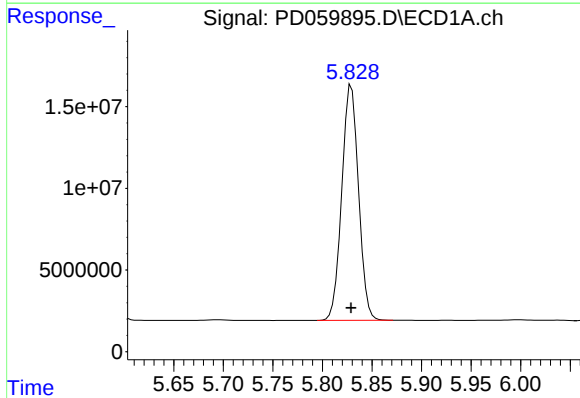


#13 Dieldrin

R.T.: 5.829 min
Delta R.T.: 0.000 min
Response: 169469515
Conc: 79.91 ng/ml

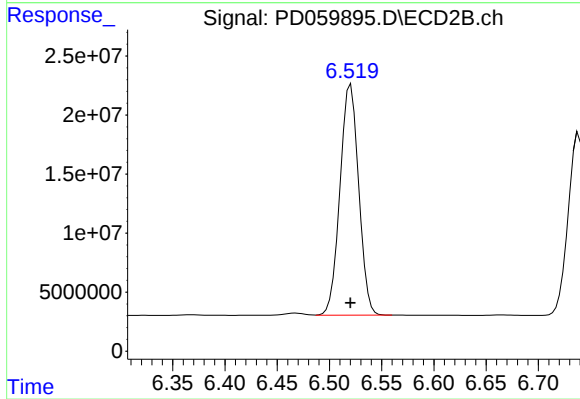

#13 Dieldrin


R.T.: 6.520 min
Delta R.T.: 0.000 min
Response: 243521677
Conc: 80.10 ng/ml

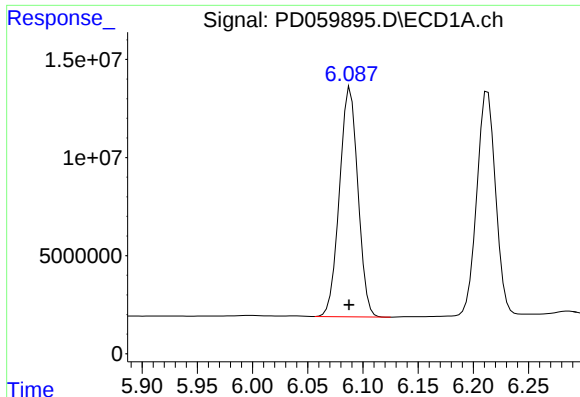

#14 Endrin


R.T.: 6.089 min
Delta R.T.: 0.001 min
Response: 135943946
Conc: 78.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

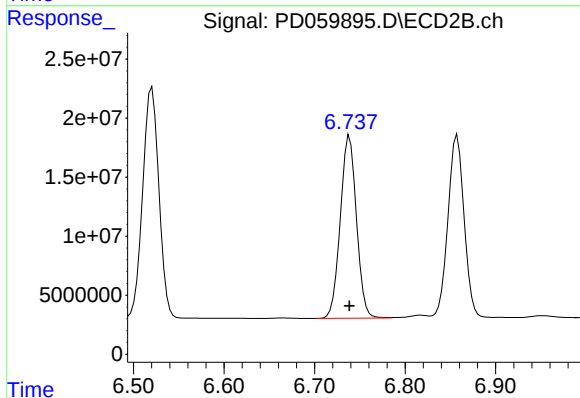


#14 Endrin

R.T.: 6.739 min
Delta R.T.: 0.000 min
Response: 191918567
Conc: 79.86 ng/ml

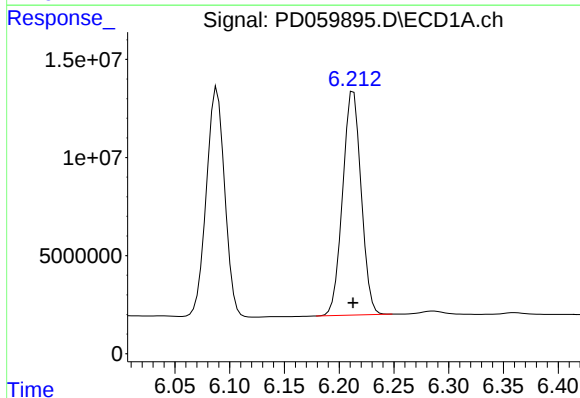


#16 4,4'-DDD

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 134235268
Conc: 79.69 ng/ml

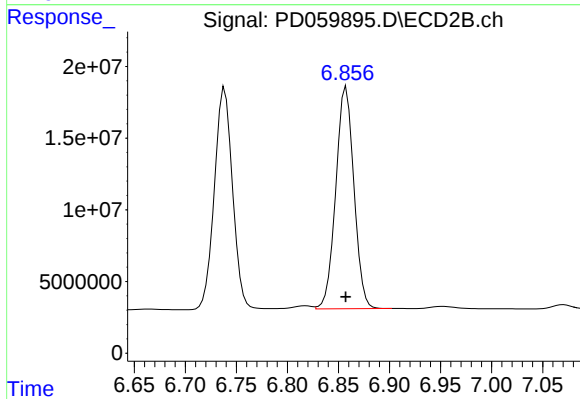

#16 4,4'-DDD


R.T.: 6.858 min
Delta R.T.: 0.000 min
Response: 191691242
Conc: 79.77 ng/ml

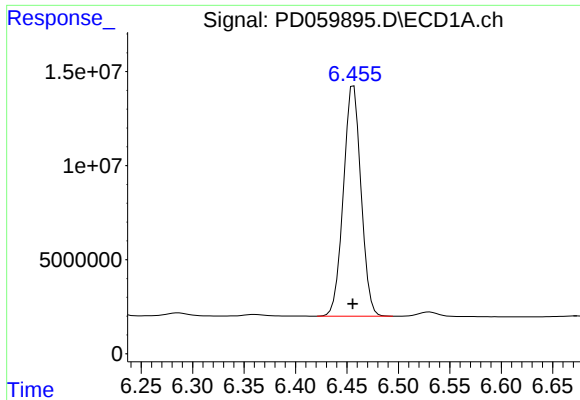

#17 4,4'-DDT


R.T.: 6.456 min
Delta R.T.: 0.000 min
Response: 145957507
Conc: 80.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

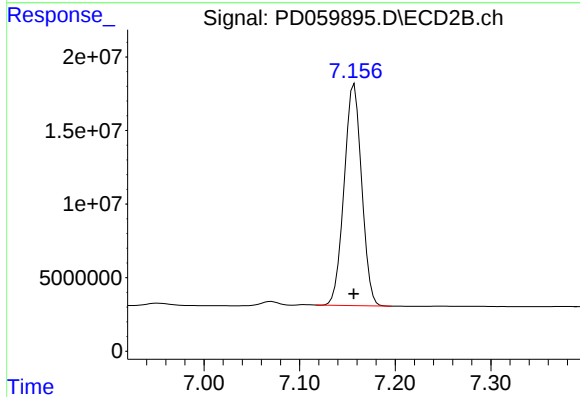


#17 4,4'-DDT

R.T.: 7.157 min
Delta R.T.: 0.000 min
Response: 192477958
Conc: 80.96 ng/ml

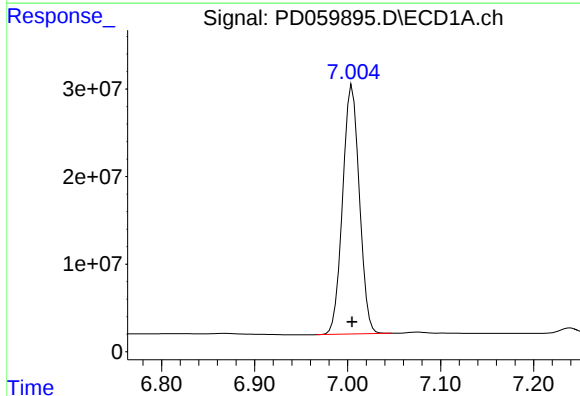


#20 Methoxychlor

R.T.: 7.005 min
Delta R.T.: 0.000 min
Response: 355751241
Conc: 382.81 ng/ml

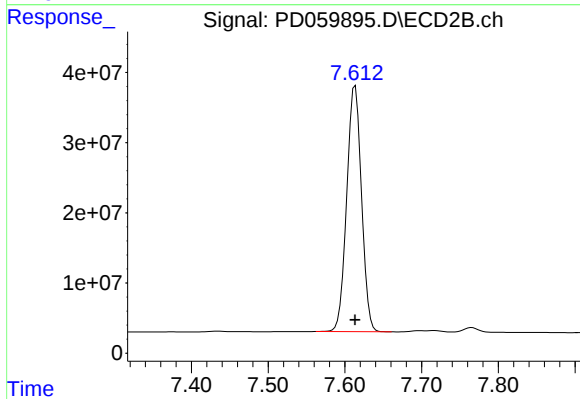

#20 Methoxychlor


R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 472482944
Conc: 384.55 ng/ml

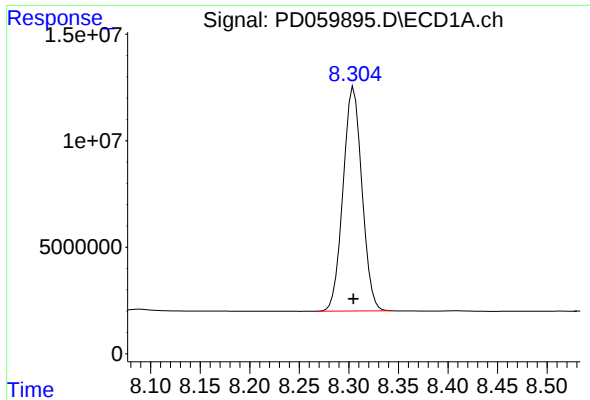

#27 Decachlorobiphenyl

R.T.: 8.305 min
Delta R.T.: 0.000 min
Response: 139617363
Conc: 75.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

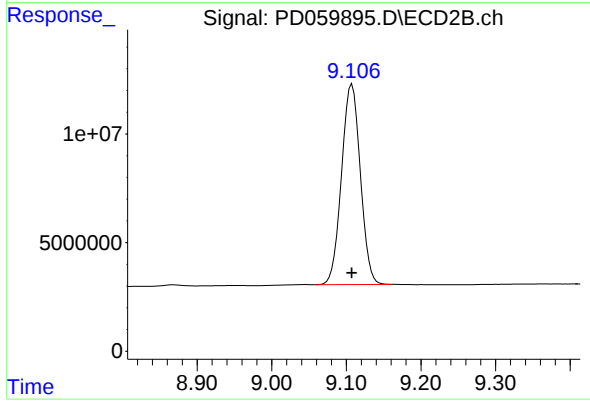

#27 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: 0.000 min
Response: 161345252
Conc: 76.59 ng/ml