

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102220\
 Data File : PD059897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2020 20:19
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 02:21:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 02:19:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.024	111.2E6	200.4E6	75.663	77.945
27)	SA Decachlor...	8.305	9.109	268.4E6	311.1E6	145.643	147.685
Target Compounds							
2)	A alpha-BHC	3.949	4.415	180.1E6	308.2E6	80.255	81.244
3)	MA gamma-BHC...	4.236	4.701	168.5E6	281.2E6	77.516	81.190
4)	MA Heptachlor	4.543	5.212	173.5E6	269.6E6	78.547	79.498
9)	A Endosulfan I	5.584	6.263	146.9E6	215.5E6	77.747	77.616
13)	MA Dieldrin	5.829	6.521	337.6E6	483.4E6	159.194	158.988
14)	MA Endrin	6.088	6.739	268.8E6	380.6E6	156.156	158.361
16)	A 4,4'-DDD	6.213	6.858	268.1E6	382.9E6	159.186	159.314
17)	MA 4,4'-DDT	6.456	7.157	292.0E6	387.4E6	160.623	162.952
20)	A Methoxychlor	7.005	7.614	671.8E6	894.6E6	722.896	728.090


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102220\
Data File : PD059897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2020 20:19
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 02:21:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 02:19:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

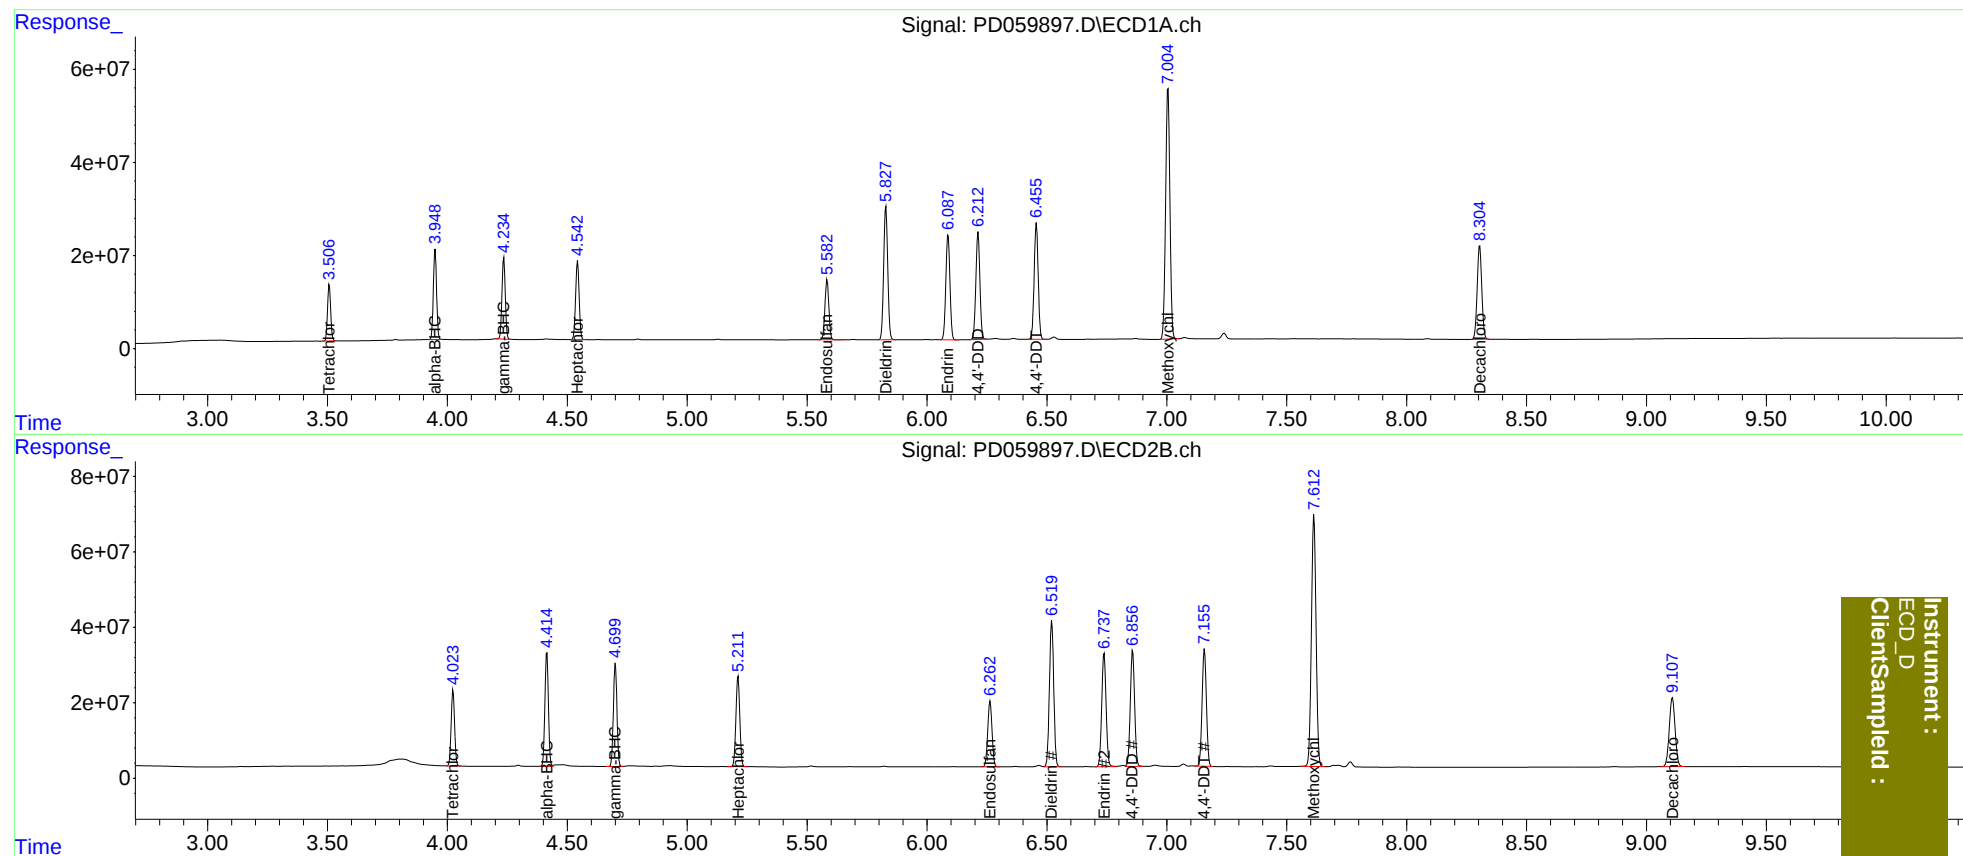


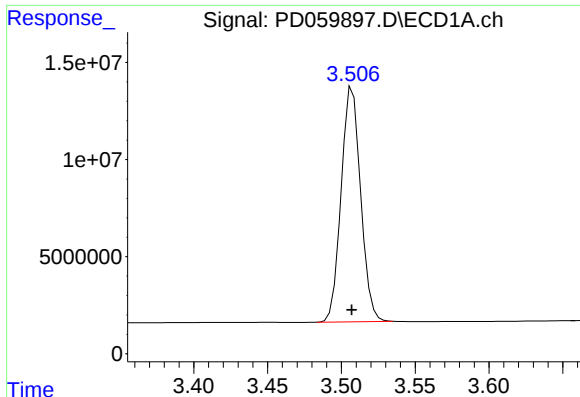

#1 Tetrachloro-m-xylene


R.T.: 3.508 min
Delta R.T.: 0.000 min
Response: 111200192
Conc: 75.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

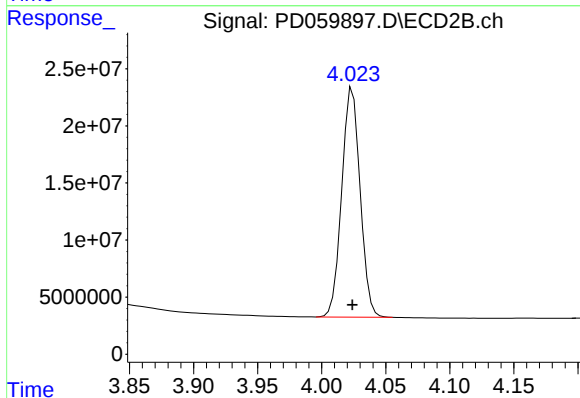


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 200369612
Conc: 77.95 ng/ml

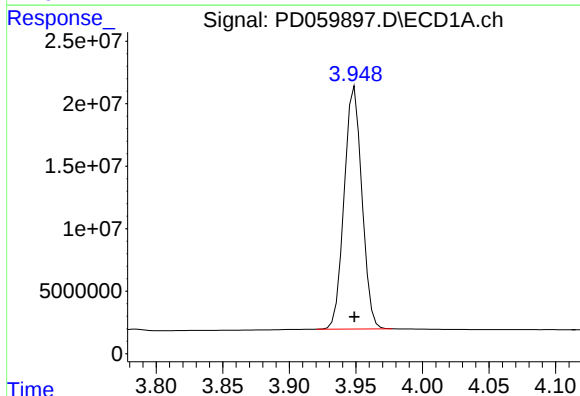


#2 alpha-BHC

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 180059646
Conc: 80.25 ng/ml

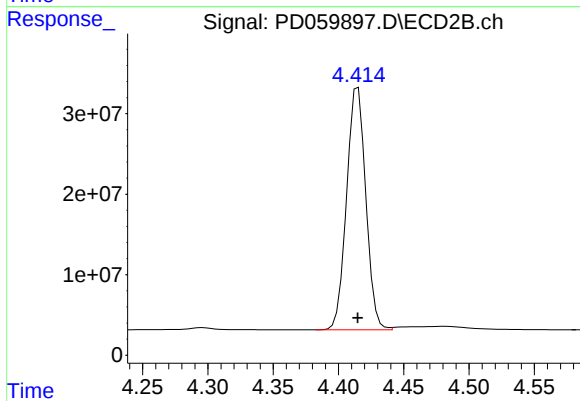

#2 alpha-BHC


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 308185207
Conc: 81.24 ng/ml

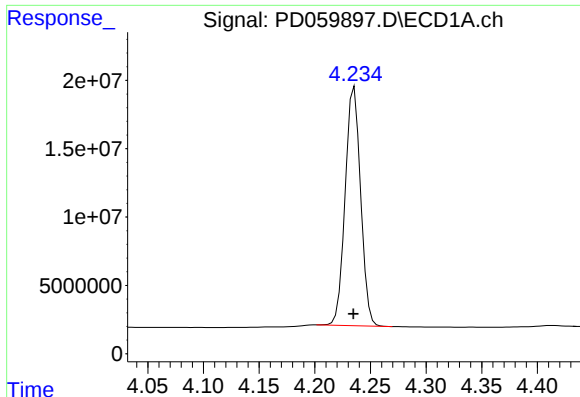

#3 gamma-BHC (Lindane)


R.T.: 4.236 min
Delta R.T.: 0.000 min
Response: 168494273
Conc: 77.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

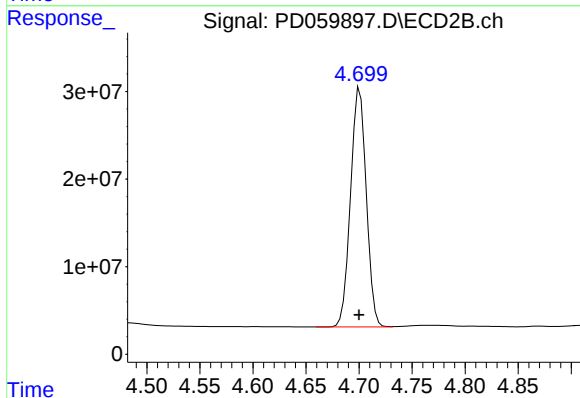


#3 gamma-BHC (Lindane)

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 281205654
Conc: 81.19 ng/ml

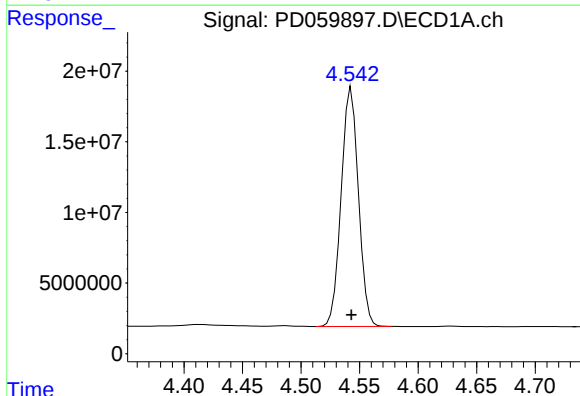


#4 Heptachlor

R.T.: 4.543 min
Delta R.T.: 0.000 min
Response: 173497714
Conc: 78.55 ng/ml

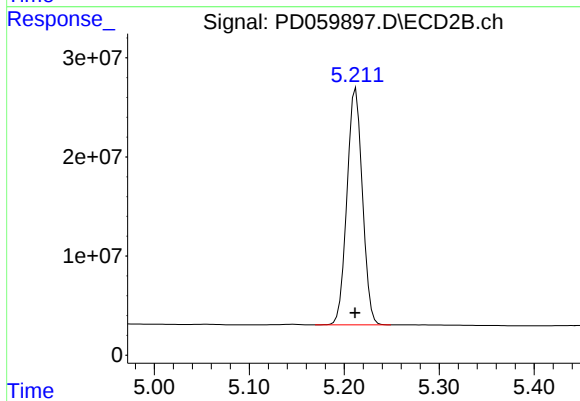

#4 Heptachlor


R.T.: 5.212 min
Delta R.T.: 0.000 min
Response: 269633835
Conc: 79.50 ng/ml

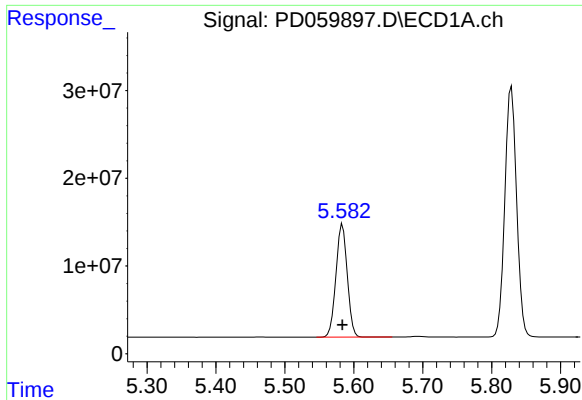

#9 Endosulfan I


R.T.: 5.584 min
Delta R.T.: 0.000 min
Response: 146872405
Conc: 77.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

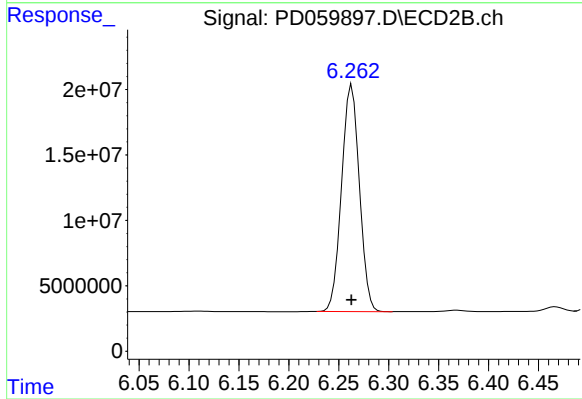


#9 Endosulfan I

R.T.: 6.263 min
Delta R.T.: 0.000 min
Response: 215509381
Conc: 77.62 ng/ml

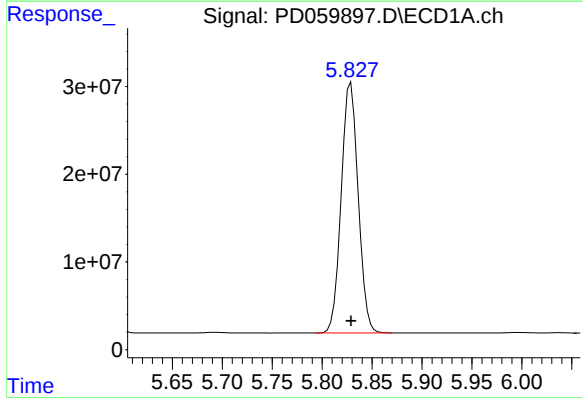


#13 Dieldrin

R.T.: 5.829 min
Delta R.T.: 0.000 min
Response: 337611219
Conc: 159.19 ng/ml

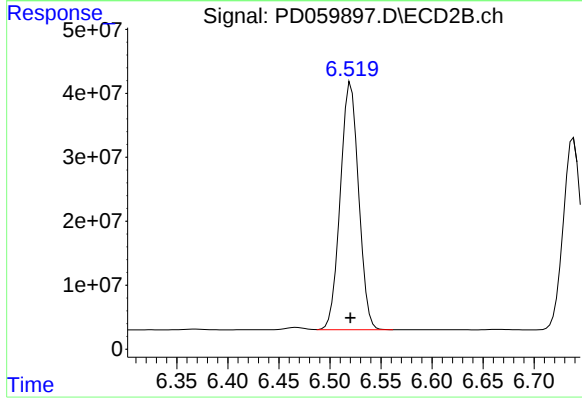

#13 Dieldrin


R.T.: 6.521 min
Delta R.T.: 0.000 min
Response: 483377420
Conc: 158.99 ng/ml

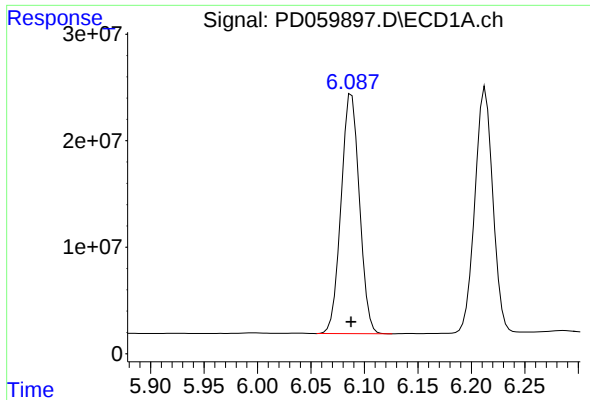

#14 Endrin


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 268777076
Conc: 156.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

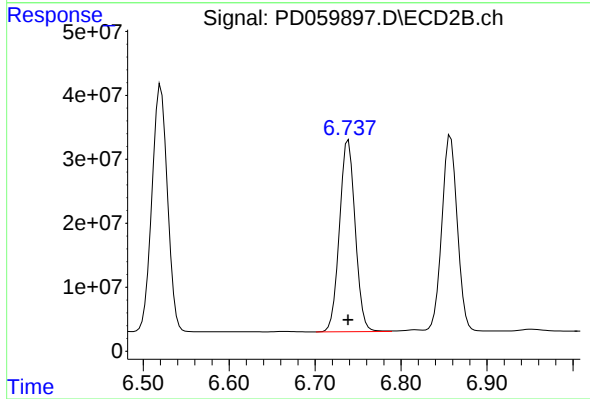


#14 Endrin

R.T.: 6.739 min
Delta R.T.: 0.000 min
Response: 380568183
Conc: 158.36 ng/ml

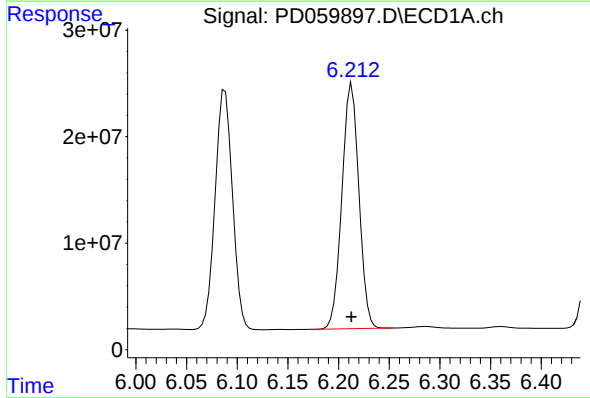


#16 4,4'-DDD

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 268138000
Conc: 159.19 ng/ml

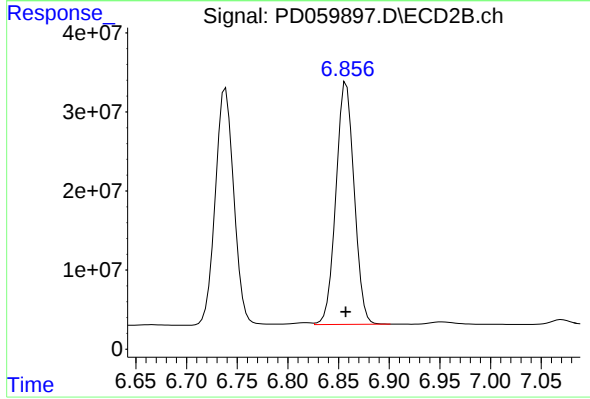

#16 4,4'-DDD


R.T.: 6.858 min
Delta R.T.: 0.000 min
Response: 382851466
Conc: 159.31 ng/ml

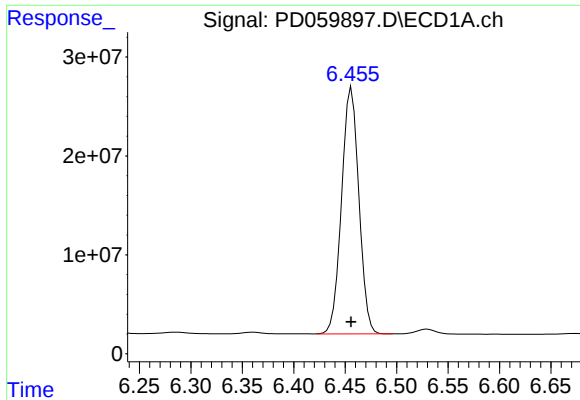

#17 4,4'-DDT


R.T.: 6.456 min
Delta R.T.: 0.000 min
Response: 291967062
Conc: 160.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

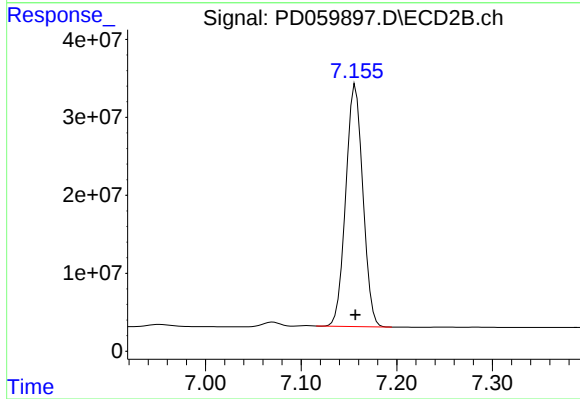


#17 4,4'-DDT

R.T.: 7.157 min
Delta R.T.: 0.000 min
Response: 387400170
Conc: 162.95 ng/ml

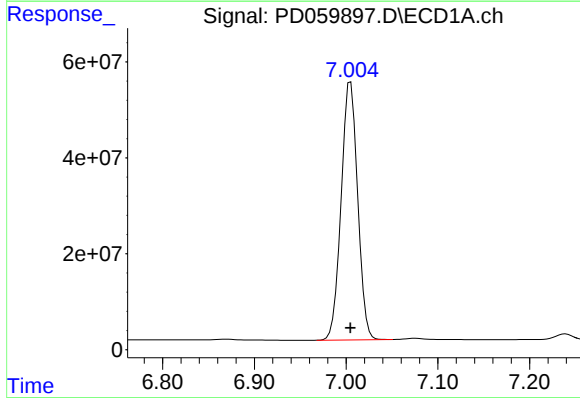


#20 Methoxychlor

R.T.: 7.005 min
Delta R.T.: 0.000 min
Response: 671800371
Conc: 722.90 ng/ml

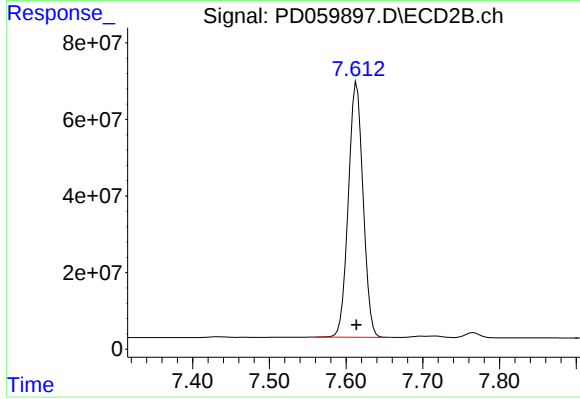

#20 Methoxychlor


R.T.: 7.614 min
Delta R.T.: 0.000 min
Response: 894571544
Conc: 728.09 ng/ml

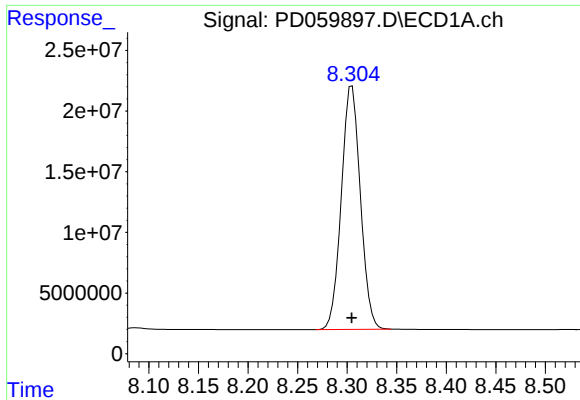

#27 Decachlorobiphenyl

R.T.: 8.305 min
Delta R.T.: 0.000 min
Response: 268376074
Conc: 145.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

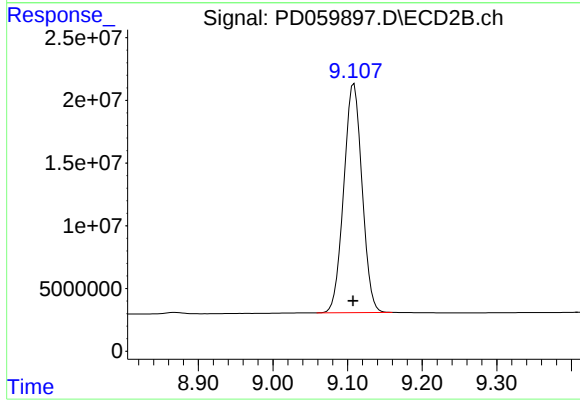

#27 Decachlorobiphenyl

R.T.: 9.109 min
Delta R.T.: 0.001 min
Response: 311115033
Conc: 147.69 ng/ml