

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102221\
 Data File : PD066509.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2021 16:30
 Operator : AJ\MA
 Sample : M4215-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 JDGC7

Manual Integrations
 APPROVED

mohammad
 10/25/2021 10:35:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 02:43:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 19 10:18:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.970	28567145	126.7E6	13.990	14.213
27)	SA Decachlor...	8.168	9.022	36119895	149.3E6	26.567	31.429
Target Compounds							
10)	B trans-Chl...	5.362	6.075	2681637	6828006	0.978m	0.755
12)	B 4,4'-DDE	5.586	6.302	2423462	4149655	0.968	0.522 #
15)	B Endosulfa...	6.260	6.894	4362091	11552582	1.942	1.621
17)	MA 4,4'-DDT	6.349	7.097	2380707	5255197	1.196m	0.801 #
18)	B Endrin al...	6.402	6.999	18006429	16540109	11.496m	3.120m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102221\
Data File : PD066509.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2021 16:30
Operator : AJ\MA
Sample : M4215-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 02:43:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101621CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 19 10:18:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

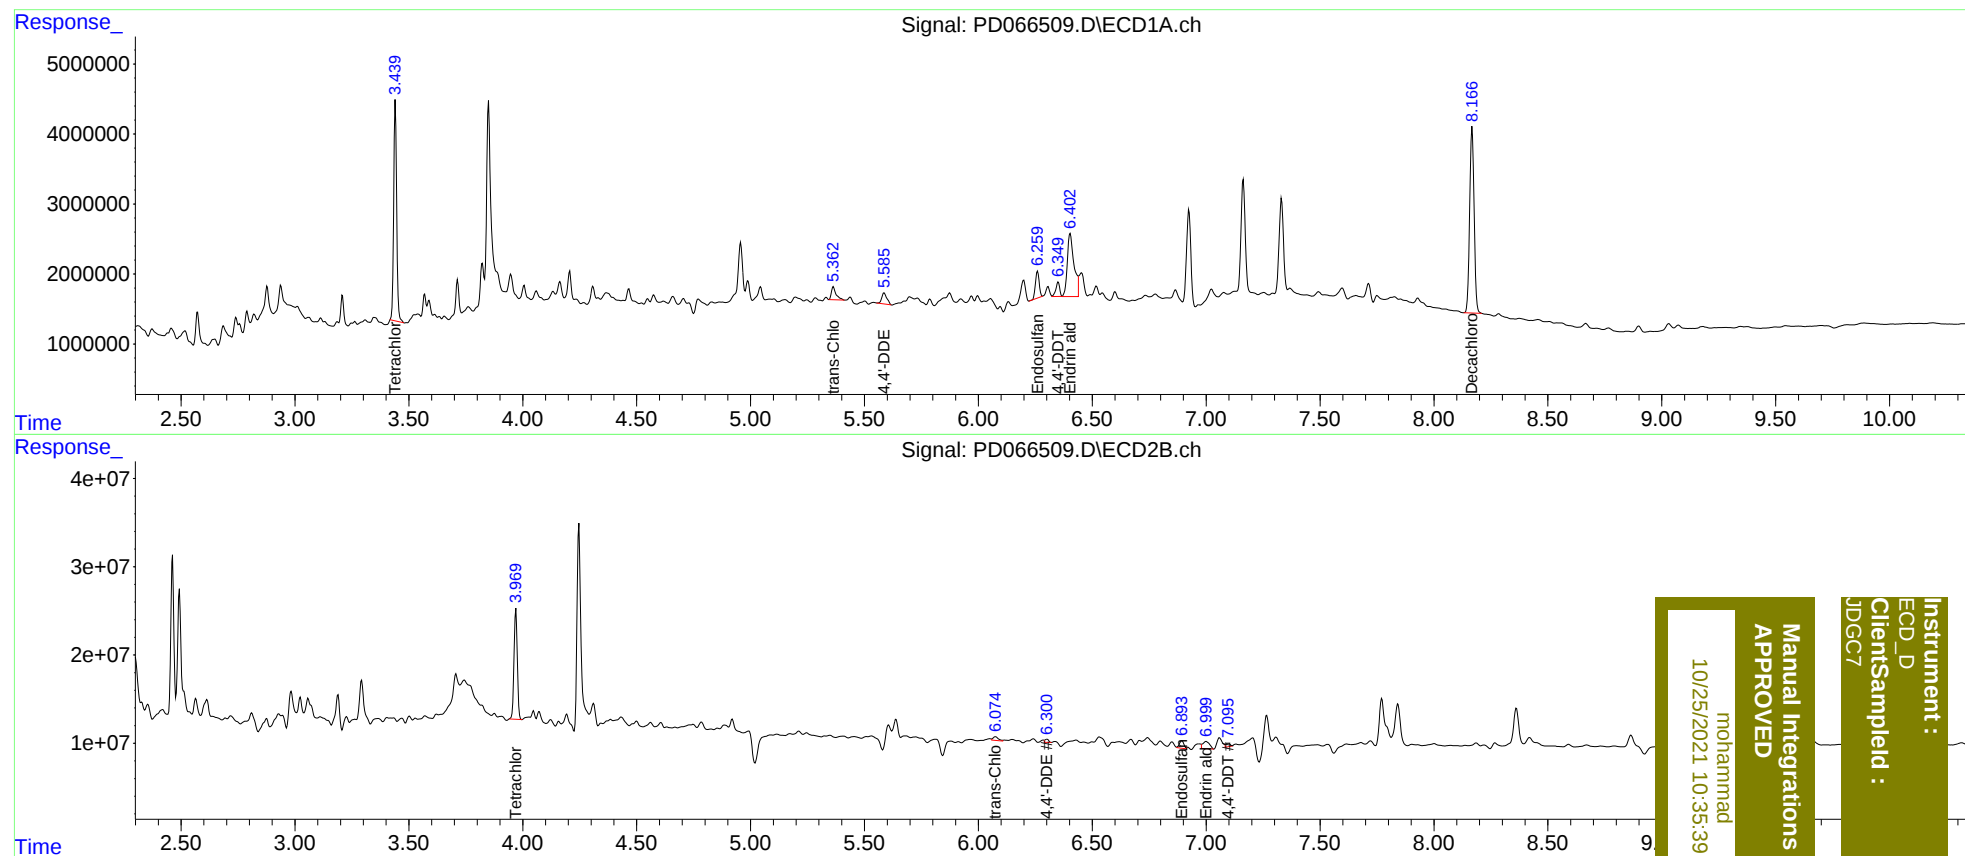

Manual Integrations
APPROVED

mohammad
10/25/2021 10:35:39 AM

Instrument :
ECD_D
ClientSampled :
JDGC7