

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102222\
 Data File : PD072569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2022 15:05
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:51:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 20 01:04:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.515f	0	14200877	N.D.	0.378
27)	SA Decachlor...	7.848	0.000	300304	0	0.150	N.D. #
Target Compounds							
4)	MA Heptachlor	3.856	0.000	41019	0	<MDL	N.D. #
5)	MB Aldrin	4.148	0.000	14432715	0	4.260	N.D. #
6)	B beta-BHC	3.856	0.000	41019	0	<MDL	N.D. #
7)	B delta-BHC	4.081	0.000	5675982	0	1.600	N.D. #
8)	B Heptachlo...	4.682	5.602	472987	253.9E6	0.156	13.050 #
10)	B trans-Chl...	4.901	0.000	2890281	0	0.930	N.D. #
11)	B cis-Chlor...	4.959	0.000	5103651	0	1.690	N.D. #
13)	MA Dieldrin	0.000	6.199f	0	30762943	N.D.	1.885
20)	A Methoxychlor	0.000	7.384f	0	61942086	N.D.	11.284
22)	Toxaphene-1	0.000	5.790	0	25726413	N.D.	402.738
23)	Toxaphene-2	0.000	6.199f	0	30762943	N.D.	270.628

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102222\
Data File : PD072569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2022 15:05
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:51:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 20 01:04:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

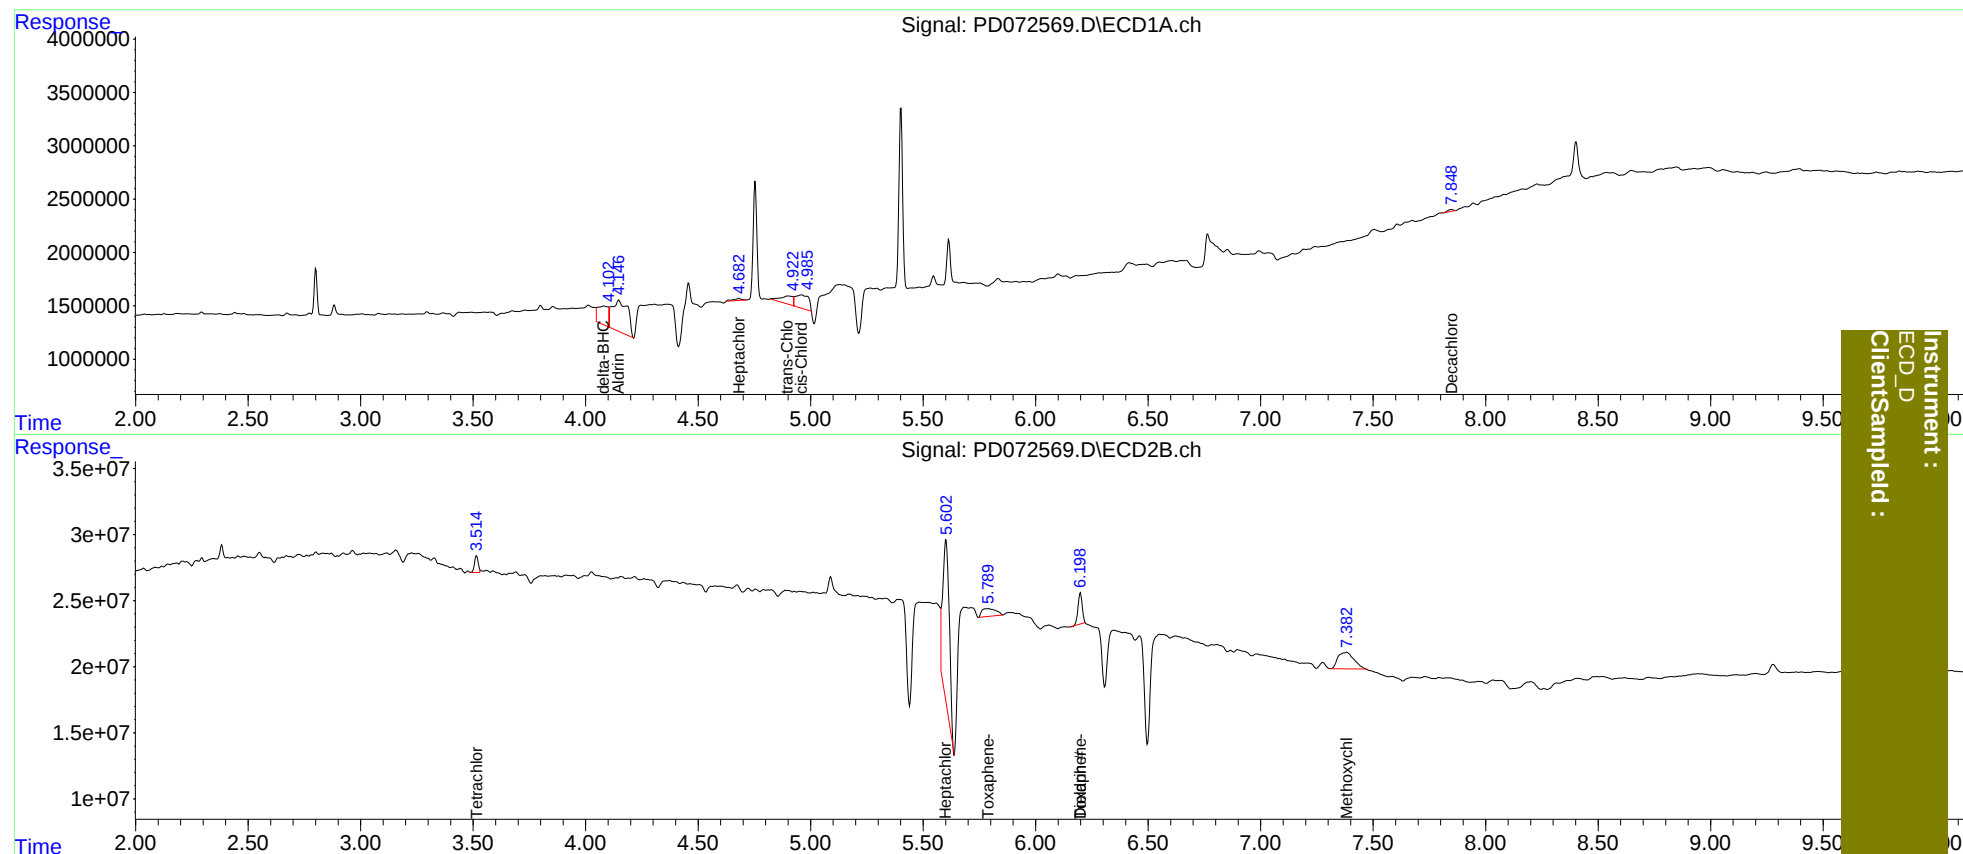


Instrument :
ECD_D
ClientSampled :
0

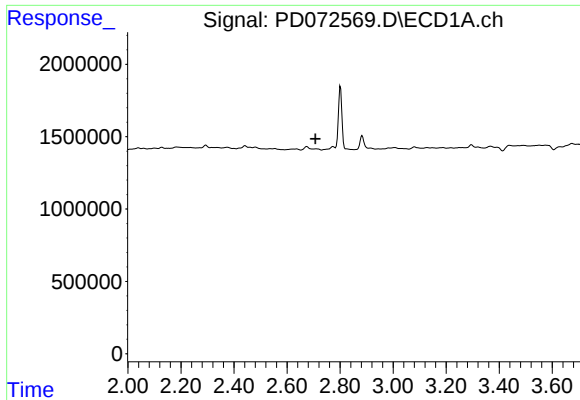

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 2.707 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

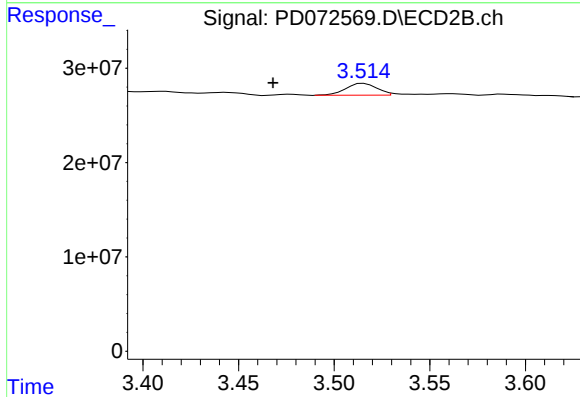


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: 0.047 min
Response: 14200877
Conc: 0.38 ng/ml

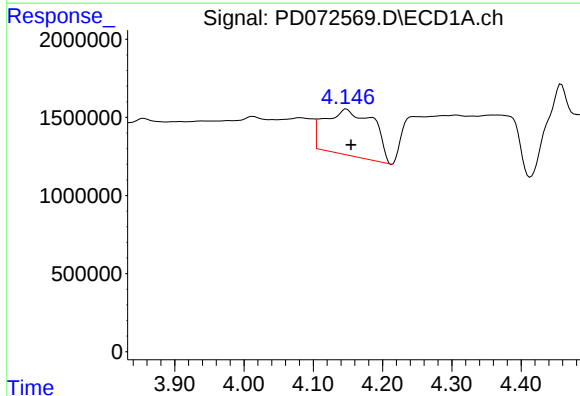


#5 Aldrin

R.T.: 4.148 min
Delta R.T.: -0.007 min
Response: 14432715
Conc: 4.26 ng/ml

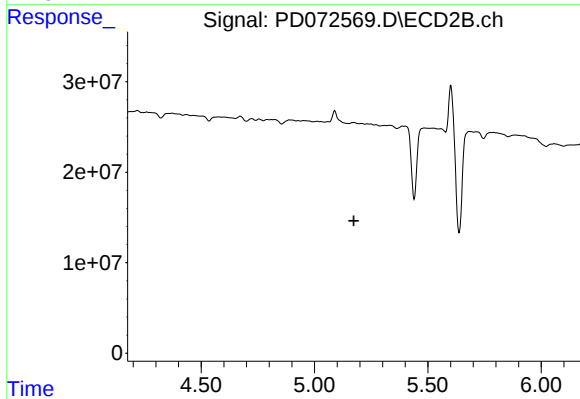

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.173 min
Response: 0
Conc: N.D.

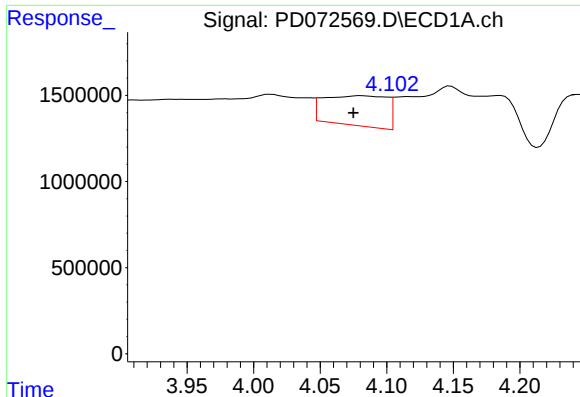

#7 delta-BHC


R.T.: 4.081 min
Delta R.T.: 0.006 min
Response: 5675982
Conc: 1.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

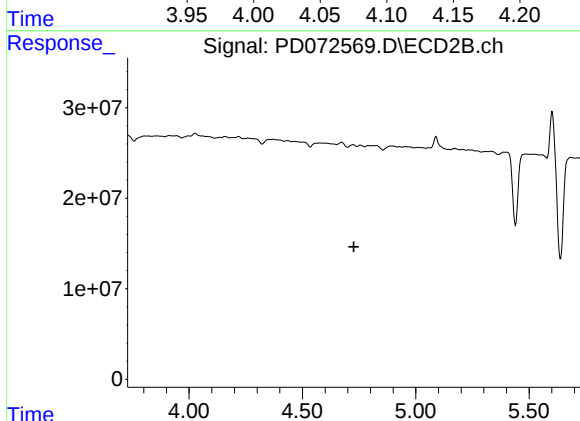


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.727 min
Response: 0
Conc: N.D.

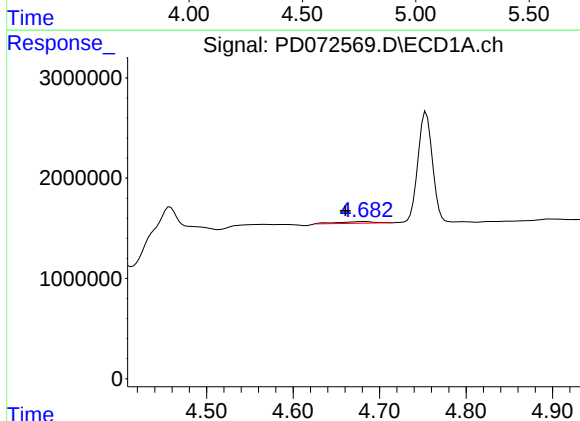


#8 Heptachlor epoxide

R.T.: 4.682 min
Delta R.T.: 0.021 min
Response: 472987
Conc: 0.16 ng/ml

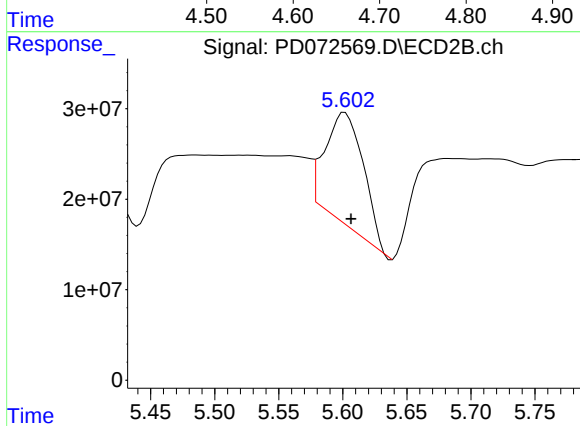

#8 Heptachlor epoxide


R.T.: 5.602 min
Delta R.T.: -0.005 min
Response: 253920786
Conc: 13.05 ng/ml

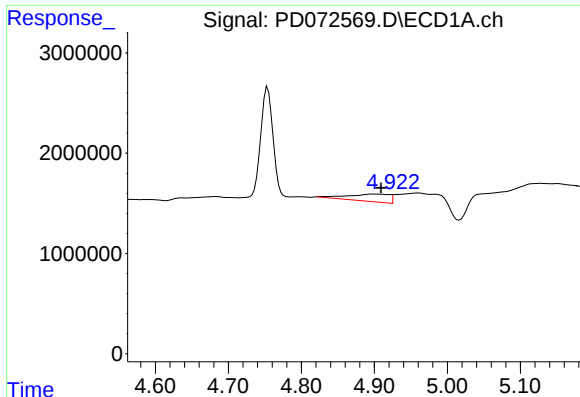

#10 trans-Chlordane


R.T.: 4.901 min
Delta R.T.: -0.009 min
Response: 2890281
Conc: 0.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

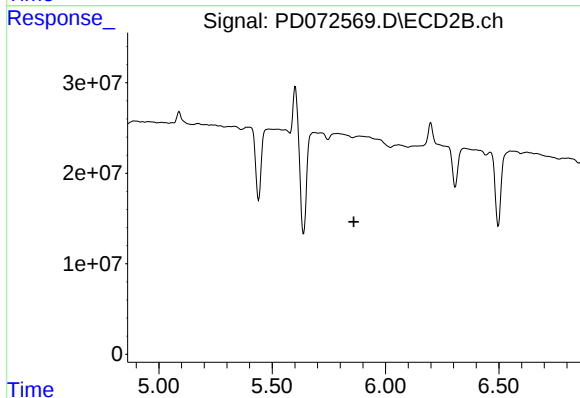


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.860 min
Response: 0
Conc: N.D.

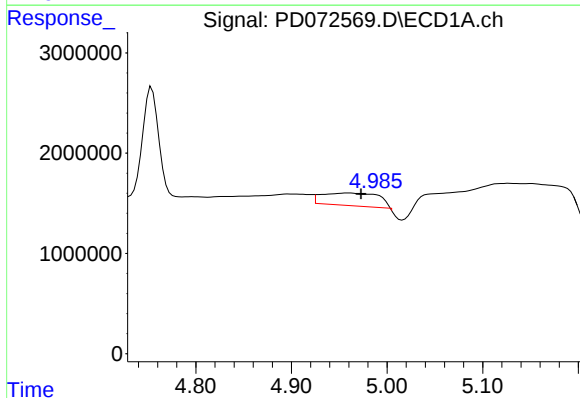


#11 cis-Chlordane

R.T.: 4.959 min
Delta R.T.: -0.014 min
Response: 5103651
Conc: 1.69 ng/ml

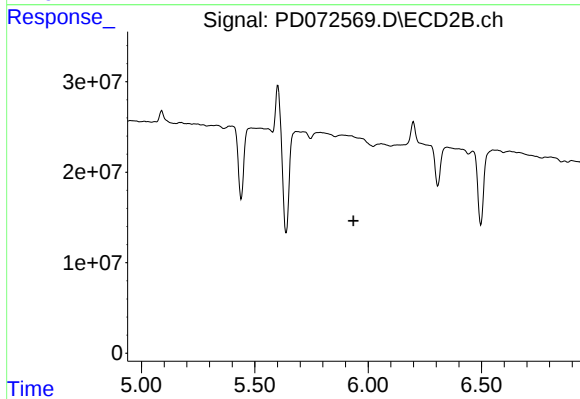

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.936 min
Response: 0
Conc: N.D.

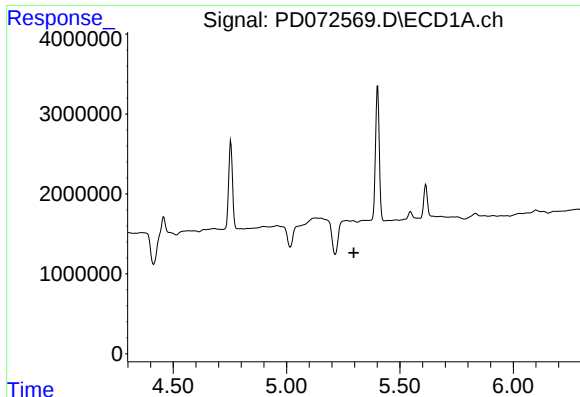

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.297 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

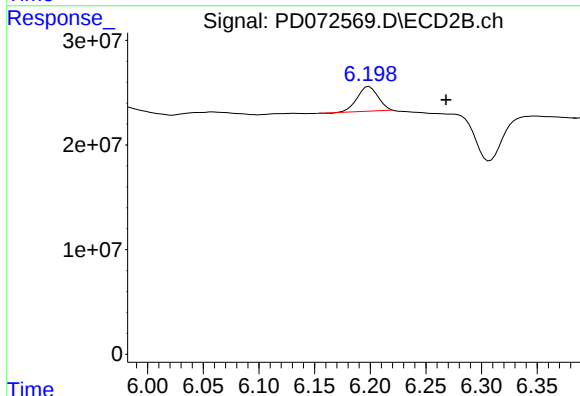


#13 Dieldrin

R.T.: 6.199 min
Delta R.T.: -0.069 min
Response: 30762943
Conc: 1.88 ng/ml

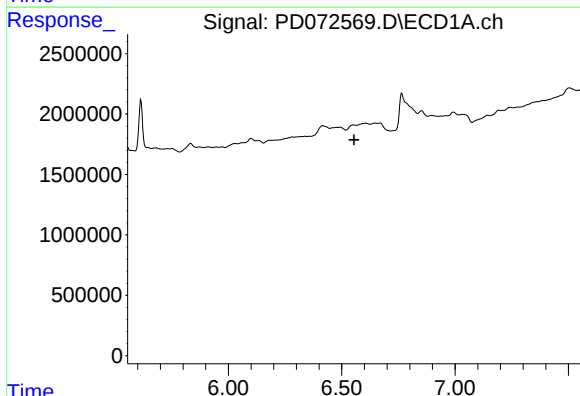


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.555 min
Response: 0
Conc: N.D.

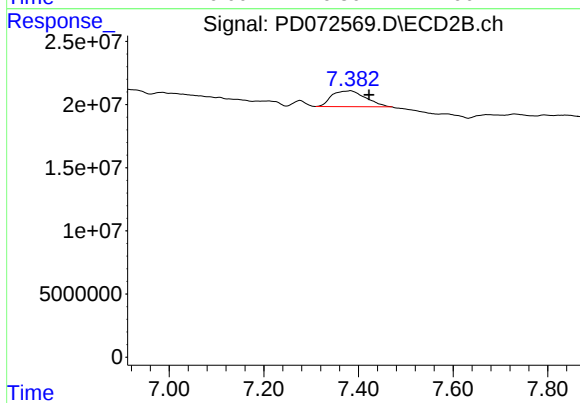

#20 Methoxychlor


R.T.: 7.384 min
Delta R.T.: -0.038 min
Response: 61942086
Conc: 11.28 ng/ml

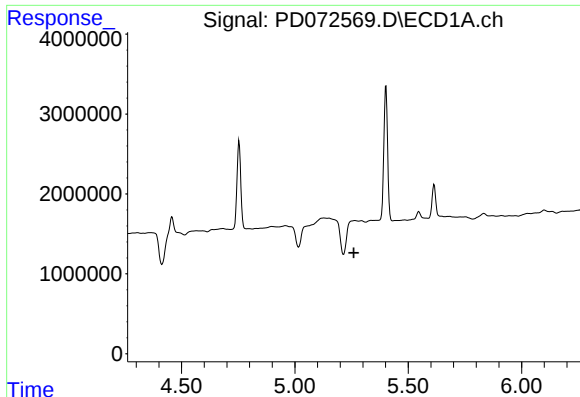

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 5.260 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

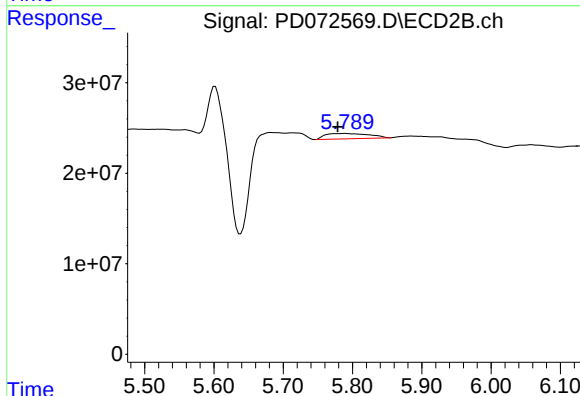


#22 Toxaphene-1

R.T.: 5.790 min
Delta R.T.: 0.011 min
Response: 25726413
Conc: 402.74 ng/ml

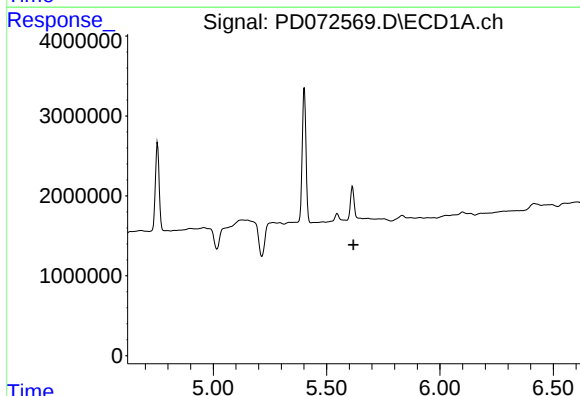


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 5.619 min
Response: 0
Conc: N.D.

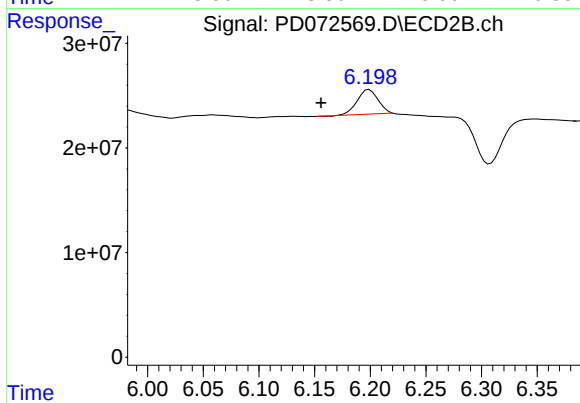

#23 Toxaphene-2


R.T.: 6.199 min
Delta R.T.: 0.043 min
Response: 30762943
Conc: 270.63 ng/ml

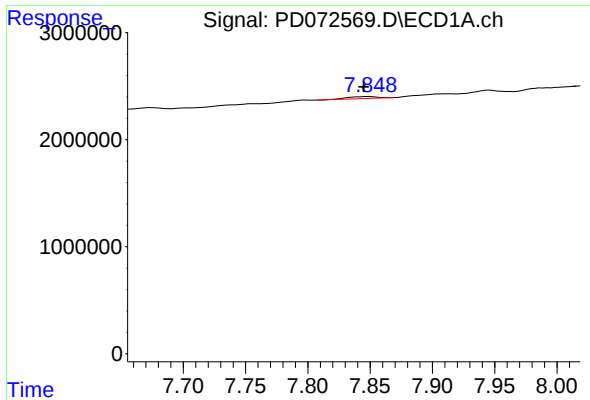

#27 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: 0.003 min
Response: 300304
Conc: 0.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

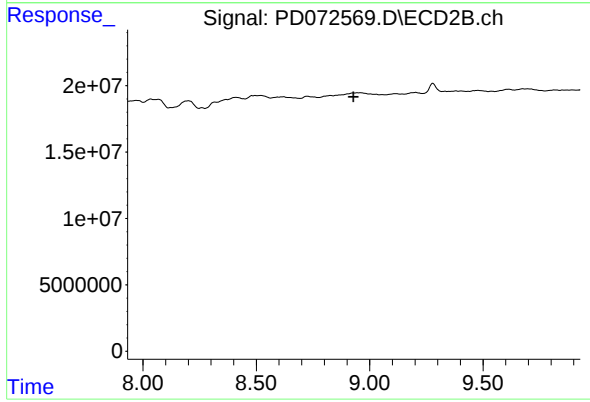

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.