

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102222\
 Data File : PD072572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2022 16:27
 Operator : AR\AJ
 Sample : PB148428BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:53:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 20 01:04:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.707	3.467	53609697	759.9E6	21.025	20.232
27)	SA Decachlor...	7.841	8.923	88165027	380.0E6	44.047	42.213
Target Compounds							
2)	A alpha-BHC	3.193	0.000	116297	0	<MDL	N.D. #
9)	A Endosulfan I	4.992f	0.000	302762	0	0.113	N.D. #
10)	B trans-Chl...	4.889	0.000	195466	0	<MDL	N.D. #
11)	B cis-Chlor...	4.992	0.000	302762	0	0.100	N.D. #
18)	B Endrin al...	6.091f	0.000	146566	0	<MDL	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102222\
Data File : PD072572.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2022 16:27
Operator : AR\AJ
Sample : PB148428BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:53:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 20 01:04:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

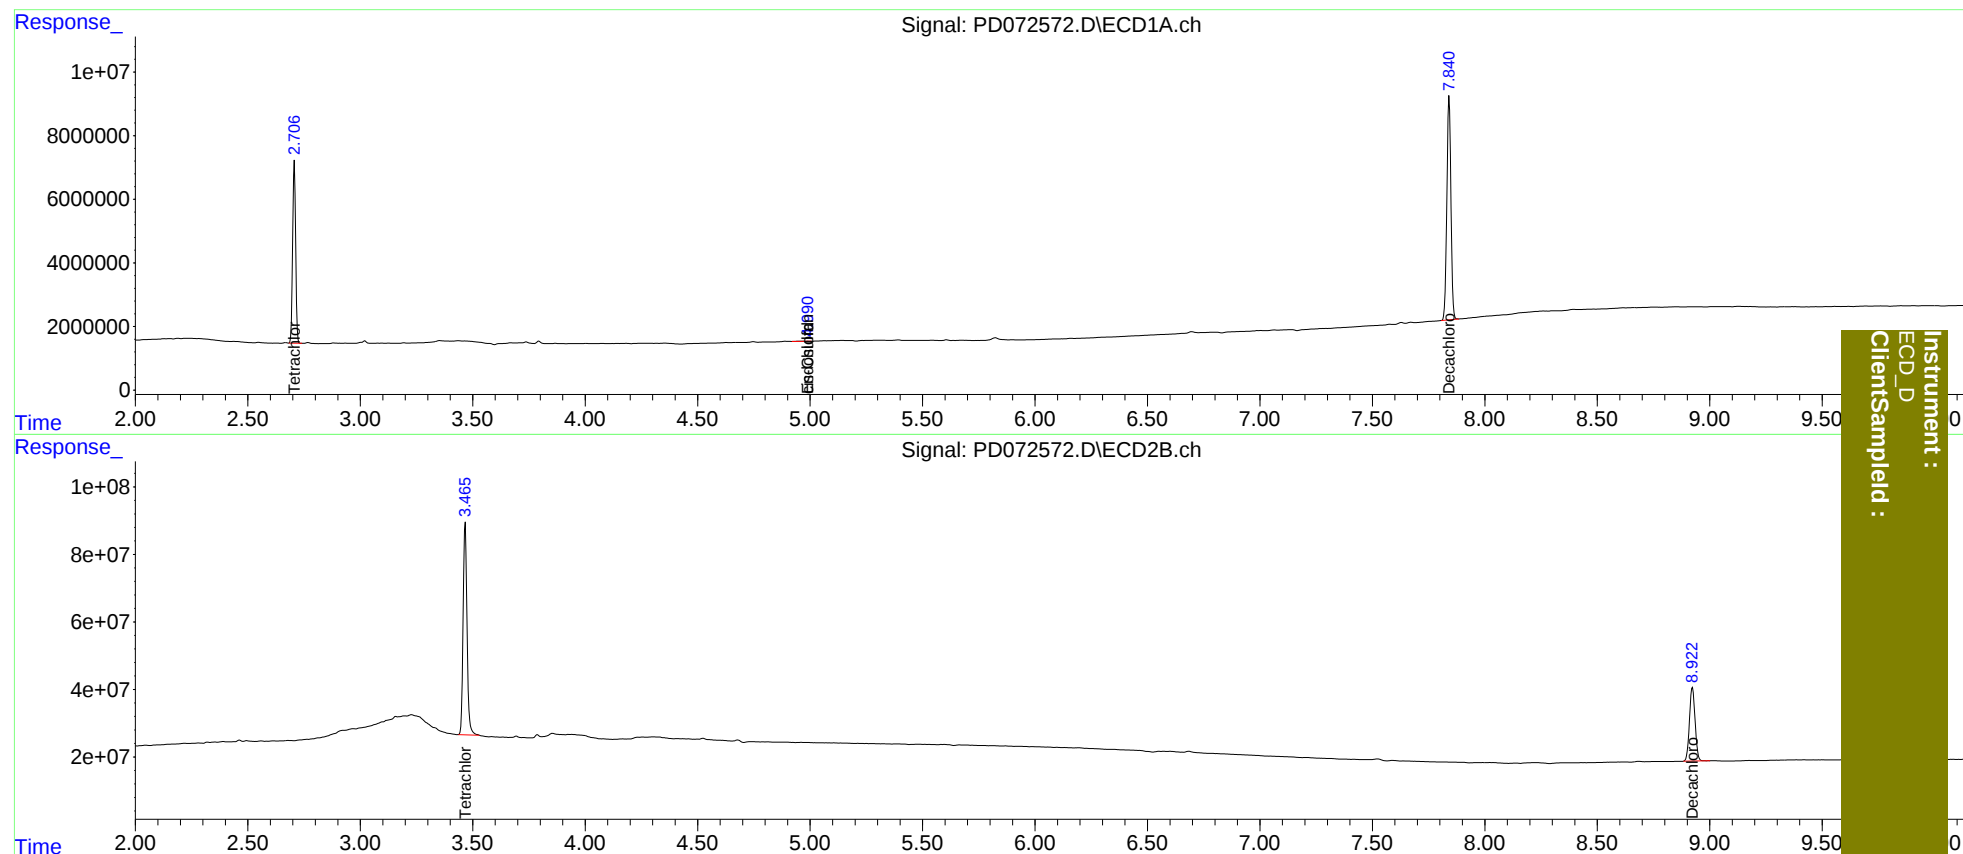


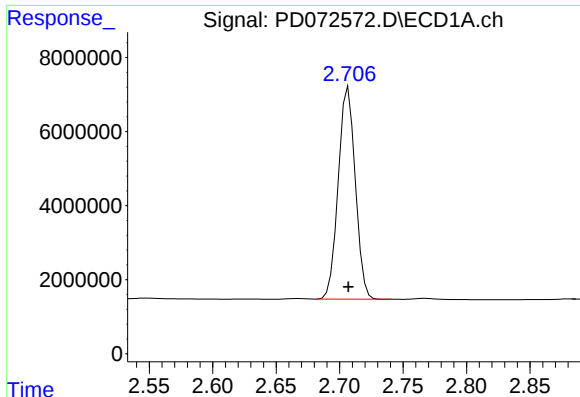

#1 Tetrachloro-m-xylene


R.T.: 2.707 min
Delta R.T.: 0.000 min
Response: 53609697
Conc: 21.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

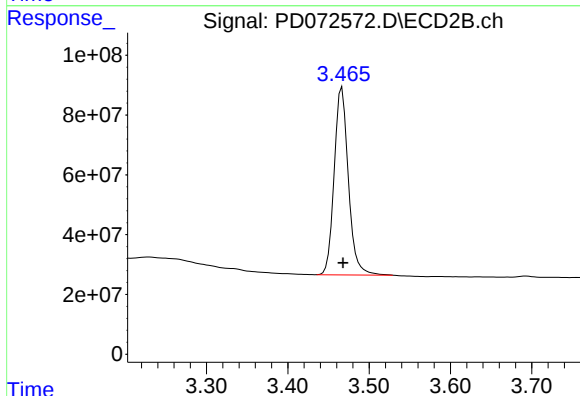


#1 Tetrachloro-m-xylene

R.T.: 3.467 min
Delta R.T.: -0.001 min
Response: 759892674
Conc: 20.23 ng/ml

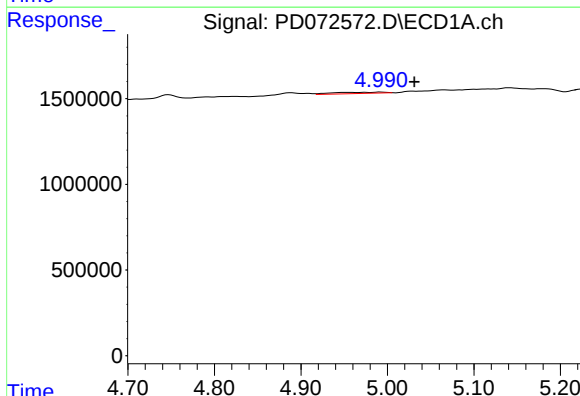


#9 Endosulfan I

R.T.: 4.992 min
Delta R.T.: -0.039 min
Response: 302762
Conc: 0.11 ng/ml

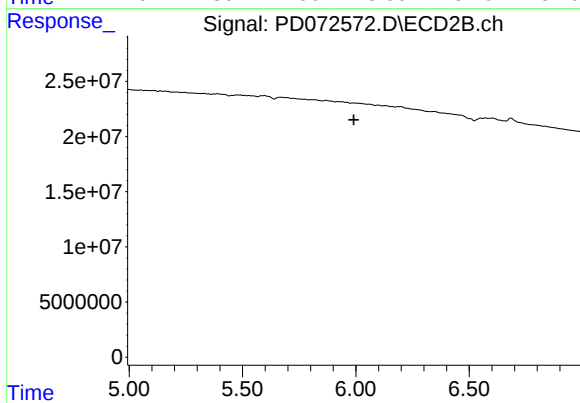

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.991 min
Response: 0
Conc: N.D.

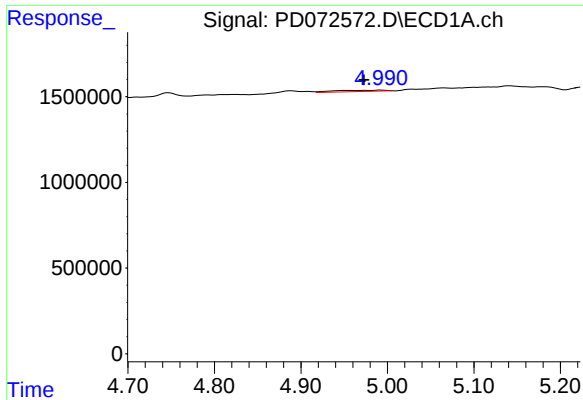

#11 cis-Chlordane


R.T.: 4.992 min
Delta R.T.: 0.019 min
Response: 302762
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

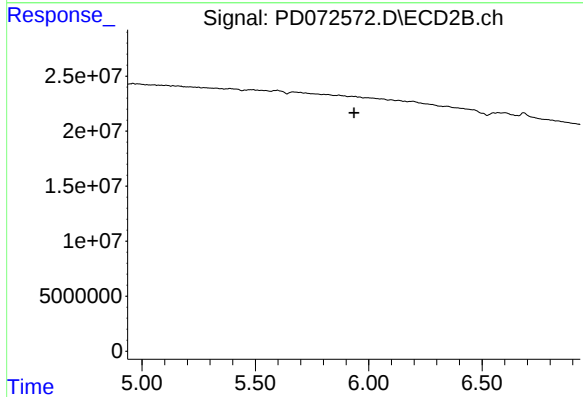


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.936 min
Response: 0
Conc: N.D.

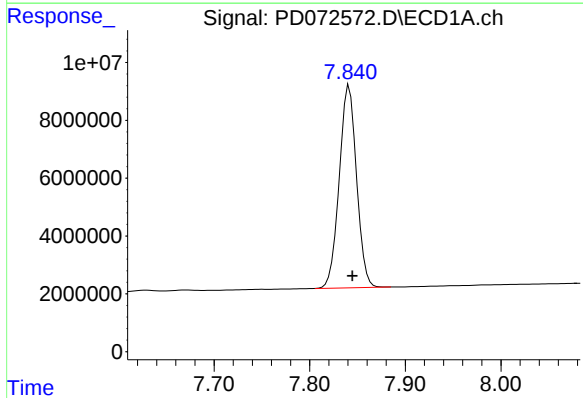

#27 Decachlorobiphenyl

R.T.: 7.841 min
Delta R.T.: -0.003 min
Response: 88165027
Conc: 44.05 ng/ml

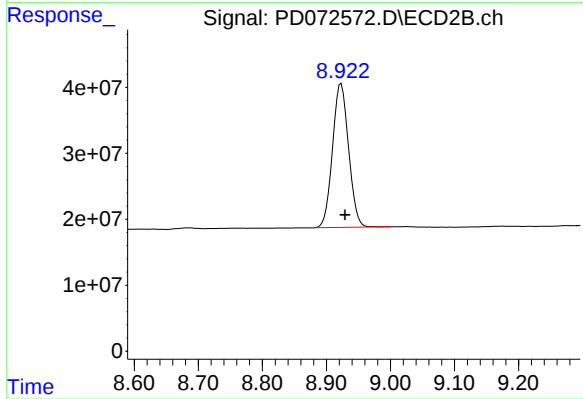

#27 Decachlorobiphenyl

R.T.: 8.923 min
Delta R.T.: -0.006 min
Response: 380011628
Conc: 42.21 ng/ml