

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102222\
 Data File : PD072573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2022 16:40
 Operator : AR\AJ
 Sample : PB148428BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS428

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/24/2022
 Supervised By : Ankita Jodhani 10/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:54:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 20 01:04:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.706	3.467	49930500	682.6E6	19.582	18.174
27)	SA Decachlor...	7.840	8.924	84107047	362.7E6	42.019	40.289
Target Compounds							
2)	A alpha-BHC	3.210	3.931	16929198	239.2E6	4.523	4.860
3)	MA gamma-BHC...	3.541	4.265	16086672	209.9E6	4.886	5.037
4)	MA Heptachlor	3.872	4.832	15997013	146.8E6	4.628m	5.100
5)	MB Aldrin	4.152	5.171	16590071	127.5E6	4.897	5.300
6)	B beta-BHC	3.842	4.480	7675255	78776520	4.801m	4.732
7)	B delta-BHC	4.073	4.724	16106655	159.4E6	4.541	5.004
8)	B Heptachlo...	4.658	5.604	14794510	100.1E6	4.877	5.144
9)	A Endosulfan I	5.028	5.987	13697622	82247005	5.095	5.120m
10)	B trans-Chl...	4.907	5.857	15647706	87073120	5.034	4.654
11)	B cis-Chlor...	4.970	5.933	14735044	85051152	4.879	4.754
12)	B 4,4'-DDE	5.159	6.106	27236244	157.6E6	9.350	9.633
13)	MA Dieldrin	5.294	6.265	28544377	166.8E6	9.746	10.219
14)	MA Endrin	5.571	6.497	23200934	131.3E6	9.062	9.548
15)	B Endosulfa...	5.869	6.727	24197373	129.8E6	10.045	10.173
16)	A 4,4'-DDD	5.718	6.631	22688527	129.0E6	9.987	10.400
17)	MA 4,4'-DDT	5.967	6.939	19757433	114.2E6	8.939	9.492
18)	B Endrin al...	6.052	6.859	21134078	110.0E6	10.256	10.229
19)	B Endosulfa...	6.274	7.091	23333635	113.5E6	9.667	9.509
20)	A Methoxychlor	6.551	7.419	60599470	276.3E6	50.774	50.333
21)	B Endrin ke...	6.785	7.580	29047219	133.7E6	10.193	10.426

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102222\
Data File : PD072573.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2022 16:40
Operator : AR\AJ
Sample : PB148428BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:54:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 20 01:04:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

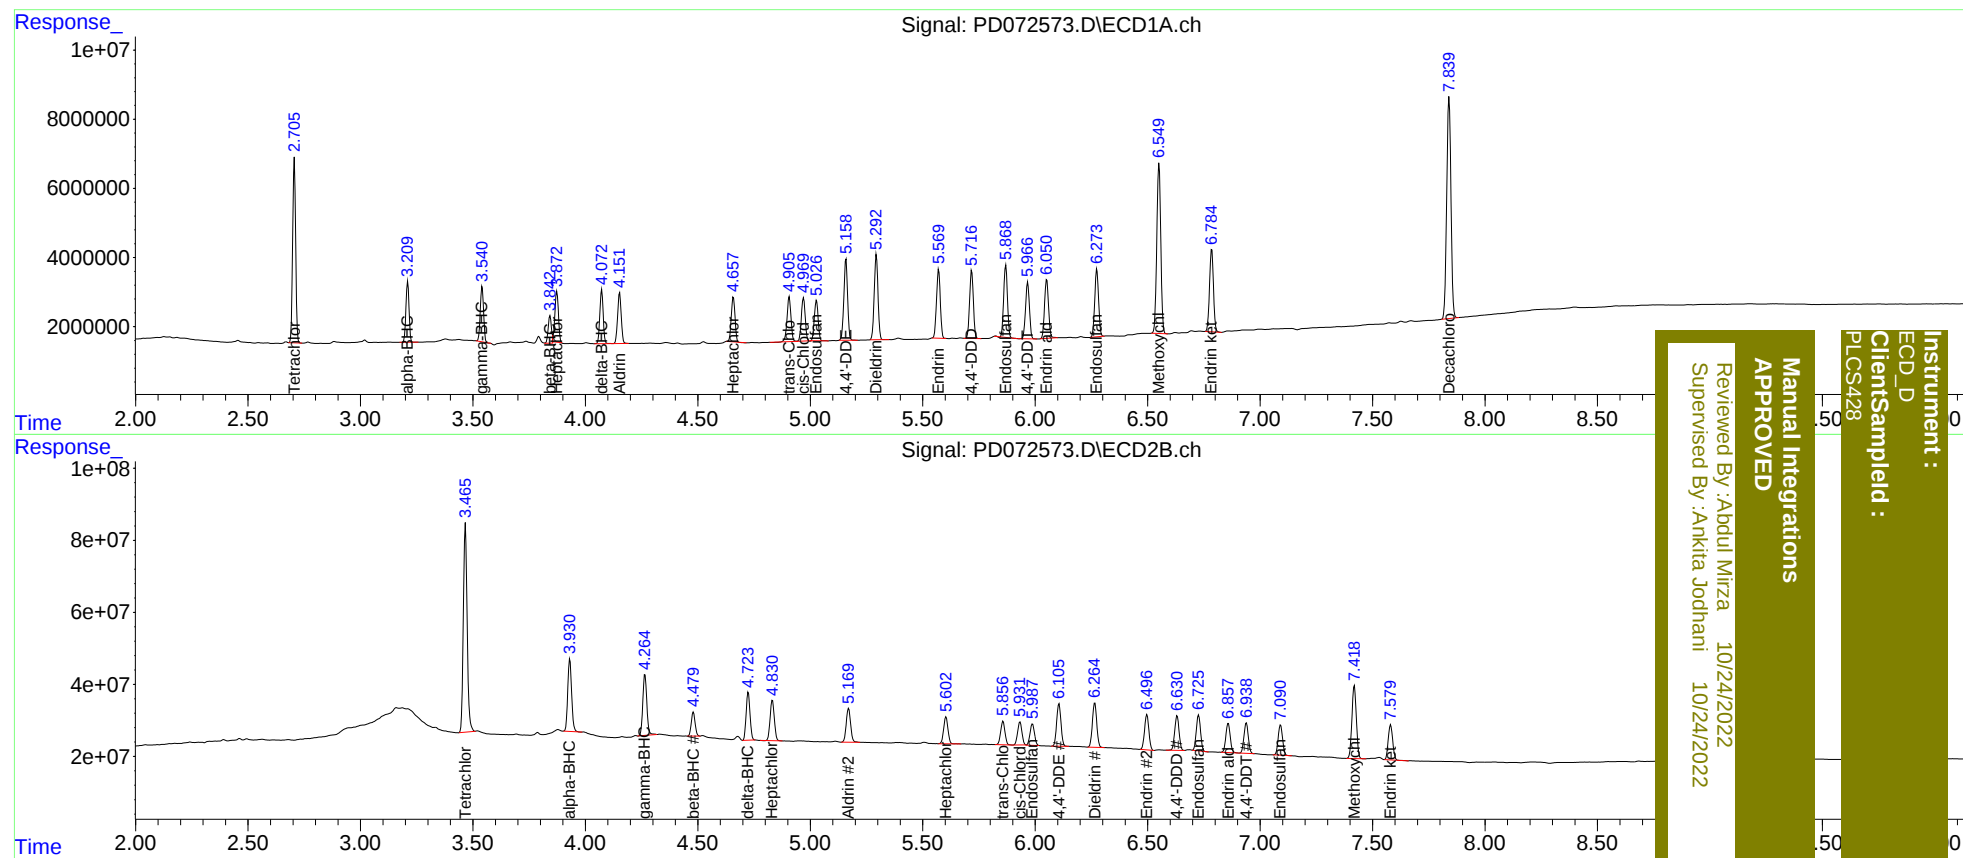

Reviewed By: Abdul Mirza 10/24/2022
Supervised By: Ankita Jodhani 10/24/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
PLCS428