

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102222\
 Data File : PD072576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2022 17:20
 Operator : AR\AJ
 Sample : N5137-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8Z4MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/24/2022
 Supervised By : Ankita Jodhani 10/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:56:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 20 01:04:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.706	3.469	27997368	517.0E6	10.980	13.765 #
27)	SA Decachlor...	7.839	8.923	29443775	182.1E6	14.710	20.229 #
Target Compounds							
2)	A alpha-BHC	3.210	3.932	176.5E6	1862.9E6	47.163	37.851
3)	MA gamma-BHC...	3.541	4.266	171.0E6	1608.5E6	51.933	38.592 #
4)	MA Heptachlor	3.872	4.831	180.0E6	1164.6E6	52.067m	40.450m
5)	MB Aldrin	4.153	5.171	180.5E6	1019.6E6	53.268	42.378
6)	B beta-BHC	3.841	4.481	66794757	685.8E6	41.784m	41.194
7)	B delta-BHC	4.073	4.724	35561785	317.3E6	10.027	9.959
8)	B Heptachlo...	4.658	5.603	151.4E6	834.6E6	49.905	42.894
9)	A Endosulfan I	5.026	5.986	123.6E6	697.8E6	45.963m	43.434m
10)	B trans-Chl...	4.906	5.857	169.2E6	826.0E6	54.431	44.145
11)	B cis-Chlor...	4.970	5.932	158.2E6	763.5E6	52.379	42.675
12)	B 4,4'-DDE	5.159	6.106	321.3E6	1436.8E6	110.301	87.836
13)	MA Dieldrin	5.294	6.265	343.0E6	1485.5E6	117.102	91.013
14)	MA Endrin	5.571	6.496	284.7E6	1238.4E6	111.204	90.060
15)	B Endosulfa...	5.868	6.726	253.9E6	1181.1E6	105.413	92.575
16)	A 4,4'-DDD	5.717	6.631	242.9E6	1158.1E6	106.921	93.385
17)	MA 4,4'-DDT	5.966	6.938	247.6E6	1159.7E6	112.016	96.408
18)	B Endrin al...	6.051	6.857	188.8E6	864.7E6	91.633	80.376
19)	B Endosulfa...	6.274	7.090	185.6E6	832.4E6	76.911	69.720
20)	A Methoxychlor	6.550	7.418	650.7E6	2675.6E6	545.208	487.423
21)	B Endrin ke...	6.784	7.580	285.5E6	1199.7E6	100.186	93.567

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102222\
Data File : PD072576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2022 17:20
Operator : AR\AJ
Sample : N5137-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:56:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 20 01:04:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

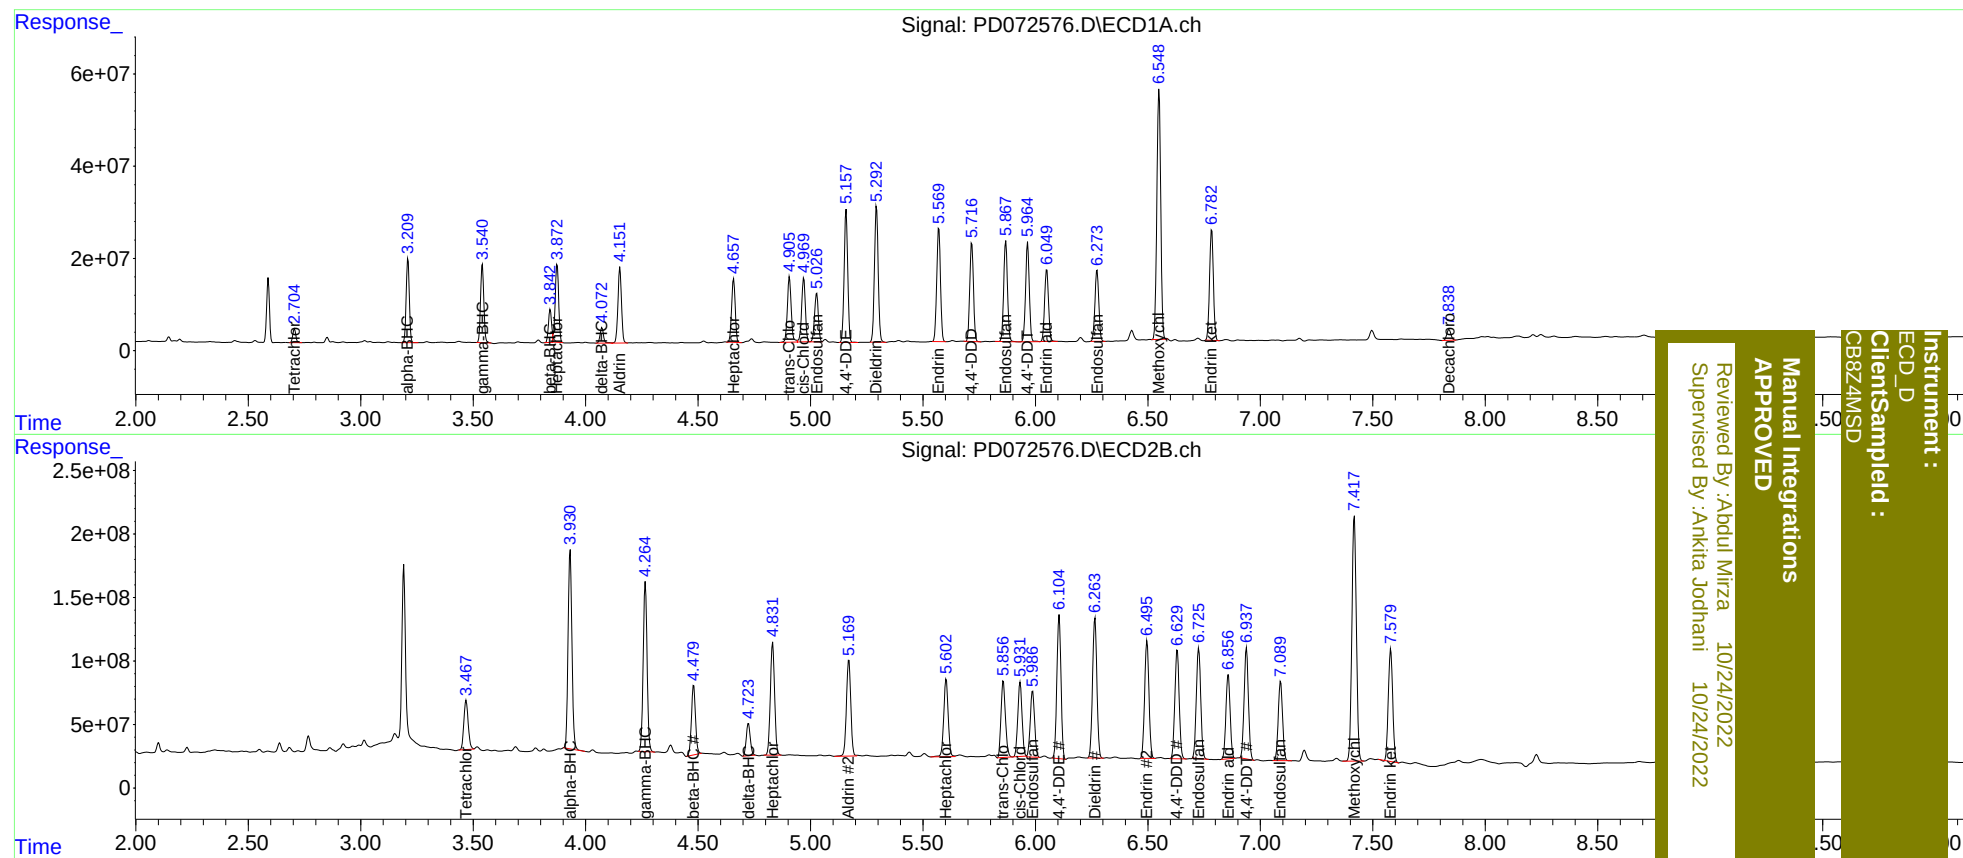

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/24/2022
Supervised By: Ankita Jodhani 10/24/2022

Instrument :
ECD_D
Client Sampled :
CB8Z4MSD