

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102222\
 Data File : PD072575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2022 17:07
 Operator : AR\AJ
 Sample : N5137-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8Z4MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/24/2022
 Supervised By : Ankita Jodhani 10/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:55:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 20 01:04:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.706	3.469	28390258	544.9E6	11.134	14.508 #
27)	SA Decachlor...	7.839	8.923	29254775	182.4E6	14.615	20.261 #
Target Compounds							
2)	A alpha-BHC	3.210	3.931	178.8E6	1908.9E6	47.761	38.785
3)	MA gamma-BHC...	3.541	4.265	172.1E6	1646.3E6	52.271	39.499
4)	MA Heptachlor	3.872	4.830	179.3E6	1184.6E6	51.881m	41.144m
5)	MB Aldrin	4.153	5.170	182.1E6	1041.0E6	53.744	43.266
6)	B beta-BHC	3.841	4.480	73410701	700.3E6	45.922m	42.066
7)	B delta-BHC	4.073	4.724	34642193	323.0E6	9.768	10.139
8)	B Heptachlo...	4.658	5.603	153.2E6	846.4E6	50.490	43.503
9)	A Endosulfan I	5.028	5.986	119.2E6	721.5E6	44.347	44.910m
10)	B trans-Chl...	4.907	5.857	170.1E6	843.5E6	54.714	45.078
11)	B cis-Chlor...	4.970	5.932	159.6E6	777.1E6	52.844	43.434
12)	B 4,4'-DDE	5.159	6.106	323.6E6	1458.8E6	111.082	89.179
13)	MA Dieldrin	5.294	6.265	344.3E6	1506.3E6	117.548	92.285
14)	MA Endrin	5.570	6.496	286.2E6	1252.4E6	111.805	91.077
15)	B Endosulfa...	5.869	6.726	254.8E6	1192.3E6	105.794	93.459
16)	A 4,4'-DDD	5.718	6.630	244.3E6	1168.8E6	107.544	94.240
17)	MA 4,4'-DDT	5.967	6.938	248.6E6	1171.8E6	112.479	97.417
18)	B Endrin al...	6.051	6.857	190.4E6	874.7E6	92.399	81.307
19)	B Endosulfa...	6.274	7.090	187.0E6	837.9E6	77.463	70.179
20)	A Methoxychlor	6.549	7.418	655.5E6	2690.3E6	549.211	490.087
21)	B Endrin ke...	6.784	7.580	288.0E6	1231.6E6	101.055	96.055

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102222\
Data File : PD072575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2022 17:07
Operator : AR\AJ
Sample : N5137-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:55:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 20 01:04:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

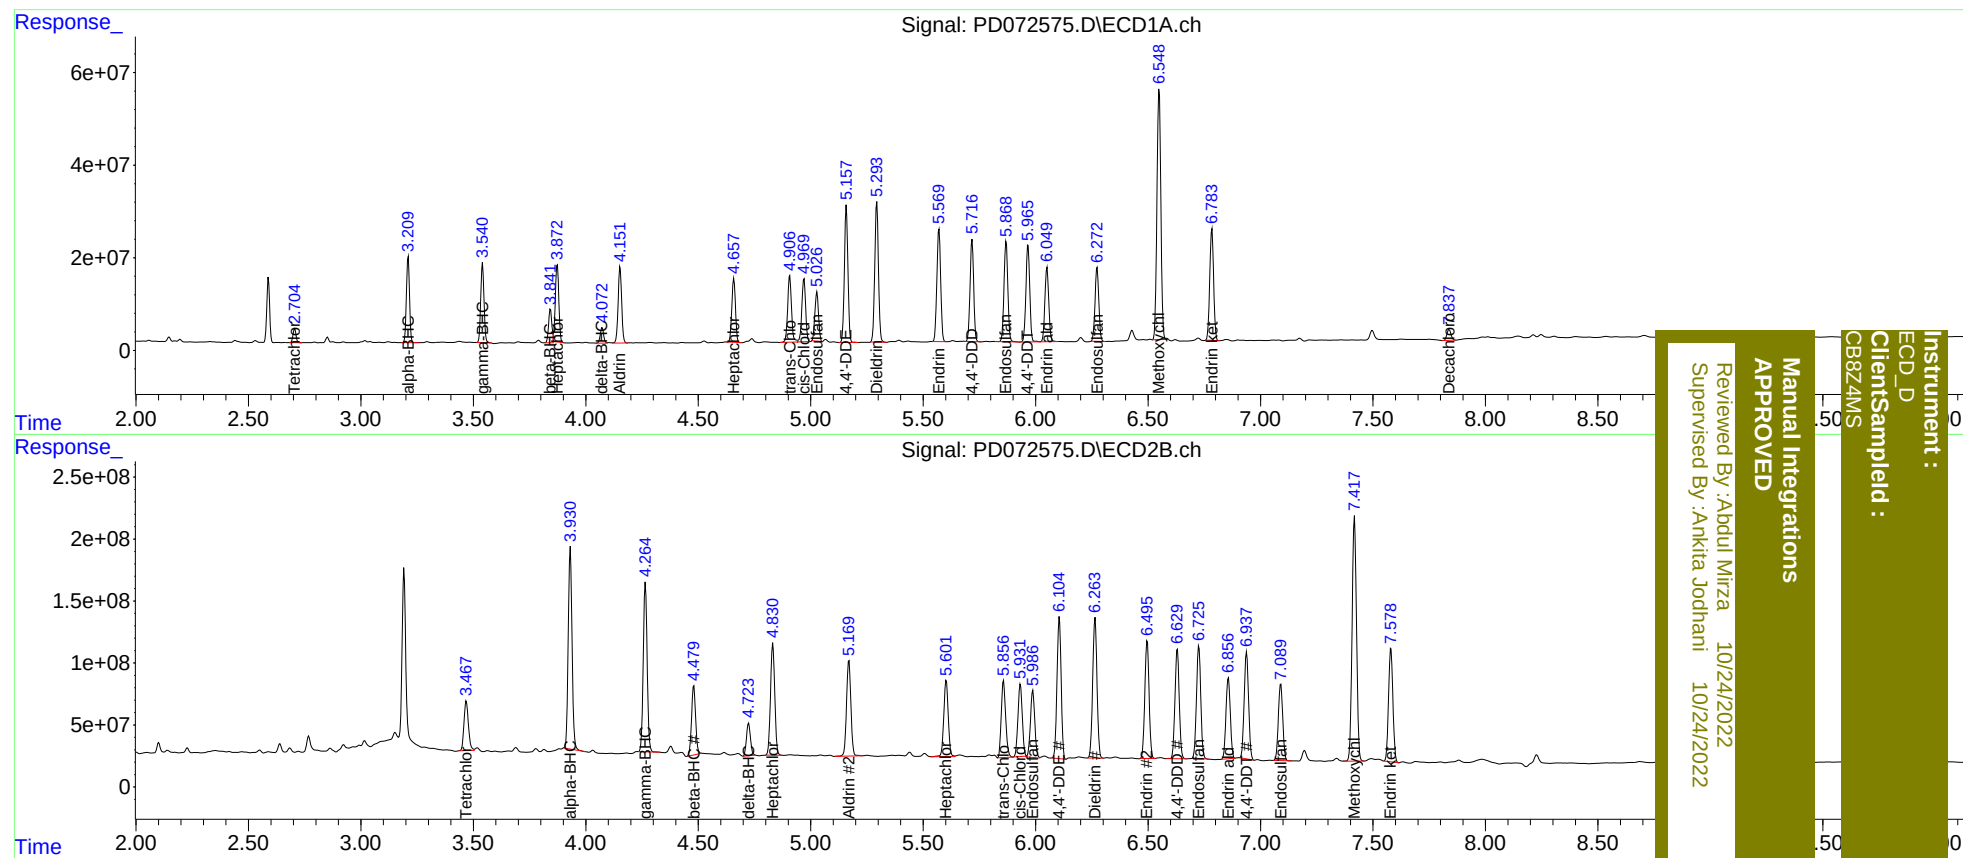

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/24/2022
Supervised By: Ankita Jodhani 10/24/2022

Instrument :
ECD_D
Client Sampled :
CB8Z4MS