

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102318\
 Data File : PD050019.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Oct 2018 20:49
 Operator : AJ\SJ
 Sample : J5604-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MS-VB-25868-BOX-1

Manual Integrations
 APPROVED

Sohil
 10/24/2018 2:07:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 04:13:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101818.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 19 07:43:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.232	4.059	11631053	548.2E6	19.401	21.360m
28)	SA Decachlor...	9.012	9.171	6926545	185.9E6	11.245	11.763

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102318\
Data File : PD050019.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Oct 2018 20:49
Operator : AJ\SJ
Sample : J5604-04
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MS-VB-25868-BOX-1


Manual Integrations
APPROVED

Sohil
10/24/2018 2:07:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 04:13:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101818.M
Quant Title : GC Extractables
QLast Update : Fri Oct 19 07:43:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

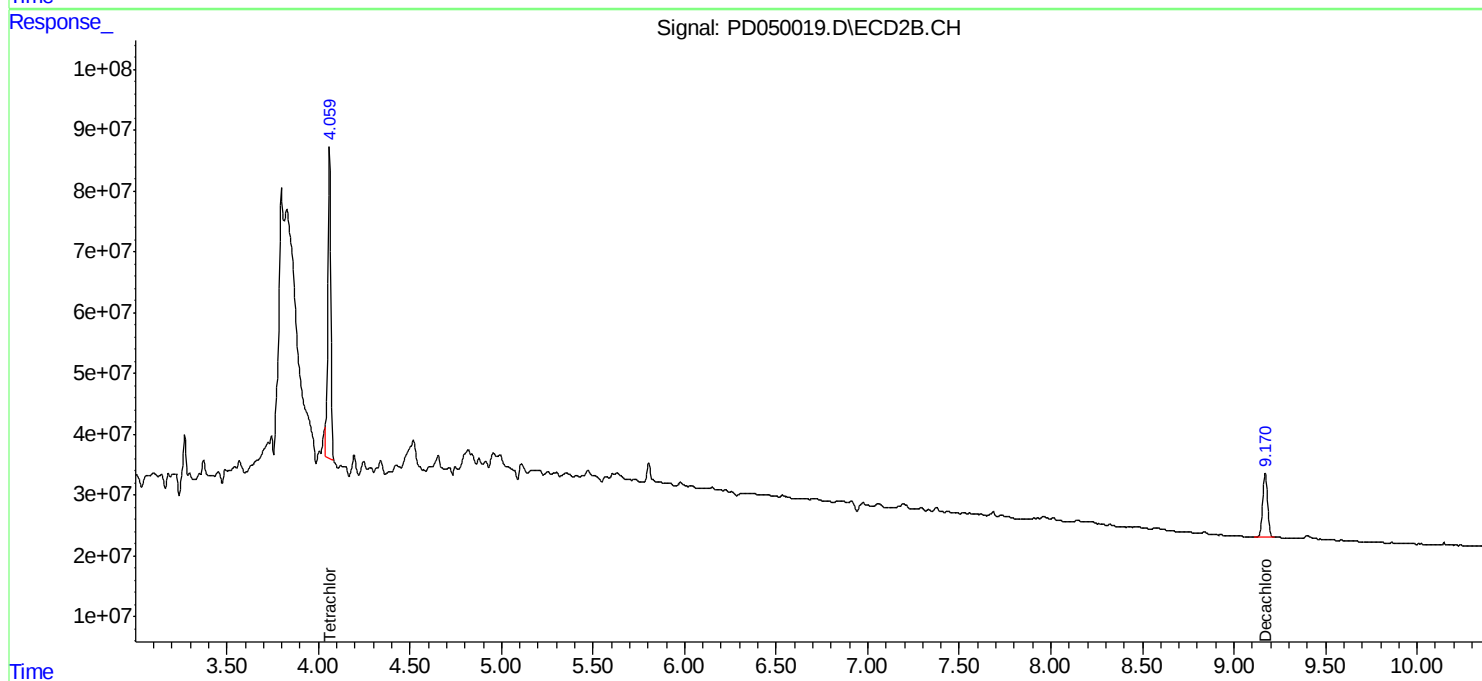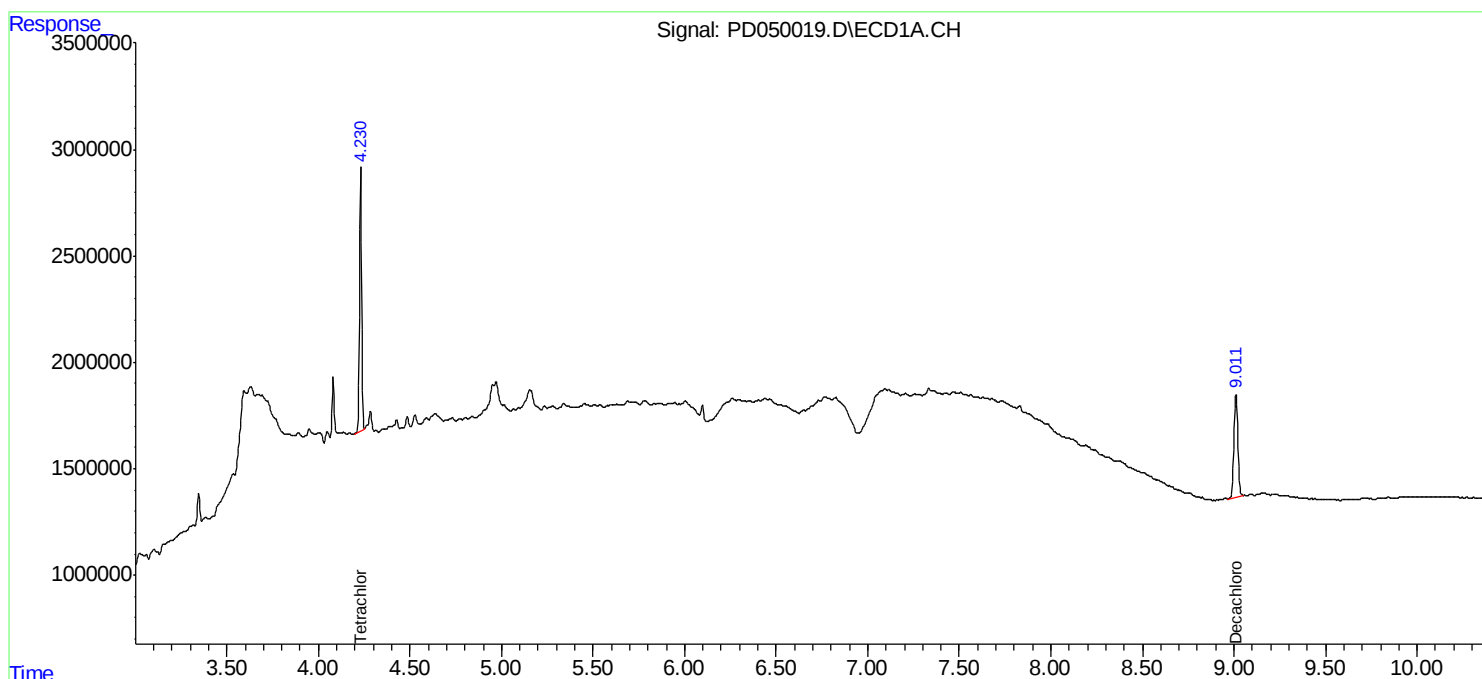

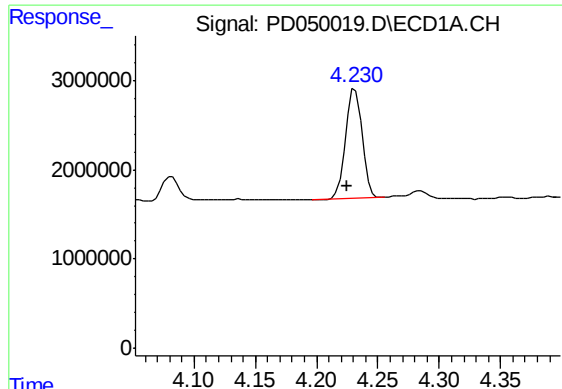


#1 Tetrachloro-m-xylene

R.T.: 4.232 min
Delta R.T.: 0.007 min
Response: 11631053
Conc: 19.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
MS-VB-25868-BOX-1


Manual Integrations
APPROVED

Sohil
10/24/2018 2:07:41 PM

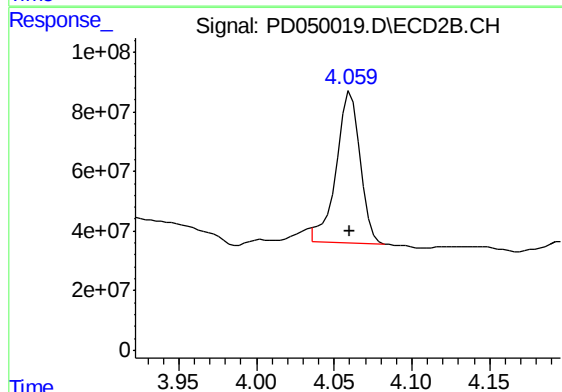


#1 Tetrachloro-m-xylene

R.T.: 4.059 min
Delta R.T.: 0.000 min
Response: 548165137
Conc: 21.36 ng/ml m

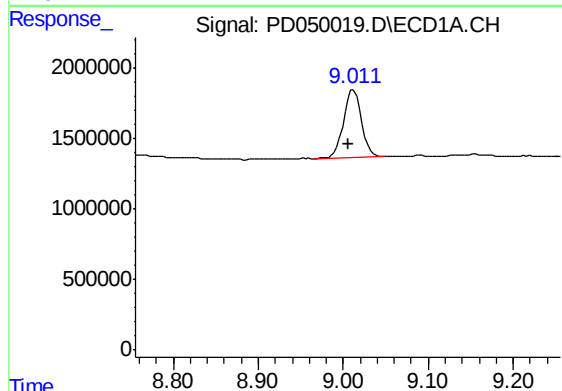

#28 Decachlorobiphenyl

R.T.: 9.012 min
Delta R.T.: 0.006 min
Response: 6926545
Conc: 11.24 ng/ml

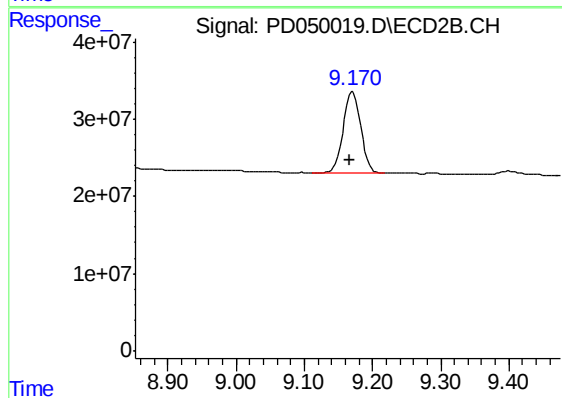

#28 Decachlorobiphenyl

R.T.: 9.171 min
Delta R.T.: 0.004 min
Response: 185874645
Conc: 11.76 ng/ml