

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102318\
 Data File : PD050023.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Oct 2018 21:45
 Operator : AJ\SJ
 Sample : J5604-08
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MS-VB-25868-BOX-1

Manual Integrations
 APPROVED

Sohil
 10/24/2018 2:07:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 04:14:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101818.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 19 07:43:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.232	4.049	3259194	123.4E6	5.436	4.810m
28)	SA Decachlor...	9.010	9.170	2419041	51833042	3.927m	3.280m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102318\
Data File : PD050023.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Oct 2018 21:45
Operator : AJ\SJ
Sample : J5604-08
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MS-VB-25868-BOX-1


Manual Integrations
APPROVED

Sohil
10/24/2018 2:07:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 04:14:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101818.M
Quant Title : GC Extractables
QLast Update : Fri Oct 19 07:43:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

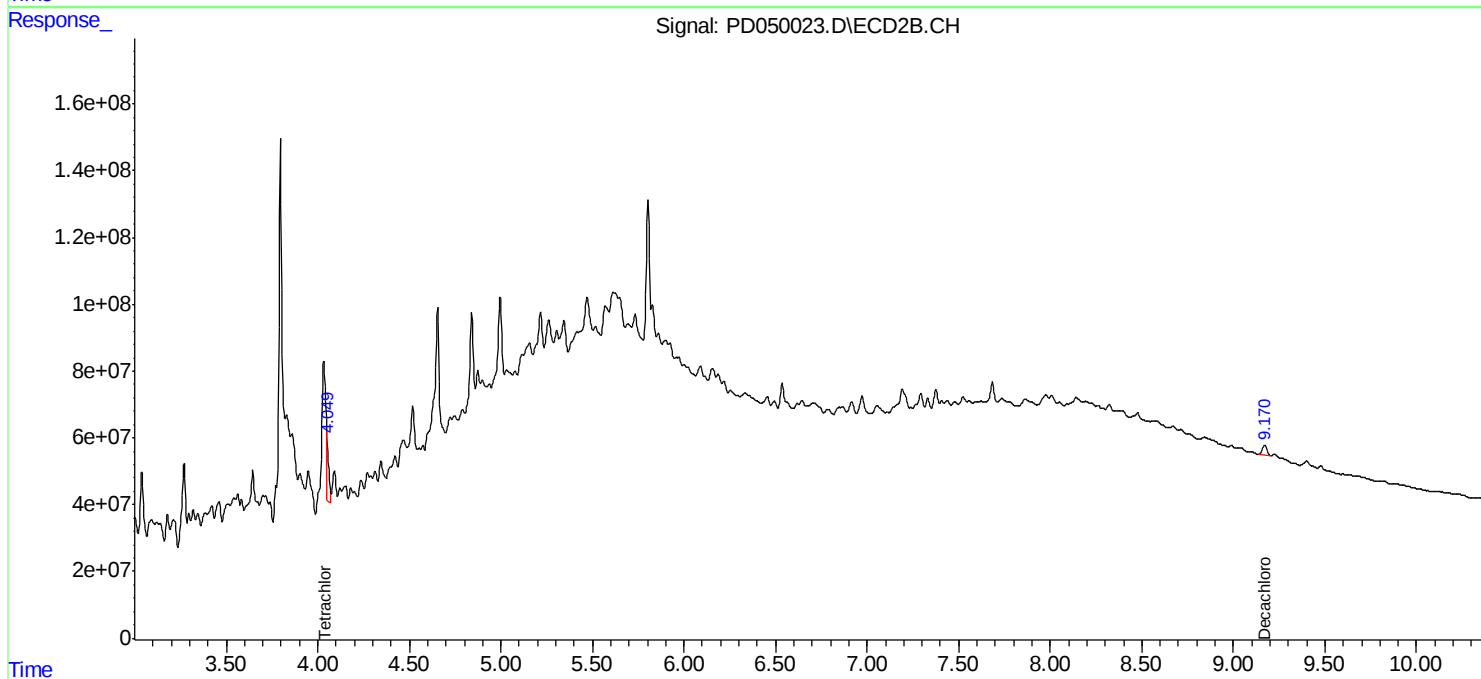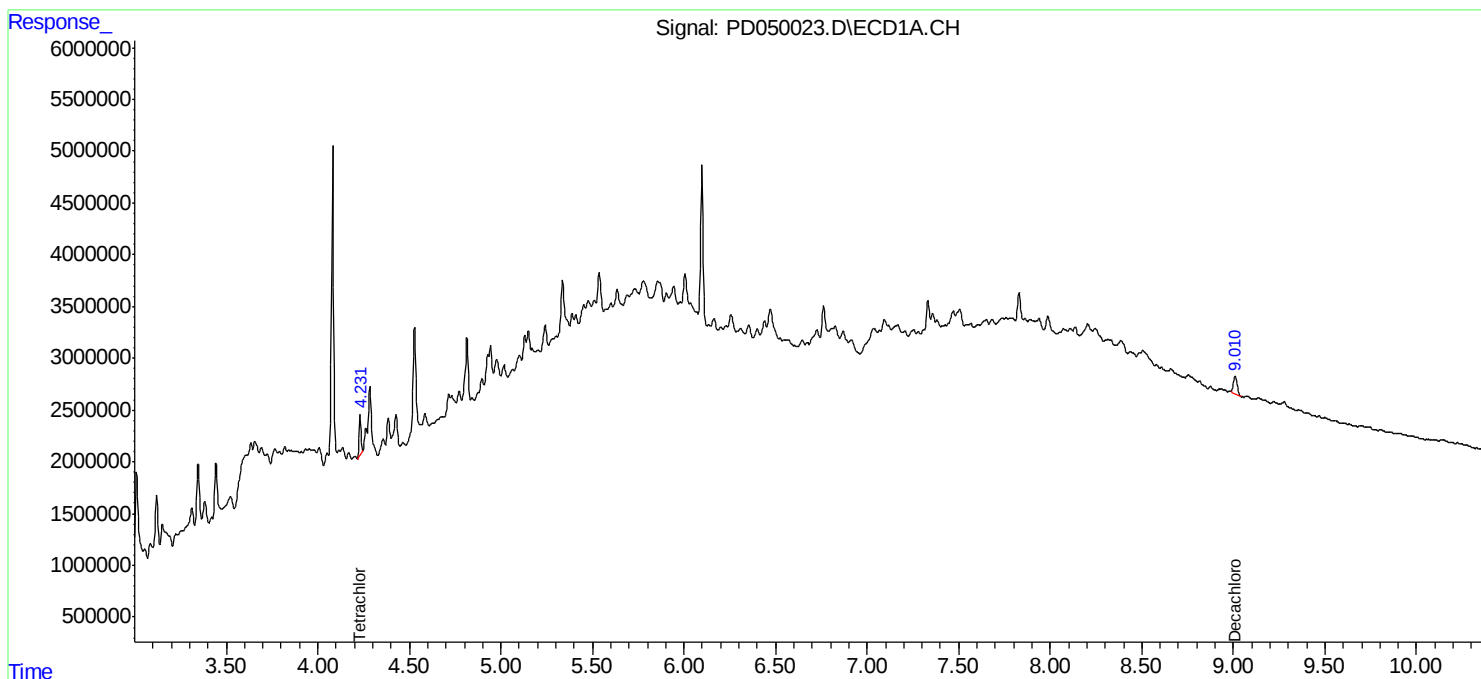

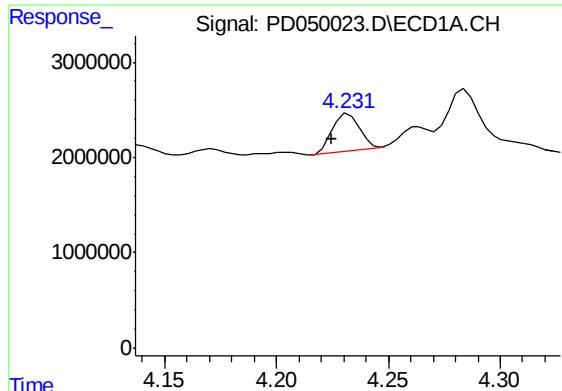


#1 Tetrachloro-m-xylene

R.T.: 4.232 min
Delta R.T.: 0.007 min
Response: 3259194
Conc: 5.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
MS-VB-25868-BOX-1


Manual Integrations
APPROVED

Sohil
10/24/2018 2:07:46 PM

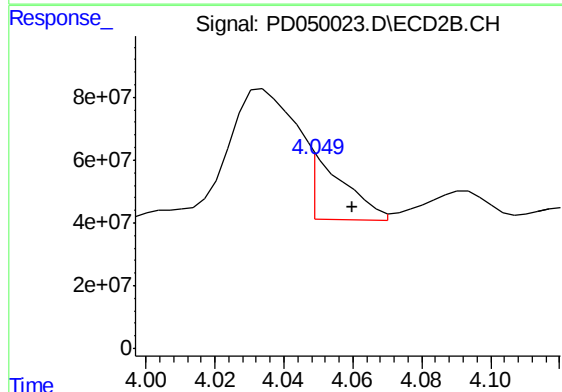


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.011 min
Response: 123449522
Conc: 4.81 ng/ml m

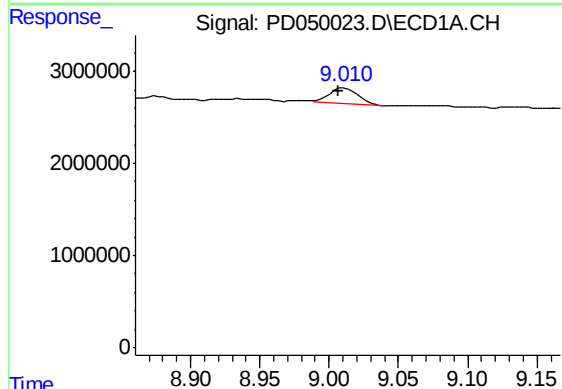

#28 Decachlorobiphenyl

R.T.: 9.010 min
Delta R.T.: 0.004 min
Response: 2419041
Conc: 3.93 ng/ml m

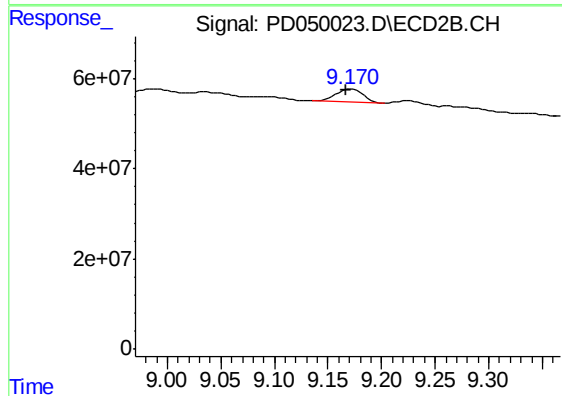

#28 Decachlorobiphenyl

R.T.: 9.170 min
Delta R.T.: 0.003 min
Response: 51833042
Conc: 3.28 ng/ml m